
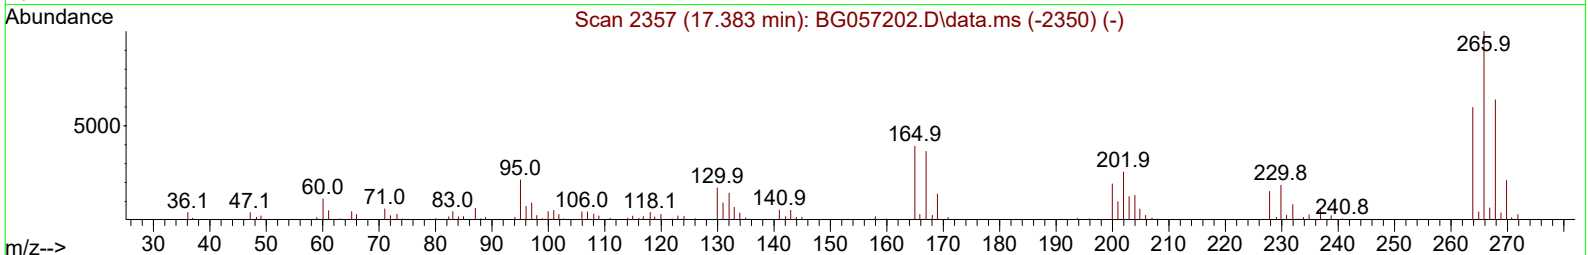
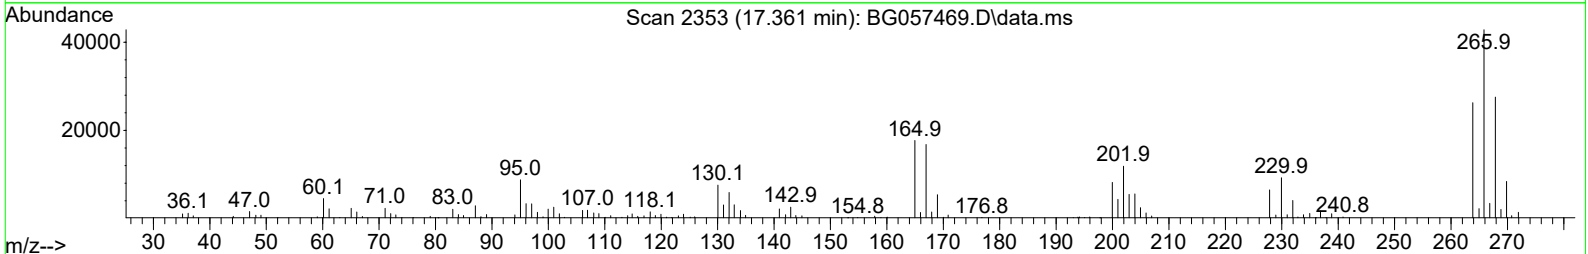


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051923\
 Data File : BG057469.D
 Acq On : 19 May 2023 16:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 05:08:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 20 04:19:55 2023
 Response via : Initial Calibration

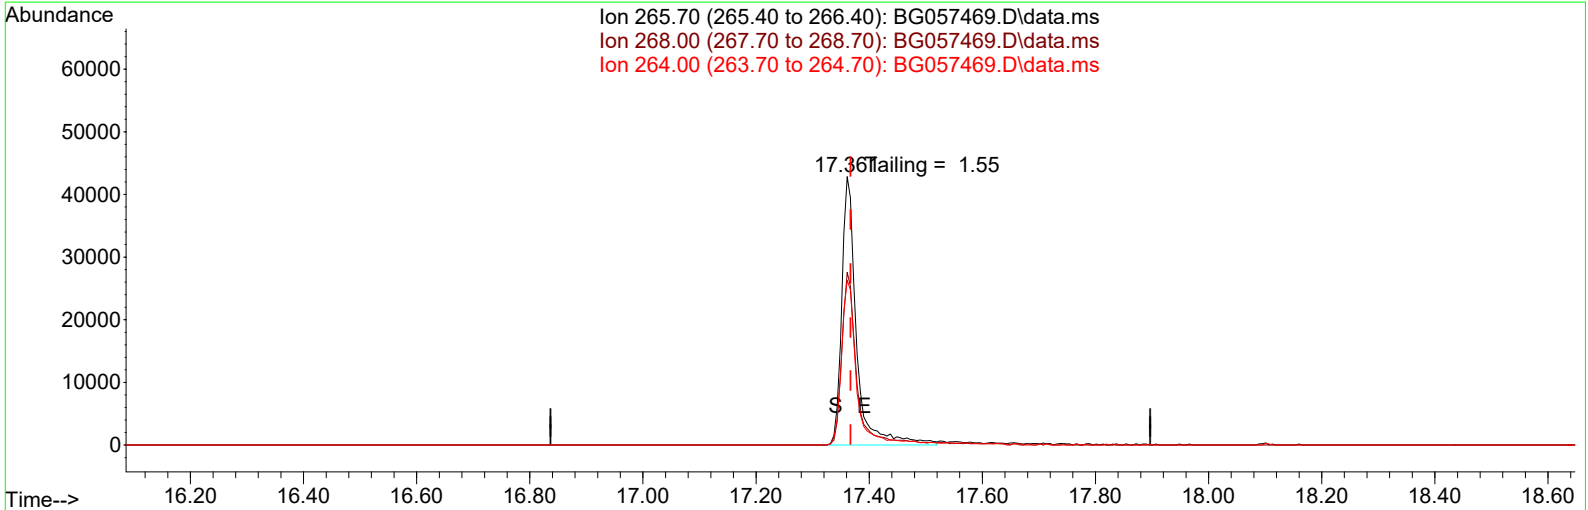

TIC: BG057469.D\data.ms

(70) Pentachlorophenol (C)




17.361min (-0.006) 34475.20 ng

response 78488

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.34
264.00	59.70	61.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051923\
 Data File : BG057469.D
 Acq On : 19 May 2023 16:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 05:08:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 20 04:19:55 2023
 Response via : Initial Calibration

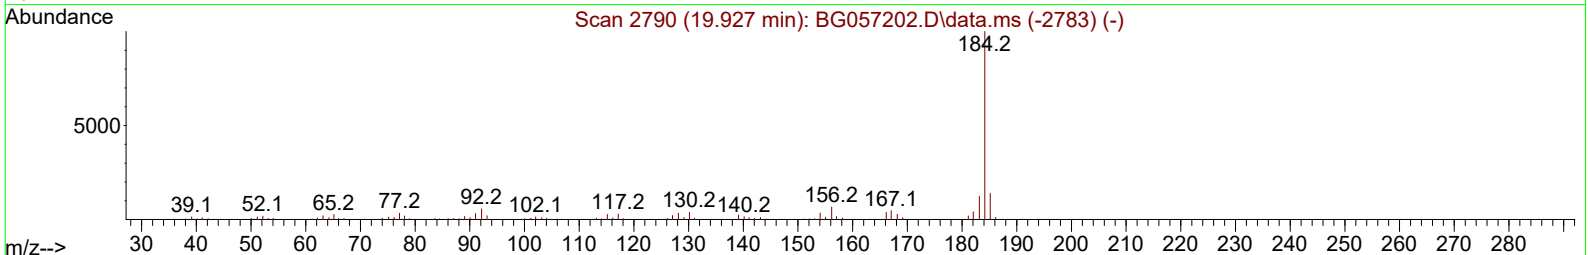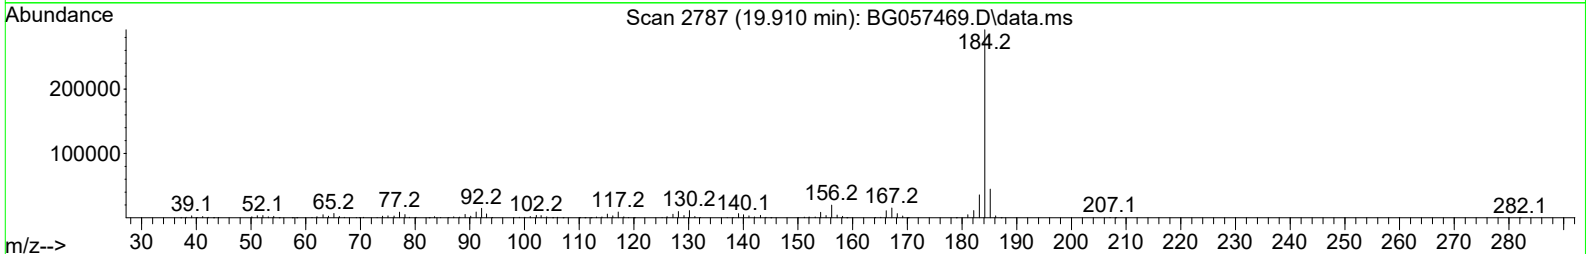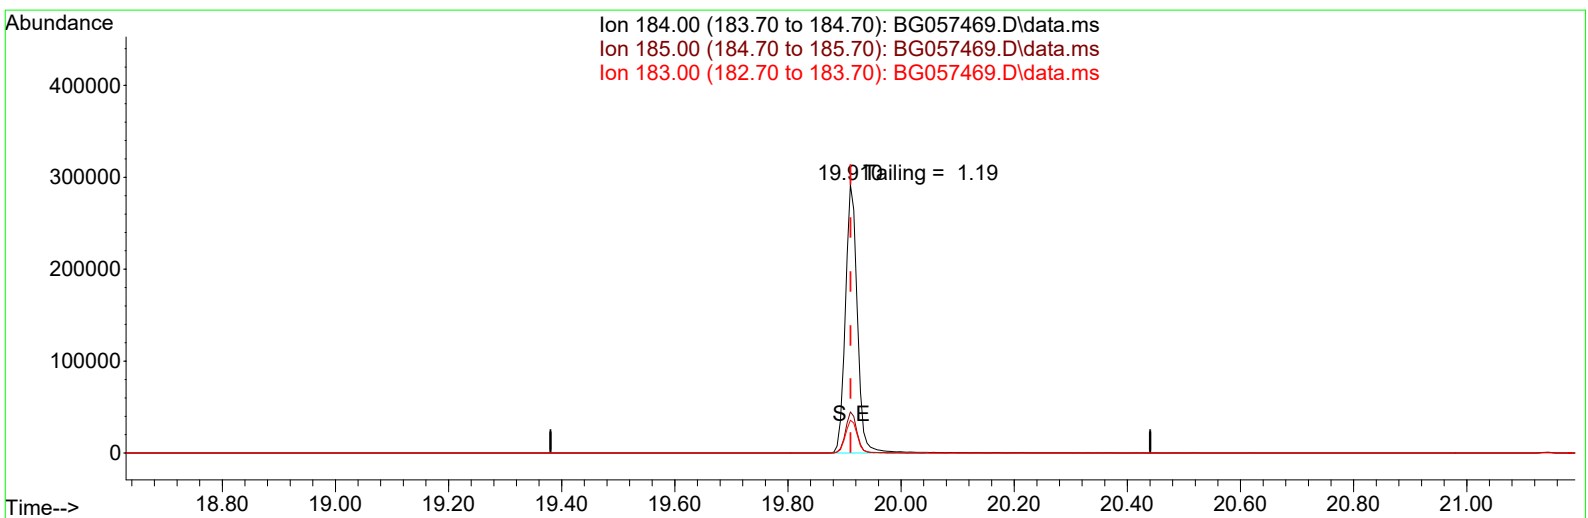

TIC: BG057469.D\data.ms

(77) Benzidine

19.910min (-0.000) 0.00 ng

response 430711

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	15.32
183.00	12.40	12.25
0.00	0.00	0.00