
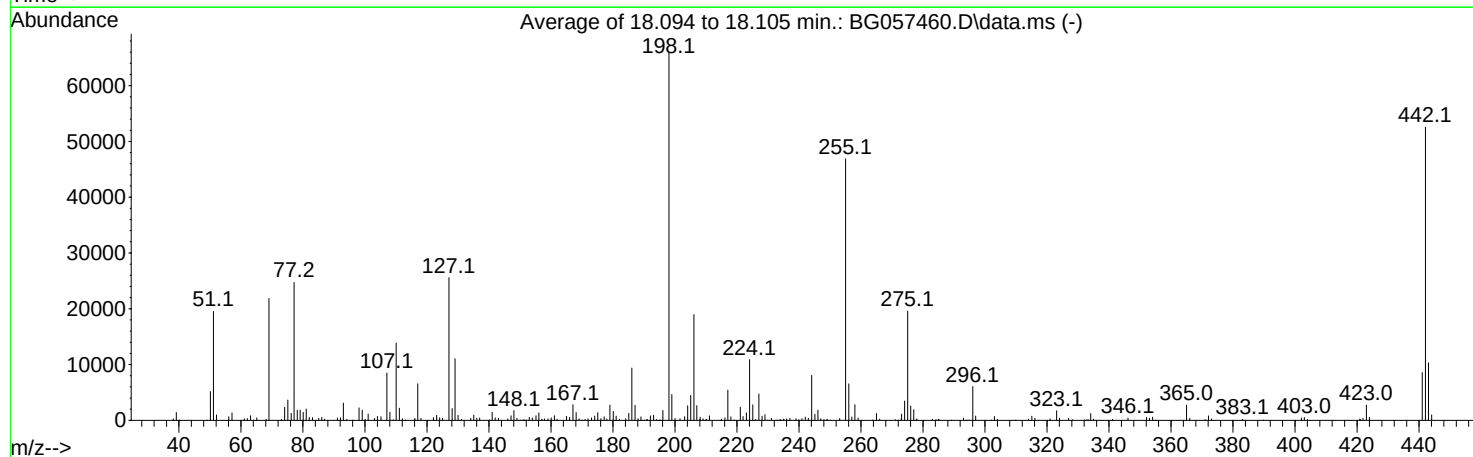


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051923\
Data File : BG057460.D
Acq On : 19 May 2023 9:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat May 20 04:19:55 2023

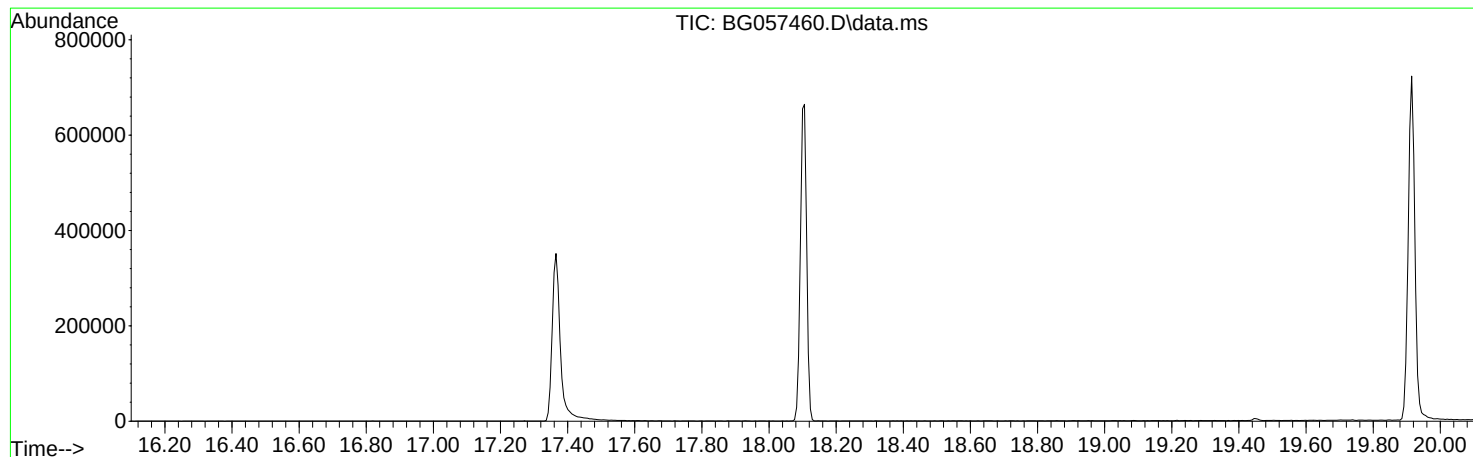

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	19535	PASS
68	69	0.00	2	0.8	179	PASS
69	198	0.00	100	33.2	21864	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.8	25576	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65933	PASS
199	198	5	9	7.0	4643	PASS
275	198	10	60	29.7	19588	PASS
365	198	1	100	4.1	2721	PASS
441	198	0.01	100	13.0	8582	PASS
442	442	50	100	100.0	52555	PASS
443	442	15	24	19.6	10323	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/19/2023	BNA_G	<u>BG057460.D</u>
Compound Name	Response	Retention Time
DDT	232889	21.143
DDD	3728	20.737
DDE	232	20.191
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3960	236849	1.67

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051923\
Data File : BG057460.D
Acq On : 19 May 2023 9:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 20 05:07:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

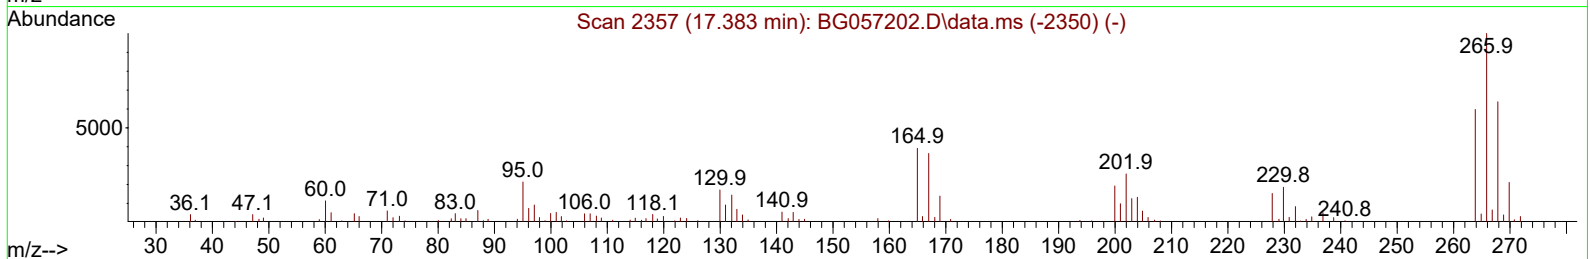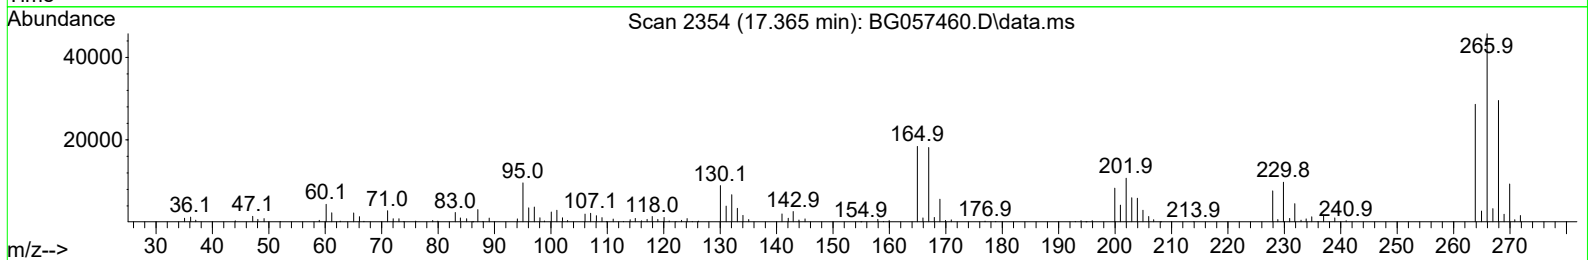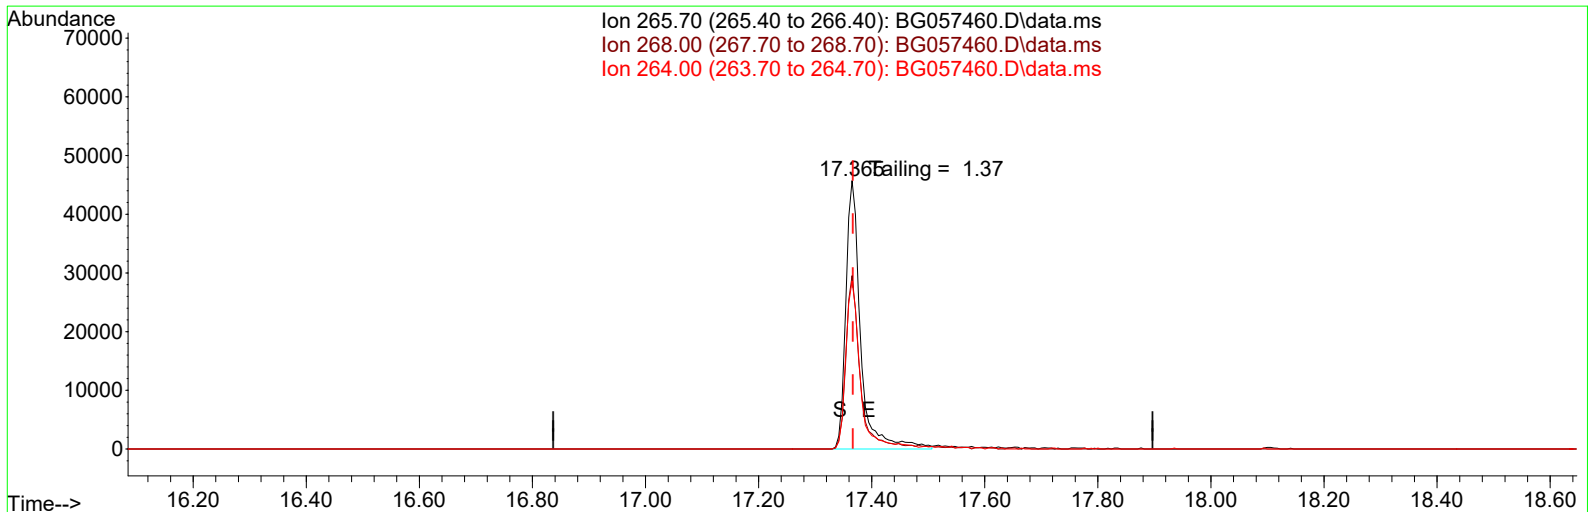

TIC: BG057460.D\data.ms

(70) Pentachlorophenol (C)

17.365min (-0.002) 32133.29 ng




response 80406

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.59
264.00	59.70	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051923\
Data File : BG057460.D
Acq On : 19 May 2023 9:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 20 05:07:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

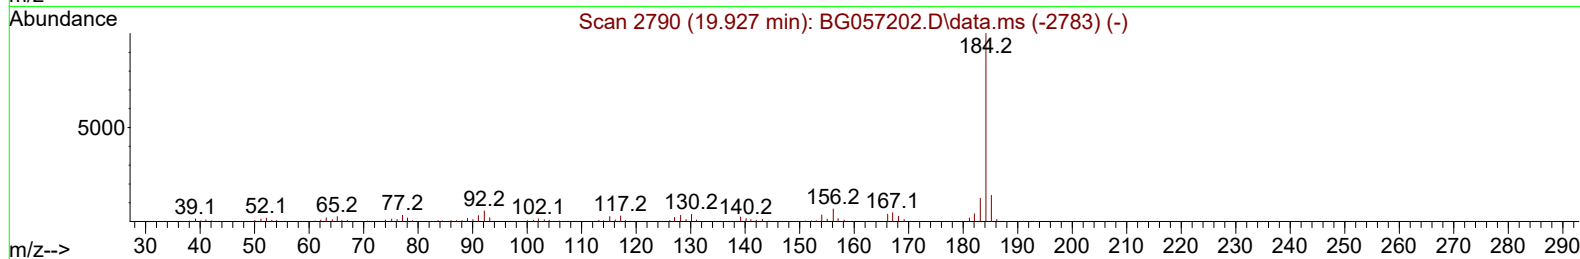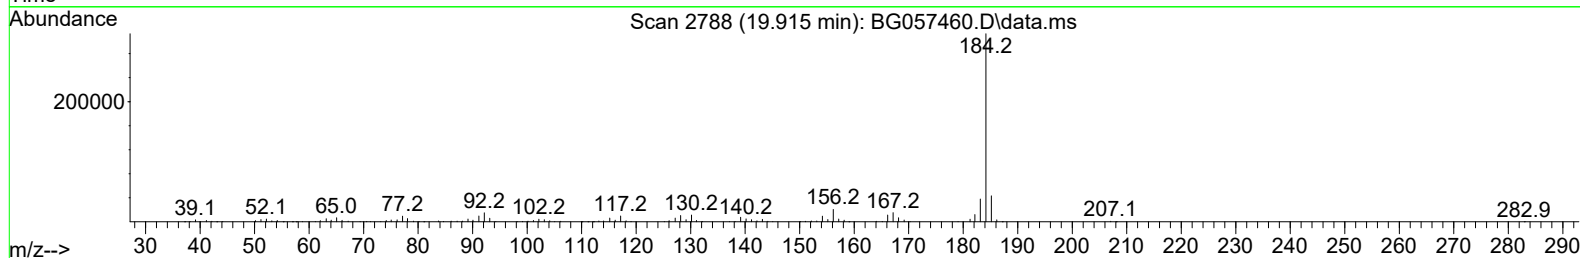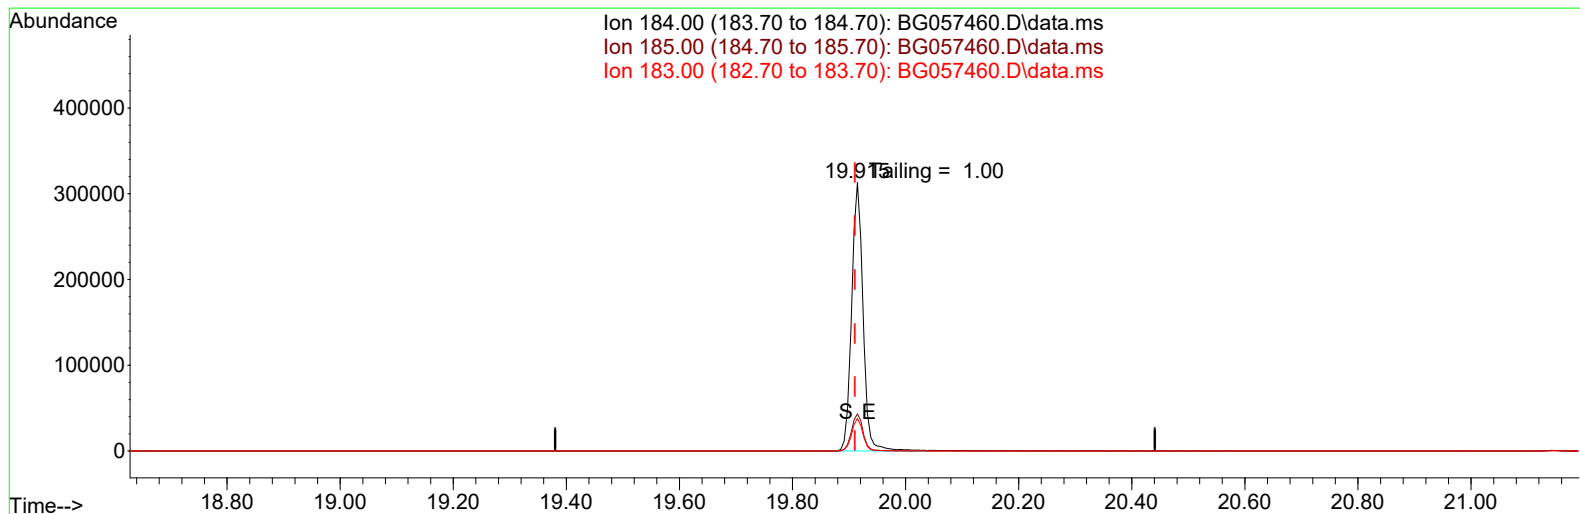

TIC: BG057460.D\data.ms

(77) Benzidine

19.915min (+ 0.004) 0.00 ng

response 440866

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.85
183.00	12.40	12.13
0.00	0.00	0.00