
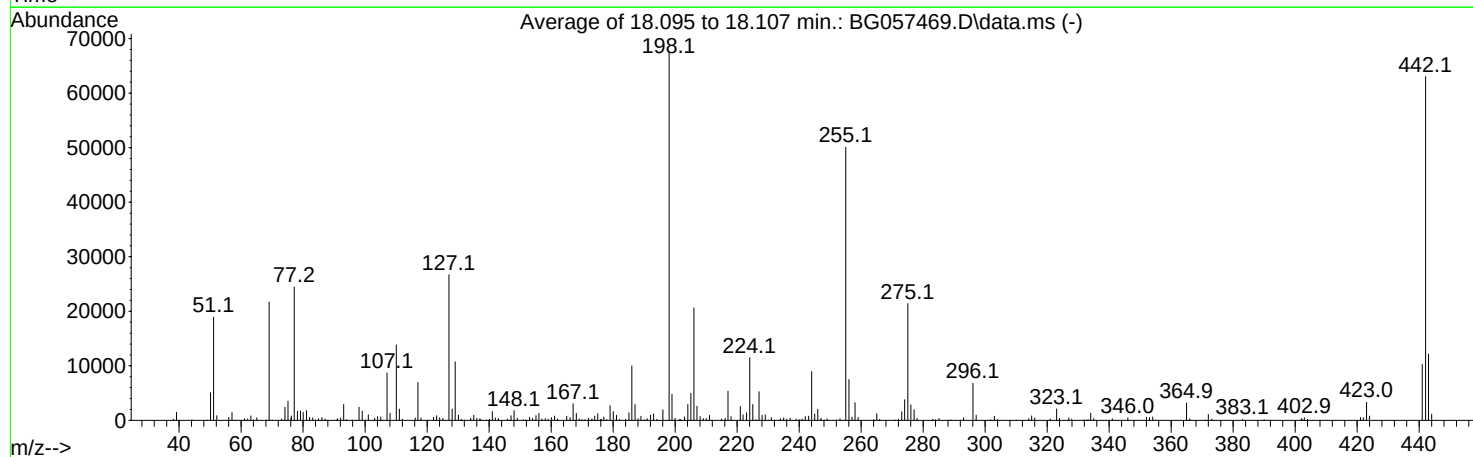


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051923\
Data File : BG057469.D
Acq On : 19 May 2023 16:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat May 20 04:19:55 2023

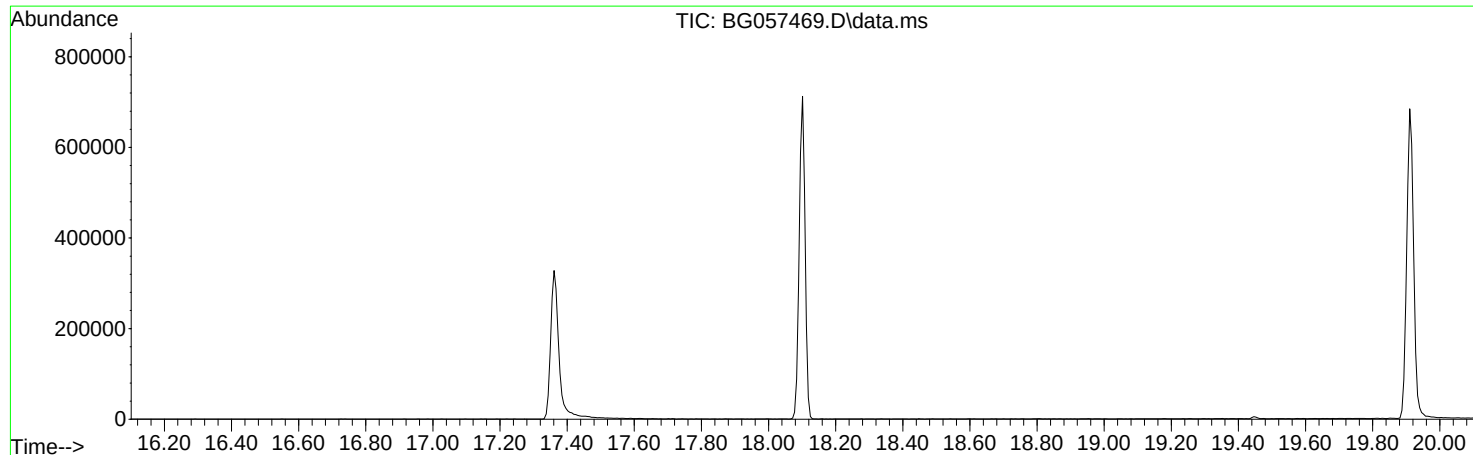

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	18908	PASS
68	69	0.00	2	0.4	92	PASS
69	198	0.00	100	32.2	21718	PASS
70	69	0.00	2	0.3	65	PASS
127	198	10	80	39.6	26699	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67440	PASS
199	198	5	9	7.1	4771	PASS
275	198	10	60	31.7	21408	PASS
365	198	1	100	4.7	3156	PASS
441	198	0.01	100	15.2	10235	PASS
442	442	50	100	100.0	63019	PASS
443	442	15	24	19.3	12170	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/19/2023	BNA_G	<u>BG057469.D</u>
Compound Name	Response	Retention Time
DDT	239031	21.144
DDD	4399	20.739
DDE	246	20.181
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4645	243676	1.91

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051923\
Data File : BG057469.D
Acq On : 19 May 2023 16:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 20 05:08:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

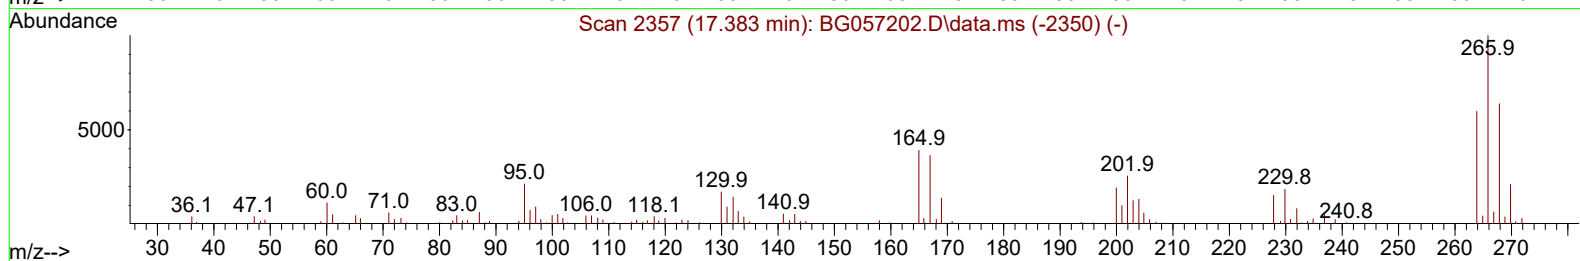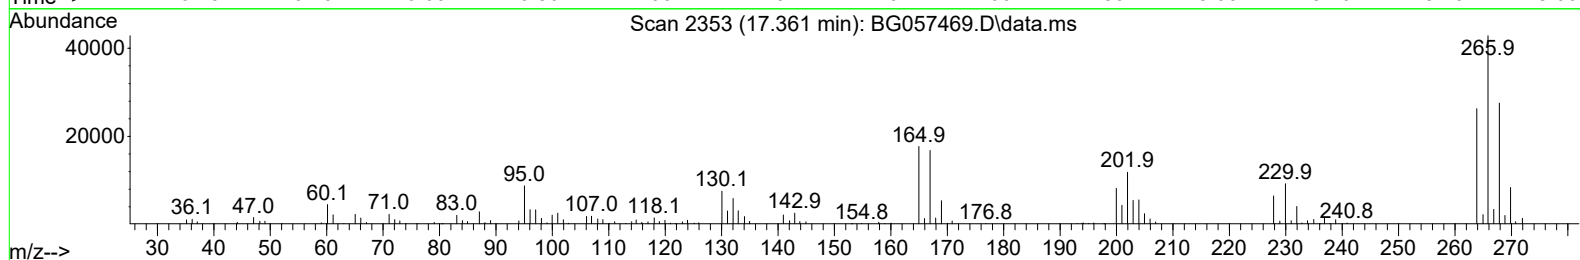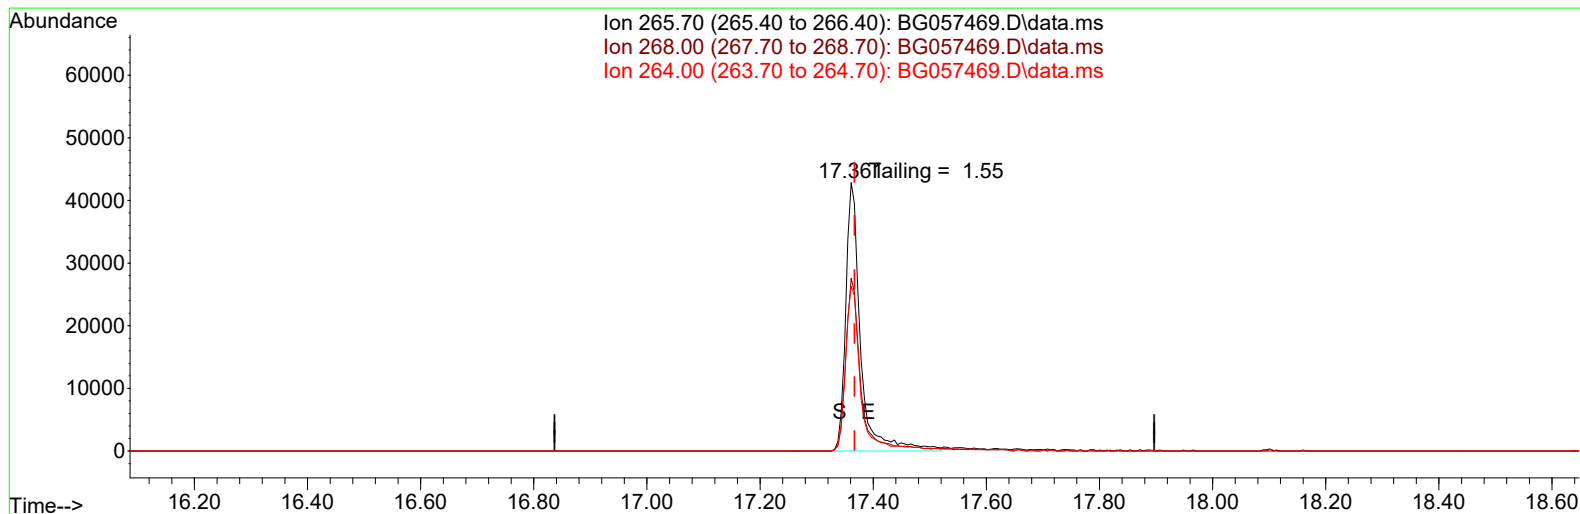

TIC: BG057469.D\data.ms

(70) Pentachlorophenol (C)

17.361min (-0.006) 34475.20 ng




response 78488

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.34
264.00	59.70	61.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051923\
Data File : BG057469.D
Acq On : 19 May 2023 16:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 20 05:08:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

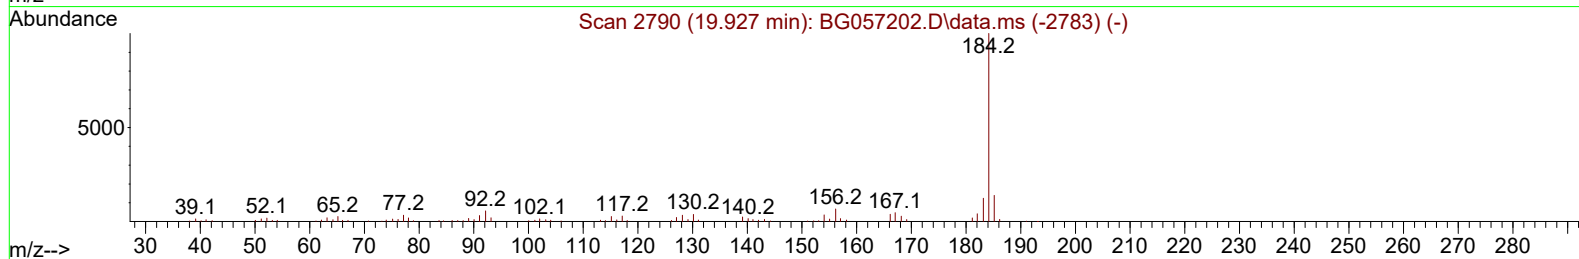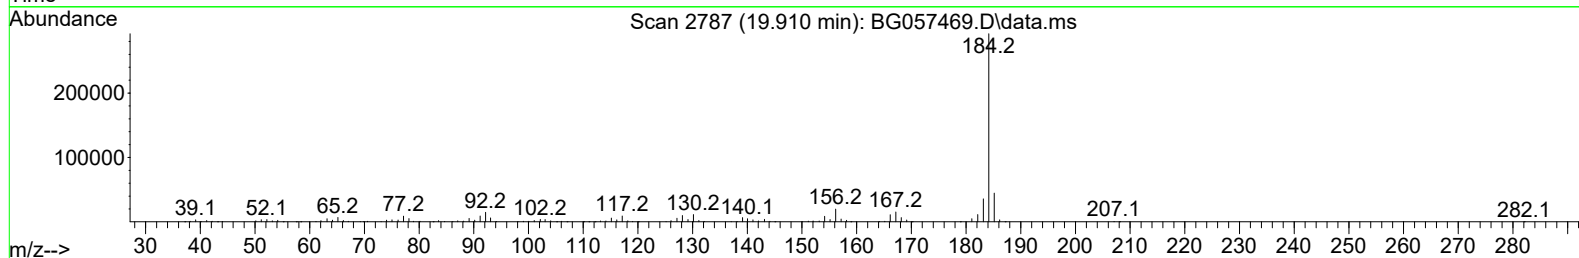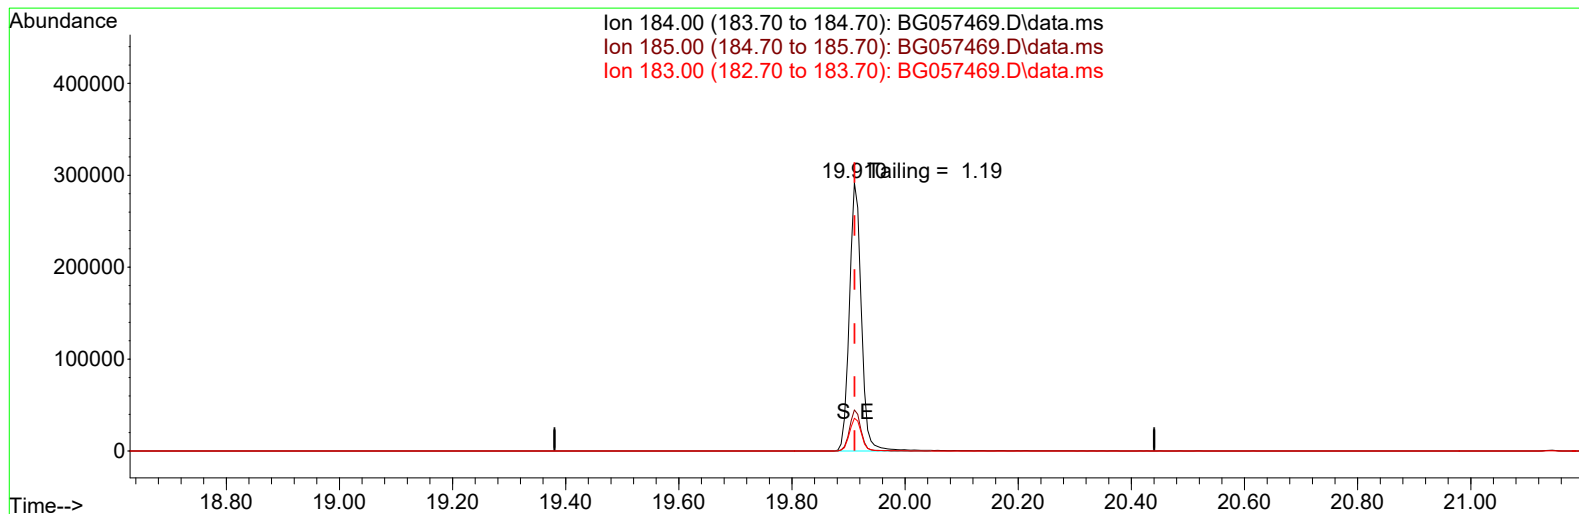

TIC: BG057469.D\data.ms

(77) Benzidine

19.910min (-0.000) 0.00 ng

response 430711

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	15.32
183.00	12.40	12.25
0.00	0.00	0.00