
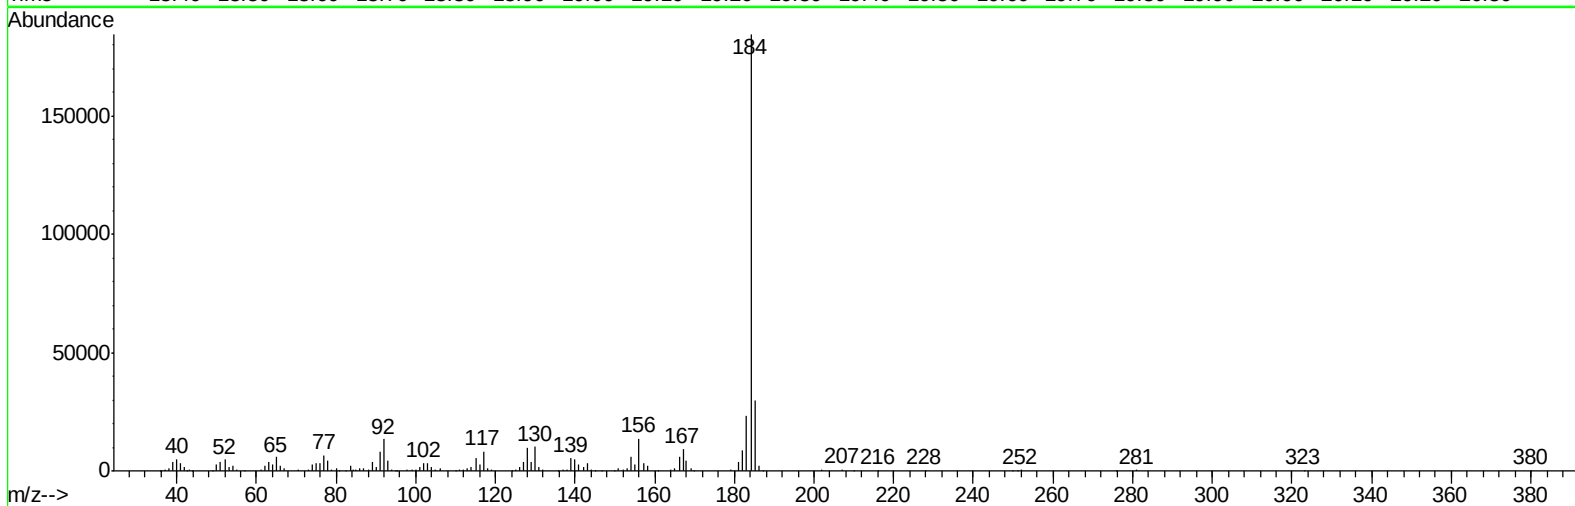


Data Path : Z:\HPCHEM1\BNA G\DATA\BG052015\
Data File : BG017213.D
Acq On : 20 May 2015 13:22
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 04:42:47 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

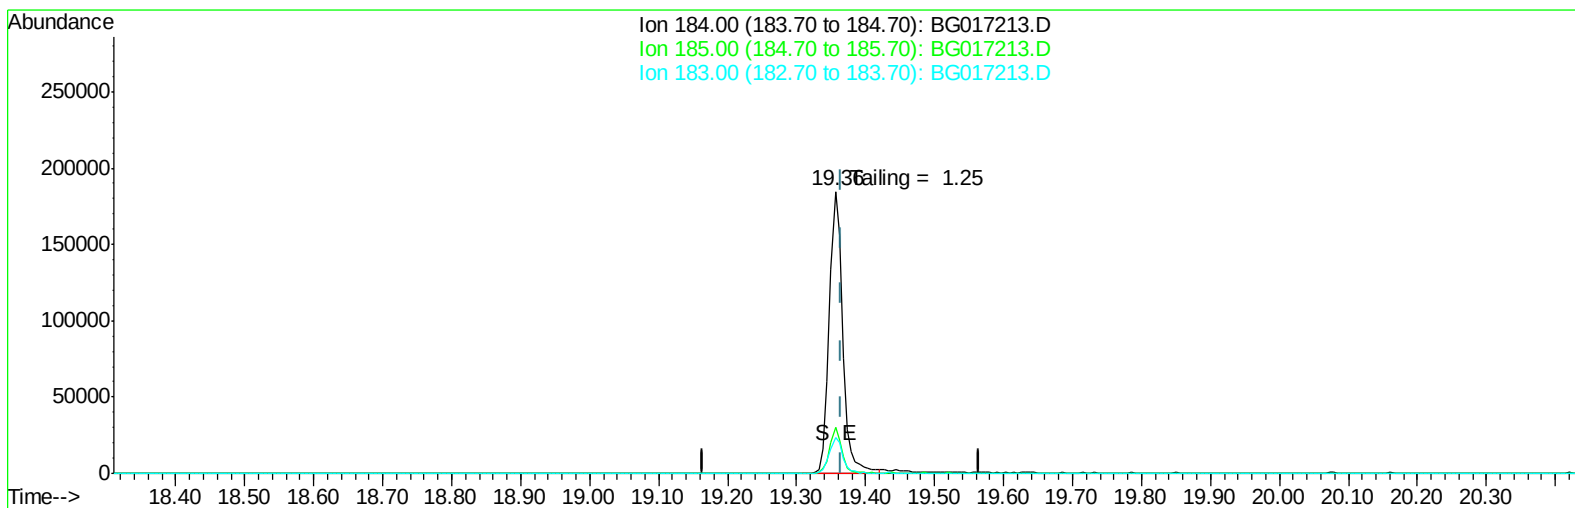

TIC: BG017213.D

(76) Benzidine



19.356min (-0.009) 83183.20ng

response 247148

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	16.19
183.00	14.30	12.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052015\
Data File : BG017213.D
Acq On : 20 May 2015 13:22
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 04:42:47 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

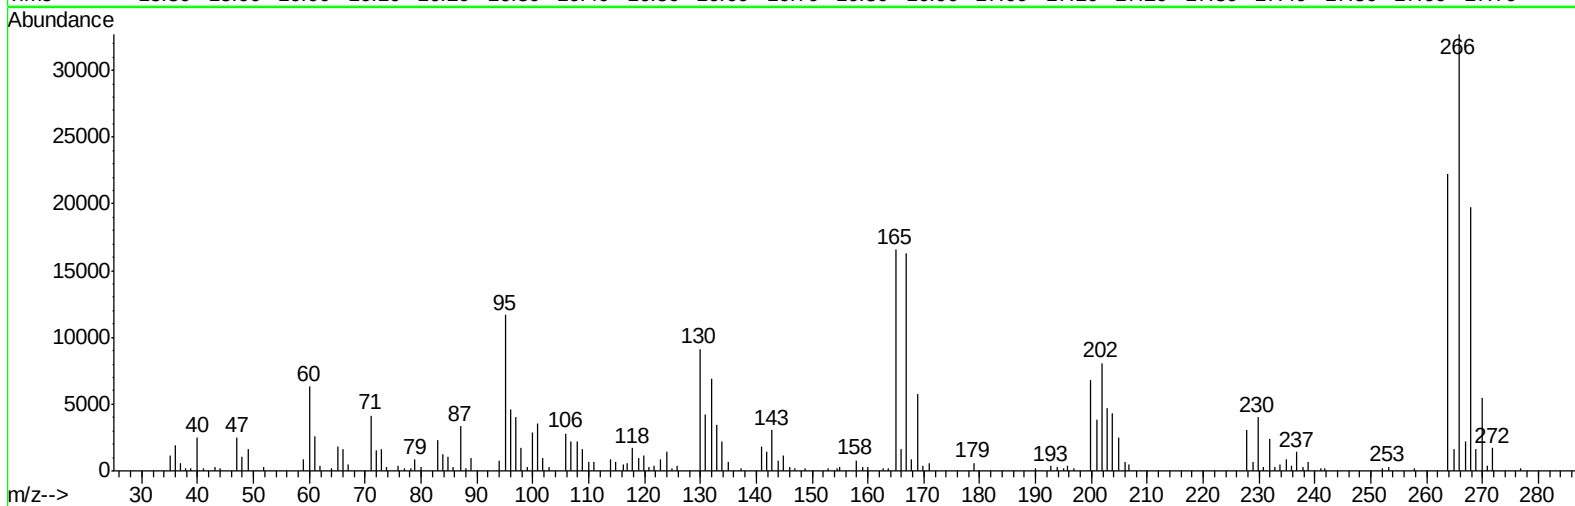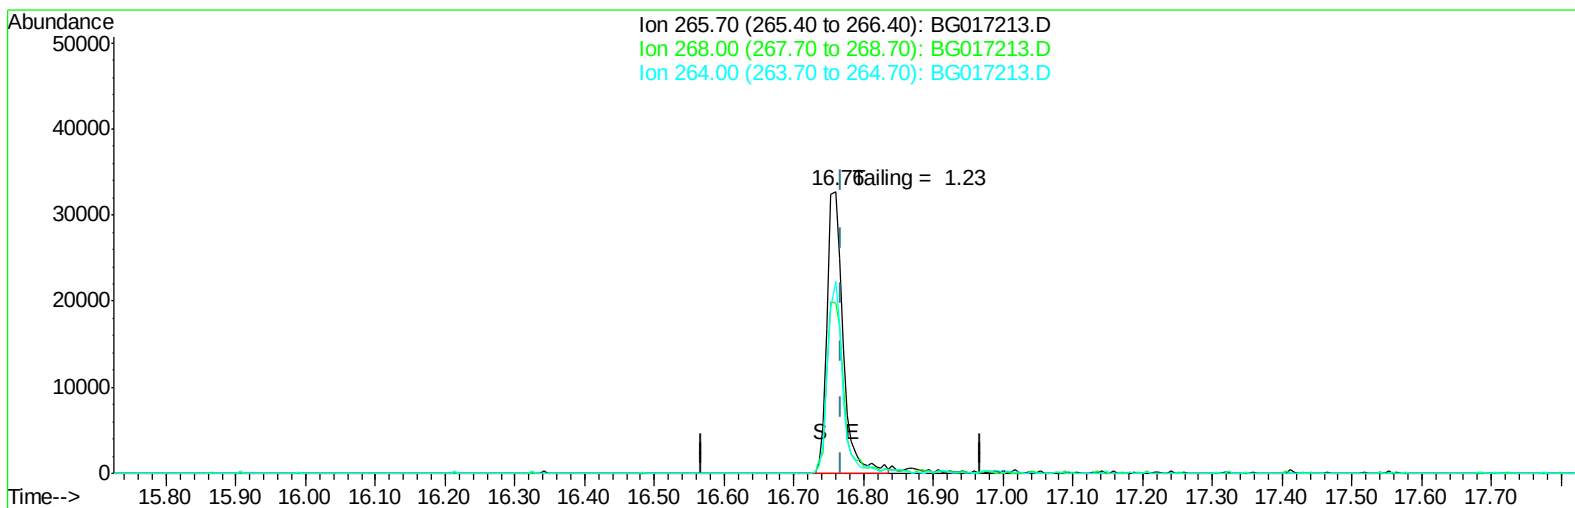

TIC: BG017213.D

(69) Pentachlorophenol (C)

16.759min (-0.009) 54839.50ng

response 51613

Ion	Exp%	Act%
265.70	100	100
268.00	70.70	60.39
264.00	61.70	68.02
0.00	0.00	0.00