
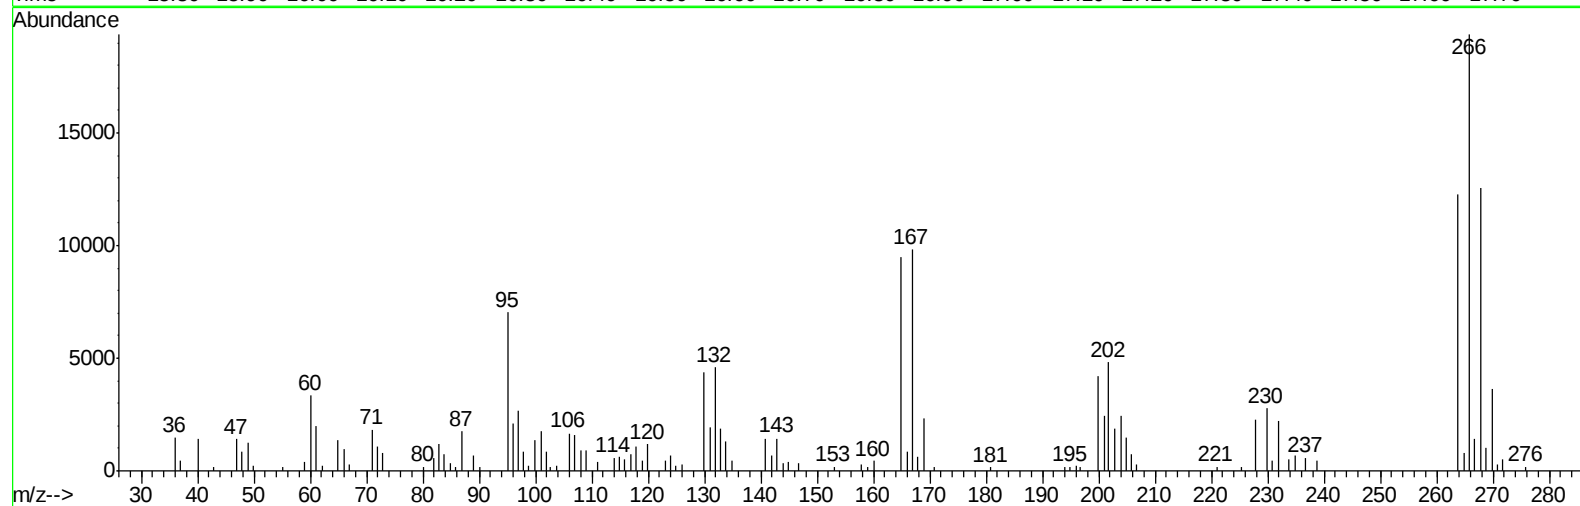


Data Path : Z:\HPCHEM1\BNA G\DATA\BG052015\
Data File : BG017227.D
Acq On : 21 May 2015 00:16
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 04:43:41 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

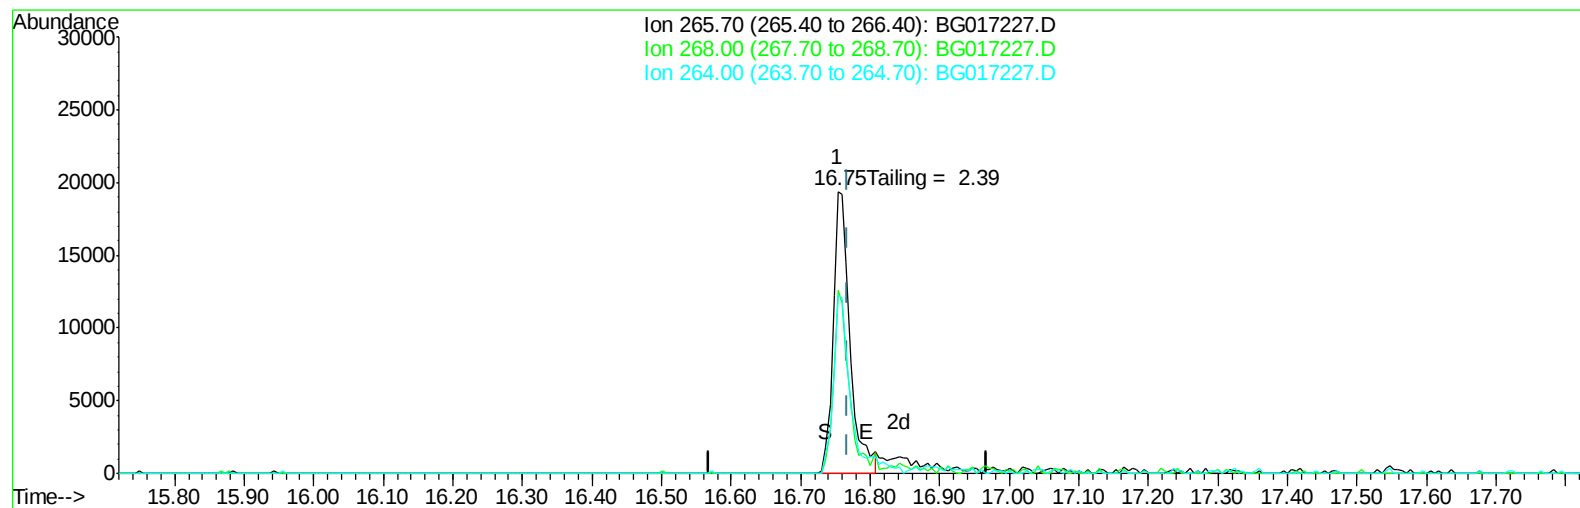

TIC: BG017227.D

(69) Pentachlorophenol (C)



16.754min (-0.014) 2581.02ng m

response 32599

Ion	Exp%	Act%
265.70	100	100
268.00	70.70	64.82
264.00	61.70	63.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052015\
Data File : BG017227.D
Acq On : 21 May 2015 00:16
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 04:43:41 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

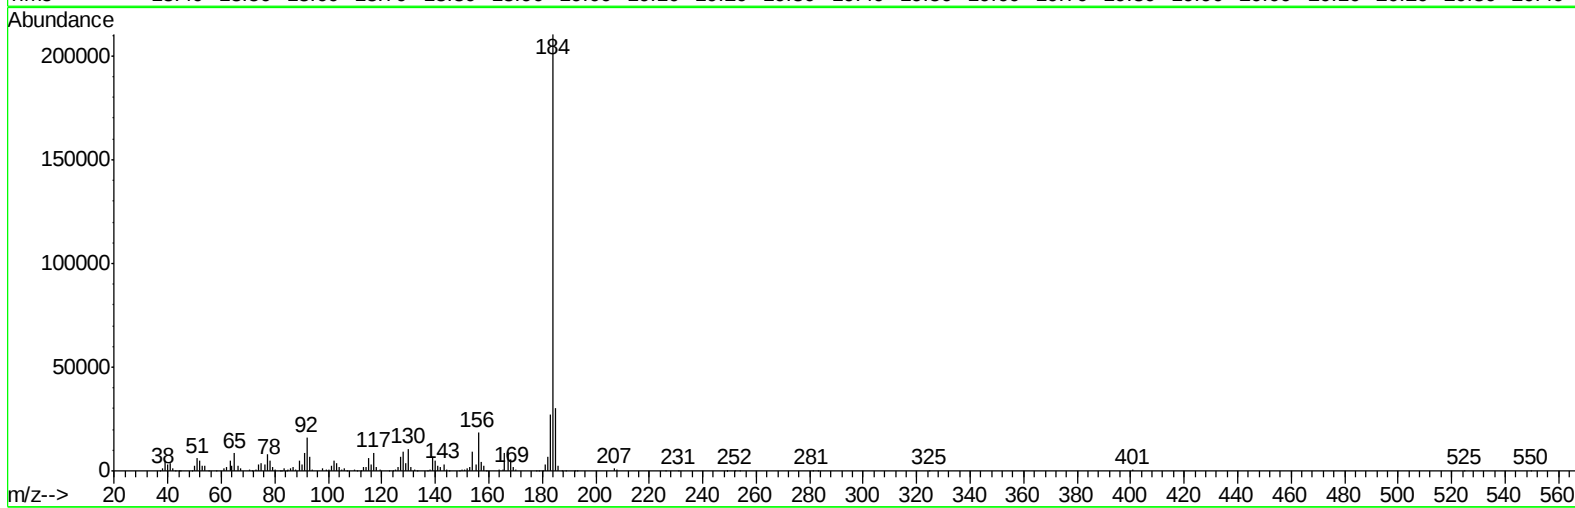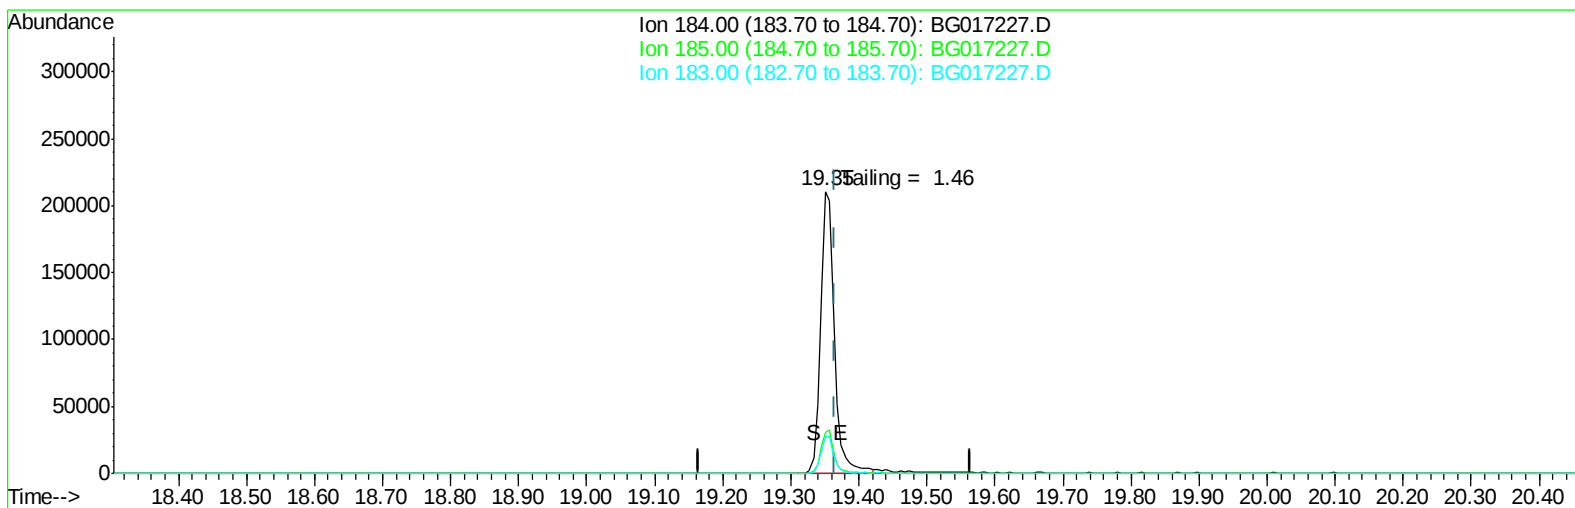

TIC: BG017227.D

(76) Benzidine

19.351min (-0.014) 168727.41ng

response 308499

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.34
183.00	14.30	12.98
0.00	0.00	0.00