

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052015\
Data File : BG017215.D
Acq On : 20 May 2015 14:38
Operator : TP/IZ
Sample : G2295-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.778	12	15	21	rVB3	17729	22905	2.60%	0.633%
2	7.690	845	851	859	rVB	156144	243641	27.62%	6.734%
3	10.486	1320	1327	1335	rVB	218531	357987	40.58%	9.895%
4	14.353	1979	1985	1993	rBV2	346336	525877	59.61%	14.535%
5	17.102	2444	2453	2467	rBV2	491930	725997	82.29%	20.066%
6	21.286	3160	3165	3174	rVB	717800	882198	100.00%	24.384%
7	23.548	3544	3550	3558	rVB2	467166	859373	97.41%	23.753%


Sum of corrected areas: 3617978

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052015\
Data File : BG017215.D
Acq On : 20 May 2015 14:38
Operator : TP/IZ
Sample : G2295-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

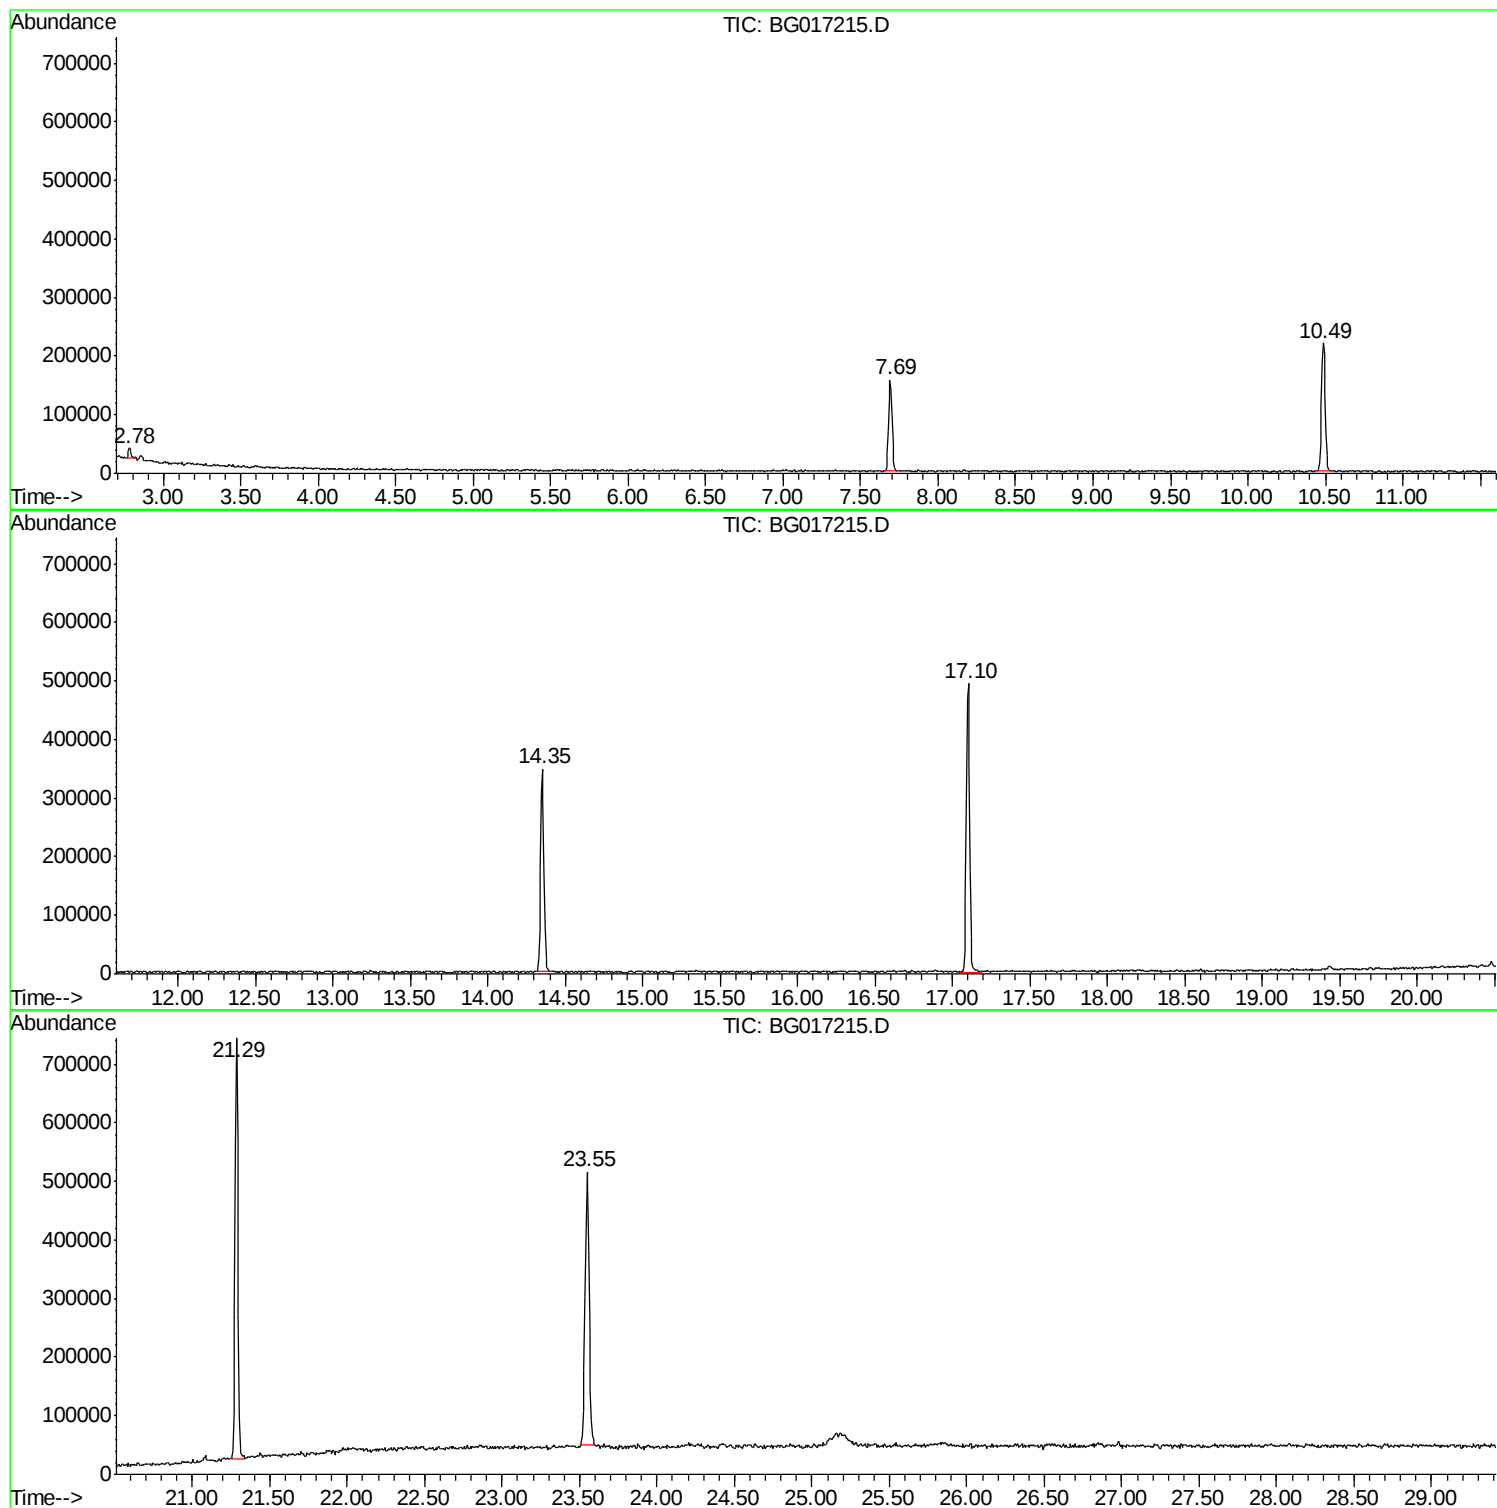

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052015\
Data File : BG017215.D
Acq On : 20 May 2015 14:38
Operator : TP/IZ
Sample : G2295-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052015\
Data File : BG017215.D
Acq On : 20 May 2015 14:38
Operator : TP/IZ
Sample : G2295-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc