

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052015\
 Data File : BG017234.D
 Acq On : 21 May 2015 4:54
 Operator : TP/IZ
 Sample : G2273-21
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-07-D1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.777	11	15	22	rVB3	64391	94966	2.52%	0.544%
2	2.871	27	31	38	rVB	389696	478231	12.68%	2.739%
3	4.805	351	360	366	rBV	324697	447022	11.85%	2.560%
4	5.286	436	442	451	rBV	840404	1177982	31.23%	6.746%
5	6.890	709	715	726	rBV	790661	1202923	31.89%	6.889%
6	7.231	766	773	781	rBV	870536	1377657	36.53%	7.890%
7	7.689	845	851	859	rVB	165267	254829	6.76%	1.459%
8	8.012	897	906	916	rBV	616322	969285	25.70%	5.551%
9	8.853	1041	1049	1059	rBV	558104	898874	23.83%	5.148%
10	10.486	1320	1327	1335	rBV	216774	346687	9.19%	1.985%
11	12.966	1743	1749	1758	rBV	1273642	1853816	49.15%	10.616%
12	14.352	1978	1985	1996	rBV3	299262	474329	12.58%	2.716%
13	15.845	2233	2239	2255	rBV	1113874	1643759	43.58%	9.413%
14	17.096	2446	2452	2460	rBV2	463917	648681	17.20%	3.715%
15	19.352	2831	2836	2846	rBV	79286	129874	3.44%	0.744%
16	19.734	2895	2901	2910	rBV	3128526	3771714	100.00%	21.600%
17	19.987	2940	2944	2949	rBV	39191	59950	1.59%	0.343%
18	20.480	3023	3028	3033	rBV4	41715	54274	1.44%	0.311%
19	21.285	3160	3165	3170	rBV	679497	808562	21.44%	4.630%
20	23.547	3543	3550	3560	rBV	402860	768341	20.37%	4.400%


Sum of corrected areas: 17461756

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052015\
Data File : BG017234.D
Acq On : 21 May 2015 4:54
Operator : TP/IZ
Sample : G2273-21
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-07-D1

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

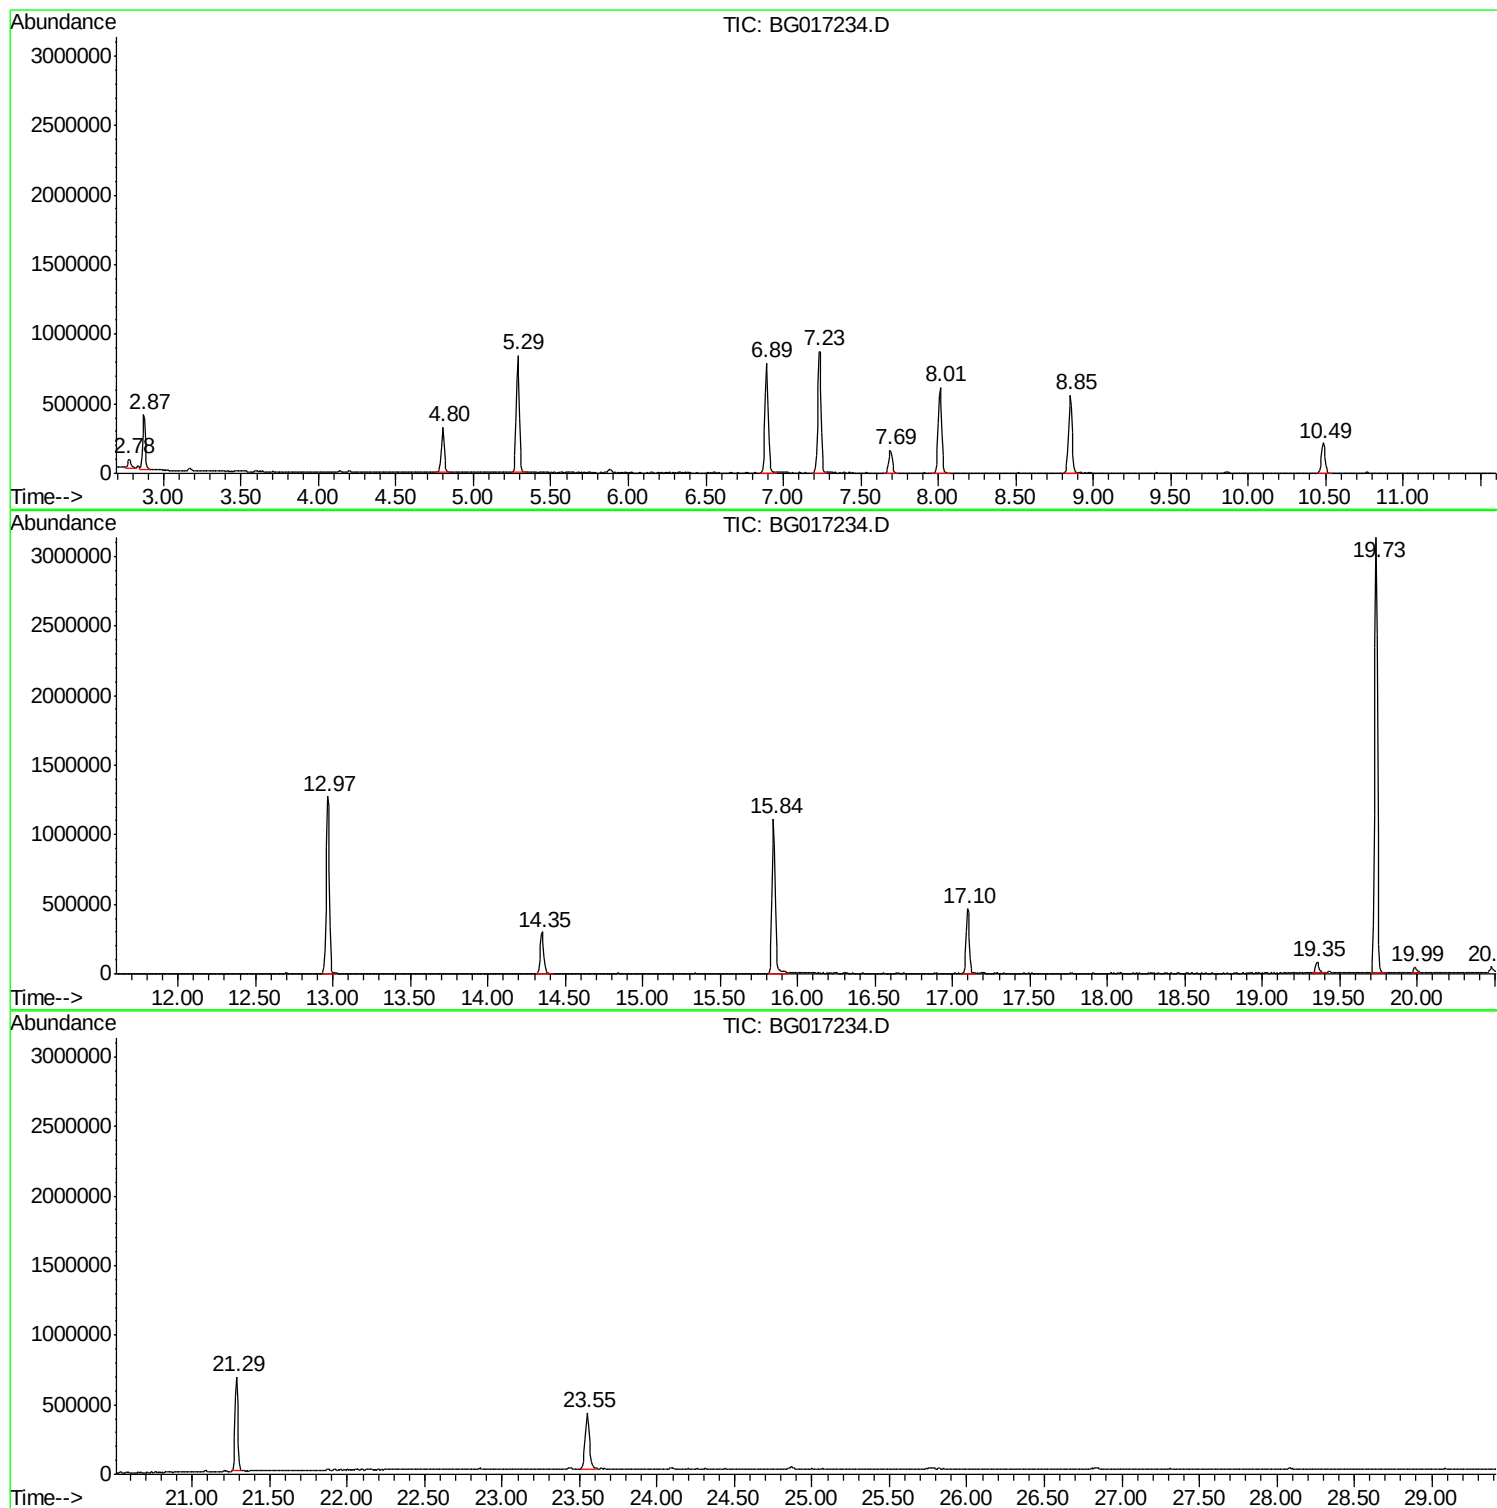

DbaaaPath::ZZ\NRPBHHM1BBAAGCDBAA\BB0020055\
 DbaaaFile::BB00I2234DD
 AcqQOn :221May2005 4454
 Operator::TPPIZ
 Sample::G0223321
 Misc :
 ASSVal :199 SampleMultiplier:11

Instrument :
 BNA_G
 ClientSampleId :
 WC-07-D1

QcadtMebdd::ZZ\NRPBHHM1BBAAGCMEEH00S8270BB005335MM
 QcadtTitle::ASBPBNASSANDABBSF00R55P000NTCALIBRATION

TICLibrary :CC\DATA\BBS\END\$S002LL
 TICIntegratIonParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
