


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052015\
Data File : BG017213.D
Acq On : 20 May 2015 13:22
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 13 16:12:13 2015

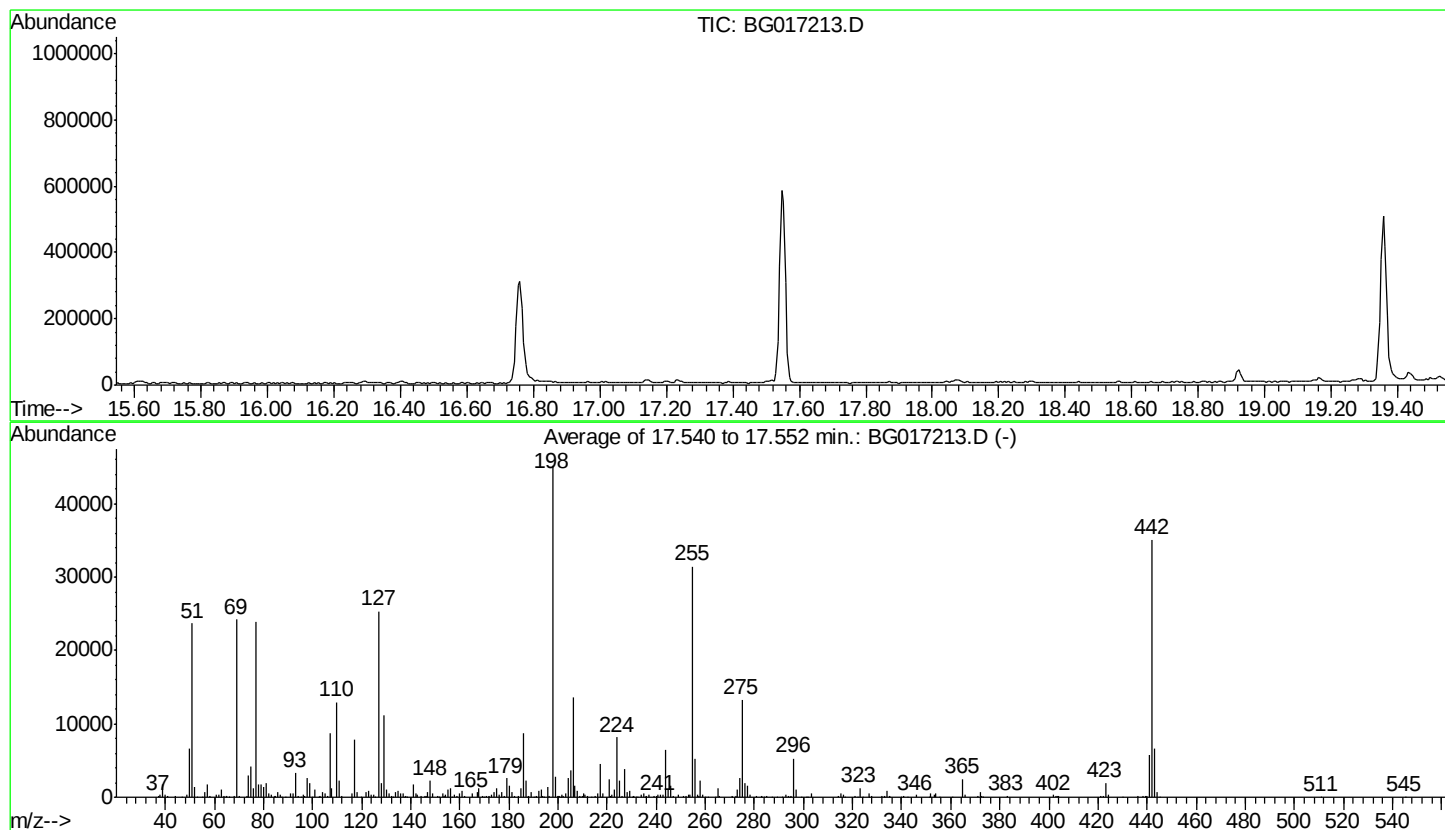

AutoFind: Scans 2528, 2529, 2530; Background Corrected with Scan 2522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	23714	PASS
68	69	0.00	2	0.6	144	PASS
69	198	0.00	100	53.6	24205	PASS
70	69	0.00	2	0.6	149	PASS
127	198	10	80	56.1	25357	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45197	PASS
199	198	5	9	6.2	2819	PASS
275	198	10	60	29.4	13274	PASS
365	198	1	100	5.5	2482	PASS
441	442	0.01	24	16.6	5836	PASS
442	198	50	100	77.8	35144	PASS
443	442	15	24	18.8	6613	PASS