


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052015\
 Data File : BG017227.D
 Acq On : 21 May 2015 00:16
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 16:12:13 2015

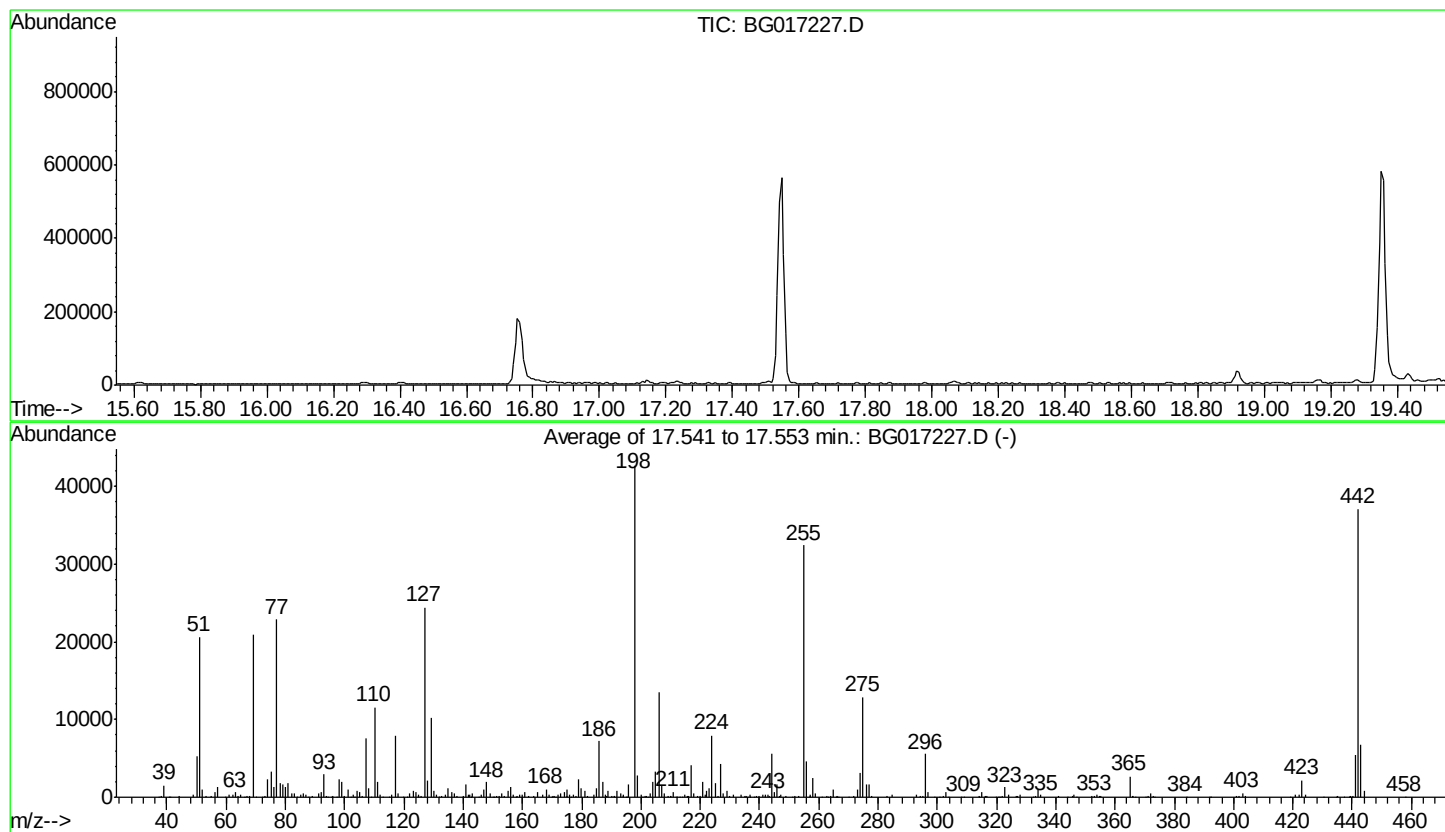

AutoFind: Scans 2528, 2529, 2530; Background Corrected with Scan 2522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	20632	PASS
68	69	0.00	2	0.5	103	PASS
69	198	0.00	100	49.0	20901	PASS
70	69	0.00	2	0.3	53	PASS
127	198	10	80	57.2	24413	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42674	PASS
199	198	5	9	6.4	2746	PASS
275	198	10	60	30.1	12861	PASS
365	198	1	100	6.3	2706	PASS
441	442	0.01	24	14.6	5410	PASS
442	198	50	100	86.9	37093	PASS
443	442	15	24	18.4	6813	PASS