
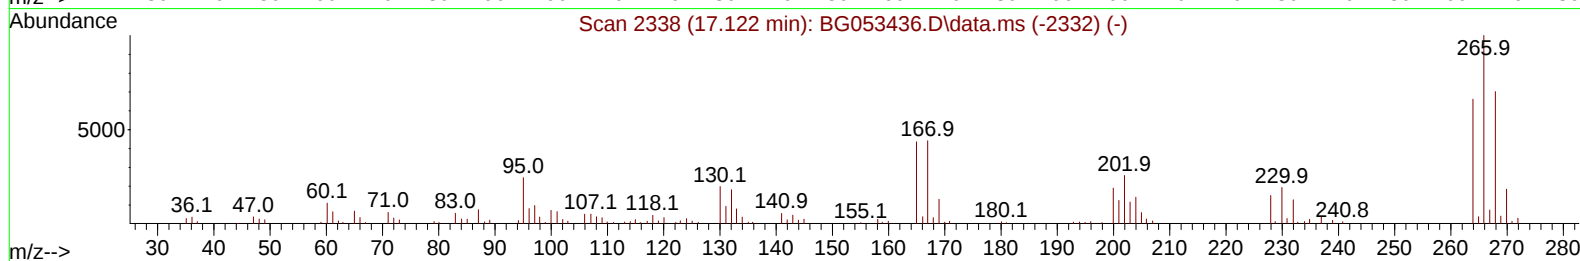
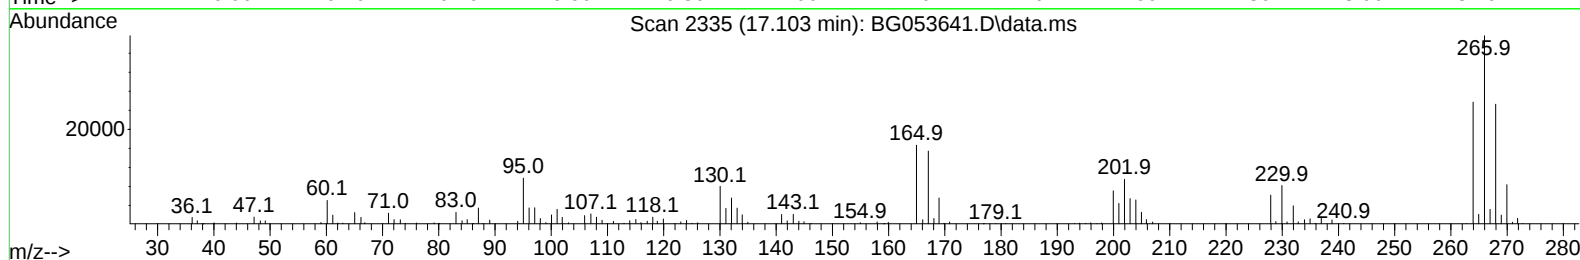


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052022\  
Data File : BG053641.D  
Acq On : 20 May 2022 12:45  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 13:29:48 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG050522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 20 03:55:28 2022  
Response via : Initial Calibration

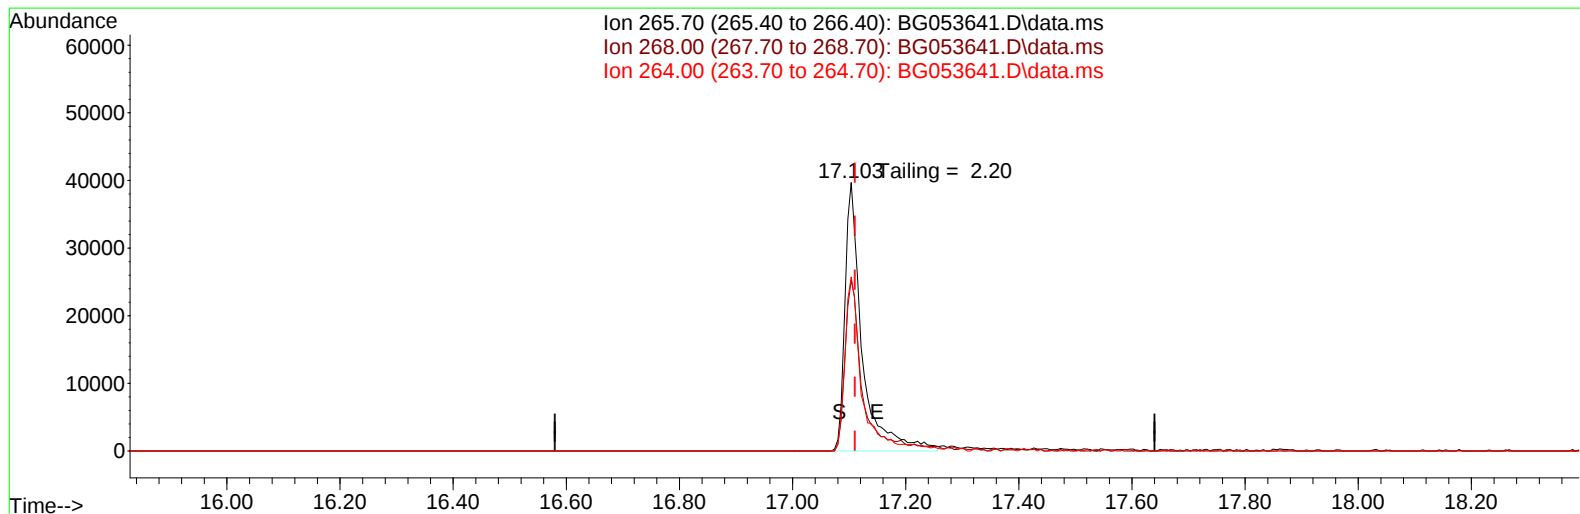

TIC: BG053641.D\data.ms

**(70) Pentachlorophenol (C)**




17.103min (-0.006) 154739.95 ng

response 81476

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 70.20  | 63.75  |
| 264.00 | 66.20  | 64.84  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052022\  
Data File : BG053641.D  
Acq On : 20 May 2022 12:45  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 13:29:48 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG050522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 20 03:55:28 2022  
Response via : Initial Calibration

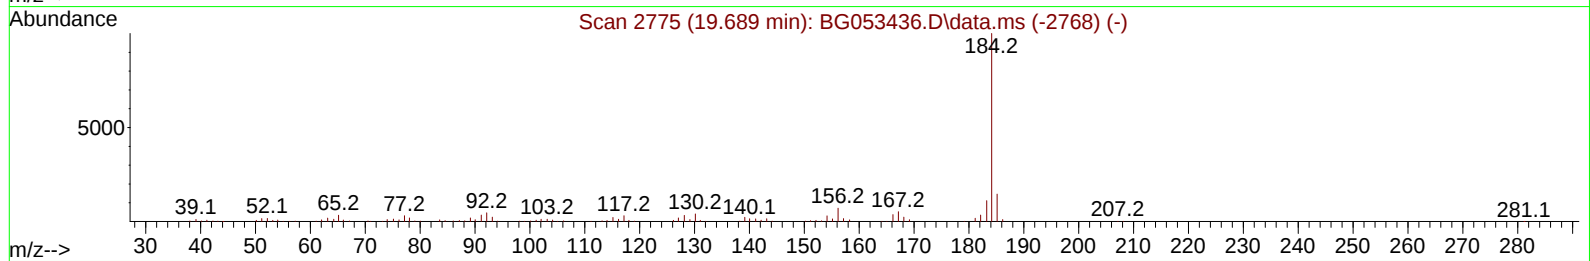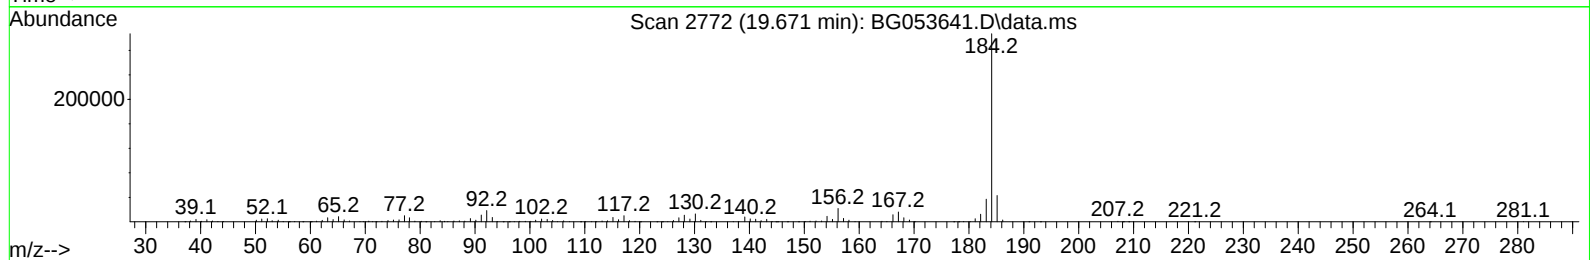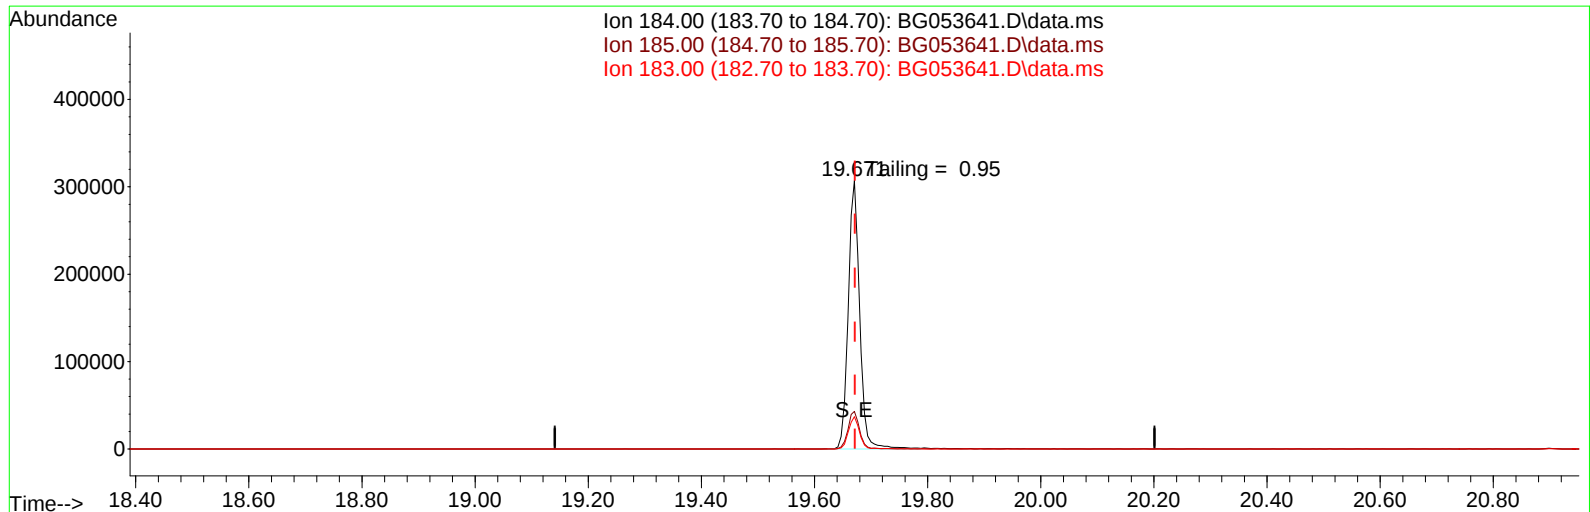

TIC: BG053641.D\data.ms

**(77) Benzidine****19.671min (-0.000) 62976.84 ng****response 431648**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.70  | 14.03  |
| 183.00 | 11.10  | 12.08  |
| 0.00   | 0.00   | 0.00   |