

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052022\
 Data File : BG053657.D
 Acq On : 20 May 2022 23:40
 Operator : CG/JU
 Sample : N2960-03 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BIN-4-SP-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.641	376	383	394	rBV	116216	214075	36.83%	4.710%
2	7.245	647	656	668	rBV	119535	242878	41.78%	5.343%
3	8.073	787	797	805	rBV	155036	273476	47.05%	6.016%
4	9.236	988	995	1012	rVB2	79438	158309	27.23%	3.483%
5	10.881	1264	1275	1285	rBV	209418	388624	66.86%	8.549%
6	13.231	1670	1675	1680	rBV4	5202	10262	1.77%	0.226%
7	13.319	1684	1690	1701	rVB	231814	350554	60.31%	7.712%
8	13.513	1717	1723	1726	rBV4	4699	7931	1.36%	0.174%
9	14.141	1823	1830	1832	rBV7	7645	14310	2.46%	0.315%
10	14.165	1832	1834	1838	rVB2	7482	9499	1.63%	0.209%
11	14.529	1892	1896	1900	rVB6	4947	7735	1.33%	0.170%
12	14.582	1900	1905	1909	rBV3	5067	9286	1.60%	0.204%
13	14.699	1914	1925	1932	rBV	333089	521329	89.68%	11.469%
14	15.087	1985	1991	1995	rBV6	4987	10341	1.78%	0.227%
15	15.527	2063	2066	2073	rVB4	6250	9956	1.71%	0.219%
16	15.933	2131	2135	2144	rVB4	9260	17578	3.02%	0.387%
17	16.150	2168	2172	2173	rBV4	5118	6219	1.07%	0.137%
18	16.191	2173	2179	2188	rVB	147024	238724	41.07%	5.252%
19	16.415	2213	2217	2221	rVB4	18312	27239	4.69%	0.599%
20	16.602	2246	2249	2252	rBV4	5944	8627	1.48%	0.190%
21	16.644	2252	2256	2260	rBV2	10487	17671	3.04%	0.389%
22	17.178	2344	2347	2350	rBV5	6383	8499	1.46%	0.187%
23	17.231	2351	2356	2361	rVV3	11024	19527	3.36%	0.430%
24	17.443	2386	2392	2401	rBV	378487	581289	100.00%	12.788%
25	17.730	2435	2441	2442	rBV6	5757	10534	1.81%	0.232%
26	17.918	2470	2473	2477	rVB5	7645	10911	1.88%	0.240%
27	18.030	2486	2492	2494	rBV7	4482	7490	1.29%	0.165%
28	18.606	2588	2590	2595	rBV5	8399	12924	2.22%	0.284%
29	18.982	2652	2654	2657	rBV4	8263	7877	1.36%	0.173%
30	19.234	2694	2697	2701	rBV6	18563	28846	4.96%	0.635%
31	20.045	2830	2835	2840	rBV	313564	403503	69.42%	8.877%
32	21.725	3116	3121	3128	rVB2	307573	512720	88.20%	11.279%
33	24.997	3674	3678	3691	rVB2	137291	396855	68.27%	8.731%


Sum of corrected areas: 4545598

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052022\
Data File : BG053657.D
Acq On : 20 May 2022 23:40
Operator : CG/JU
Sample : N2960-03 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BIN-4-SP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

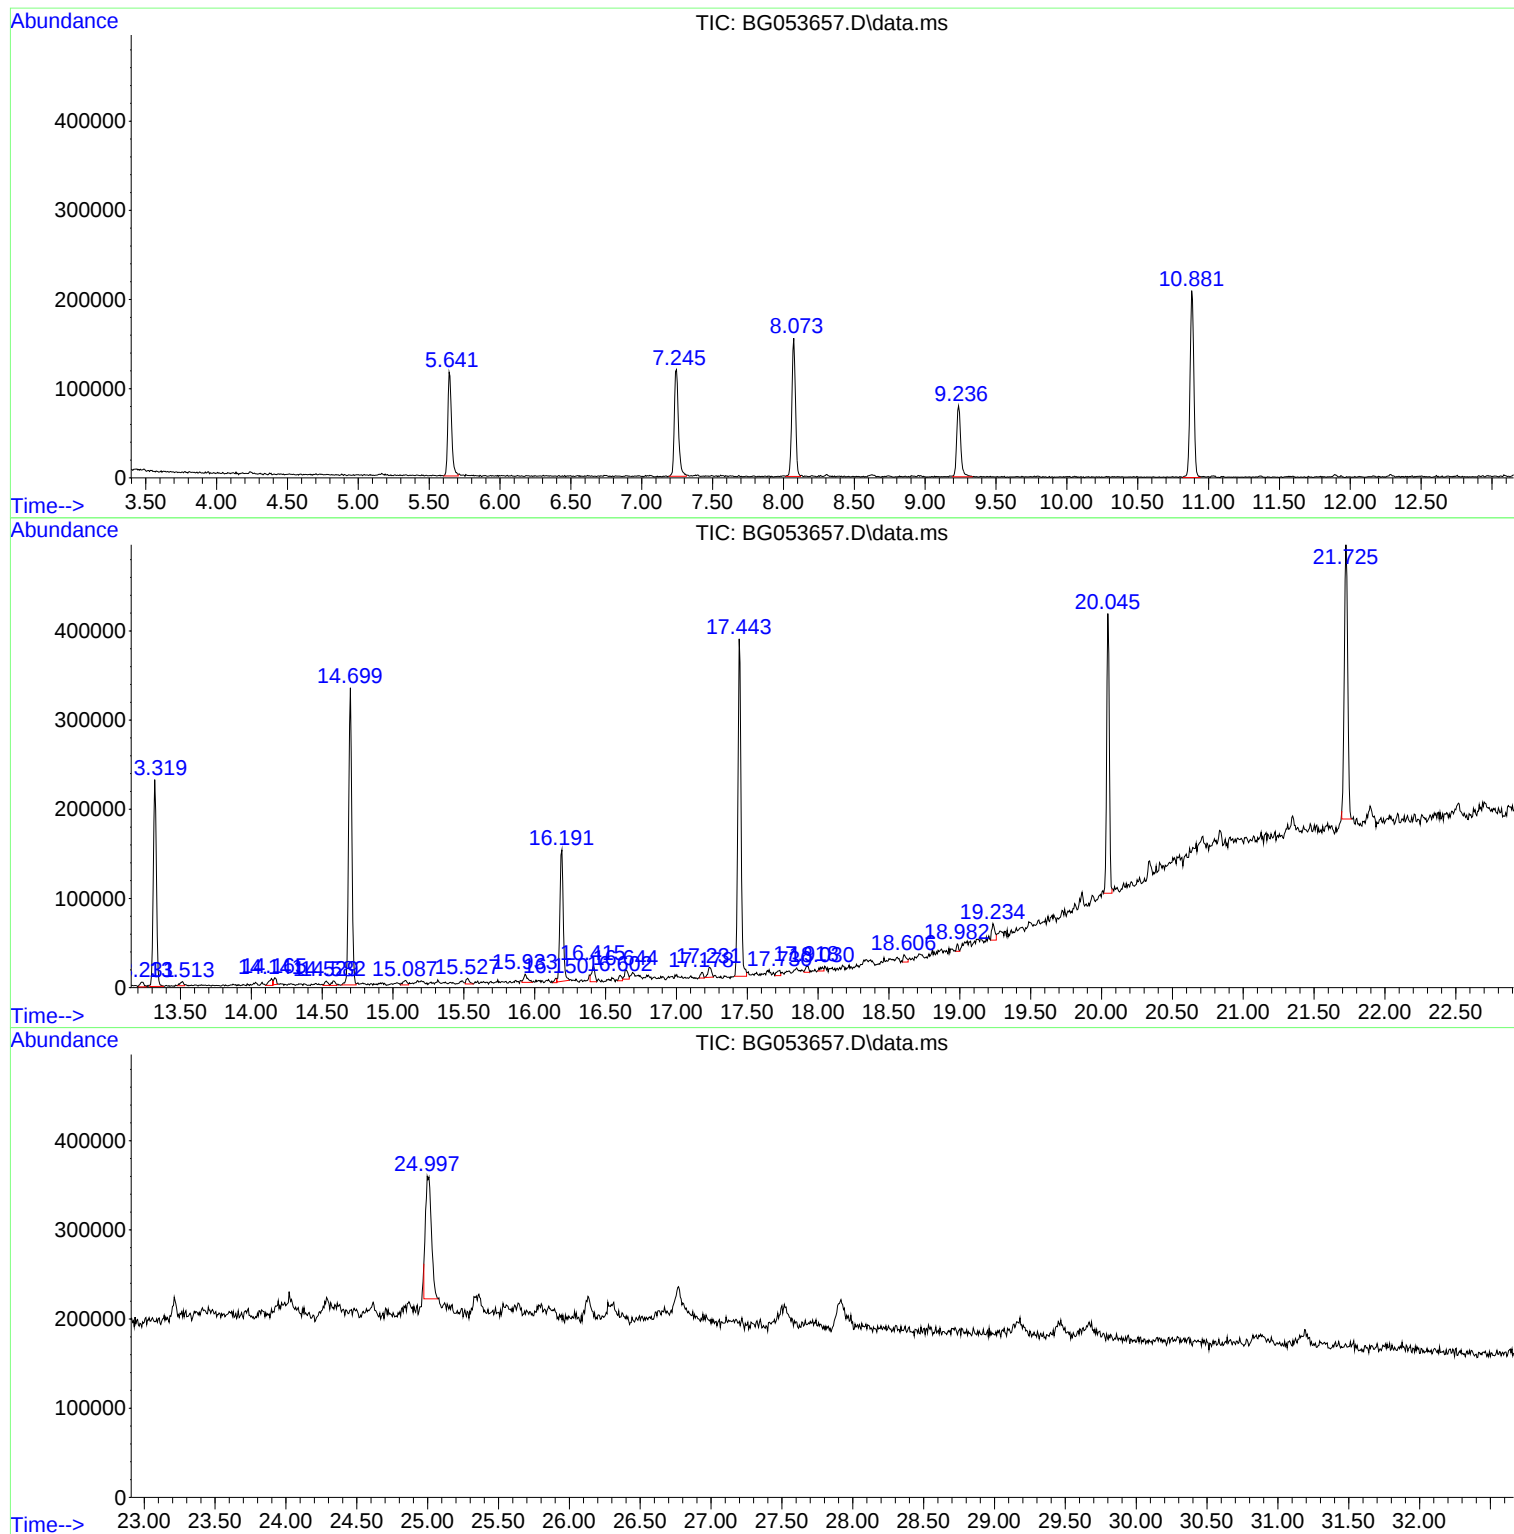

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052022\
Data File : BG053657.D
Acq On : 20 May 2022 23:40
Operator : CG/JU
Sample : N2960-03 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BIN-4-SP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052022\
Data File : BG053657.D
Acq On : 20 May 2022 23:40
Operator : CG/JU
Sample : N2960-03 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BIN-4-SP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------