


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052022\
 Data File : BG053641.D
 Acq On : 20 May 2022 12:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 20 03:55:28 2022

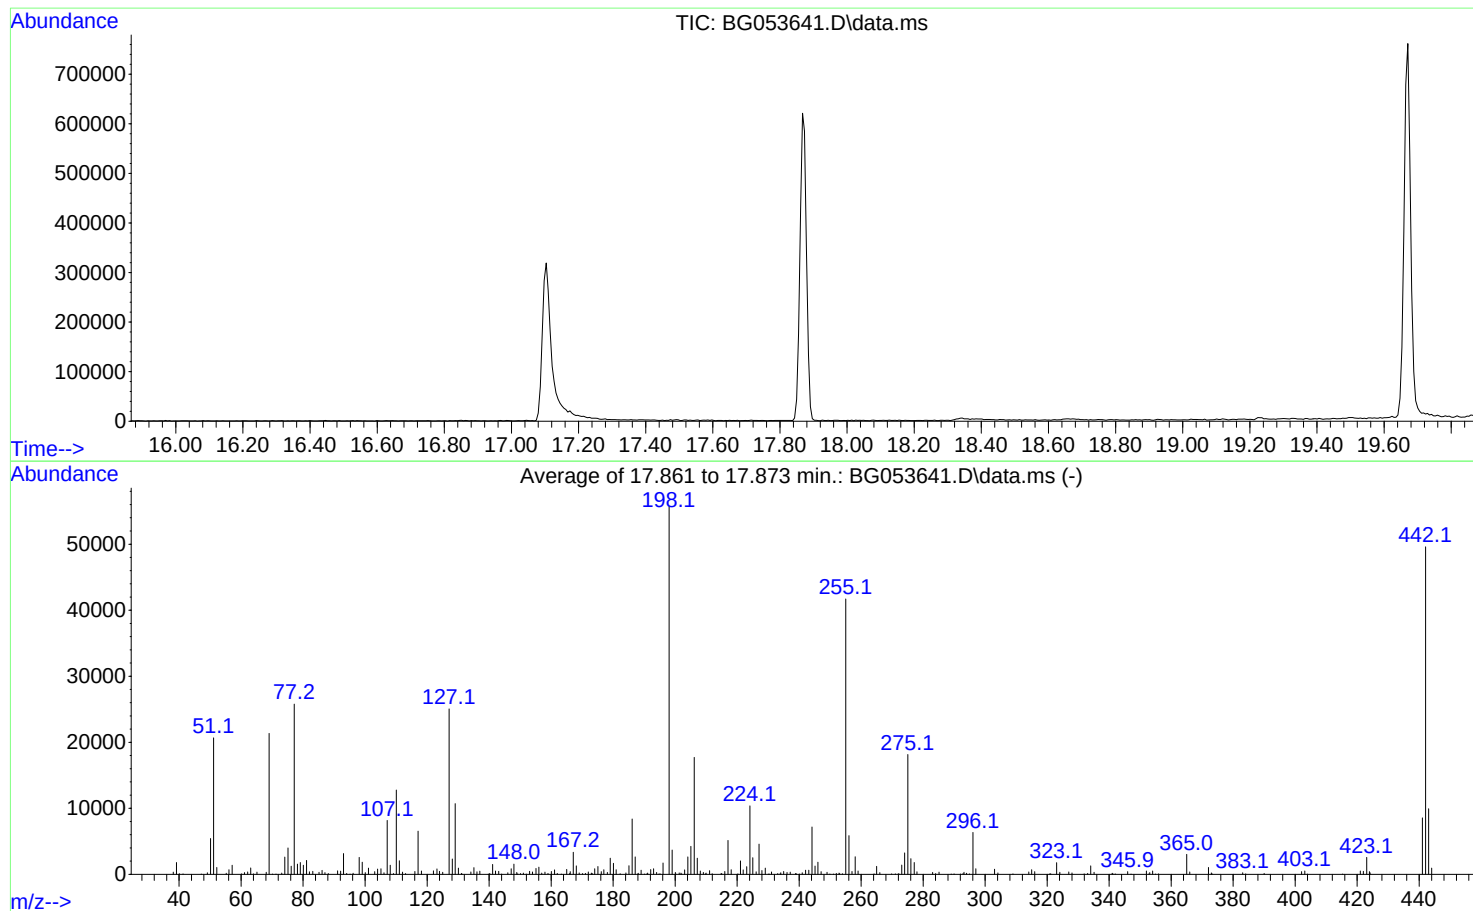




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	20675	PASS
68	69	0.00	2	1.5	314	PASS
69	198	0.00	100	38.3	21352	PASS
70	69	0.00	2	0.3	54	PASS
127	198	10	80	45.0	25059	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55709	PASS
199	198	5	9	6.6	3685	PASS
275	198	10	60	32.6	18160	PASS
365	198	1	100	5.4	3024	PASS
441	198	0.01	100	15.4	8555	PASS
442	442	50	100	100.0	49613	PASS
443	442	15	24	20.0	9933	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052022\
Data File : BG053641.D
Acq On : 20 May 2022 12:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 20 13:29:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 03:55:28 2022
Response via : Initial Calibration

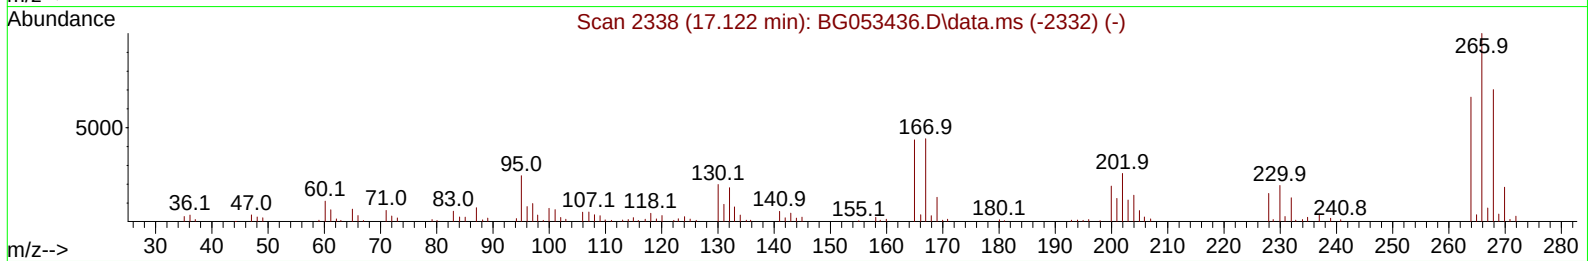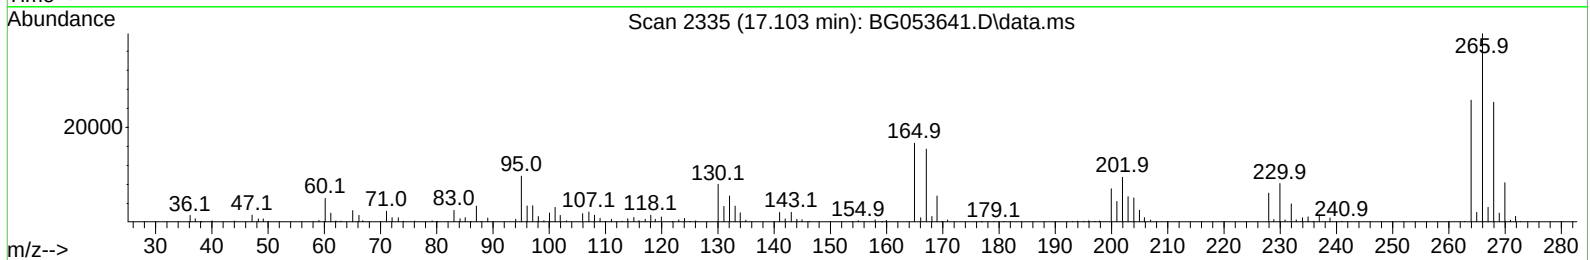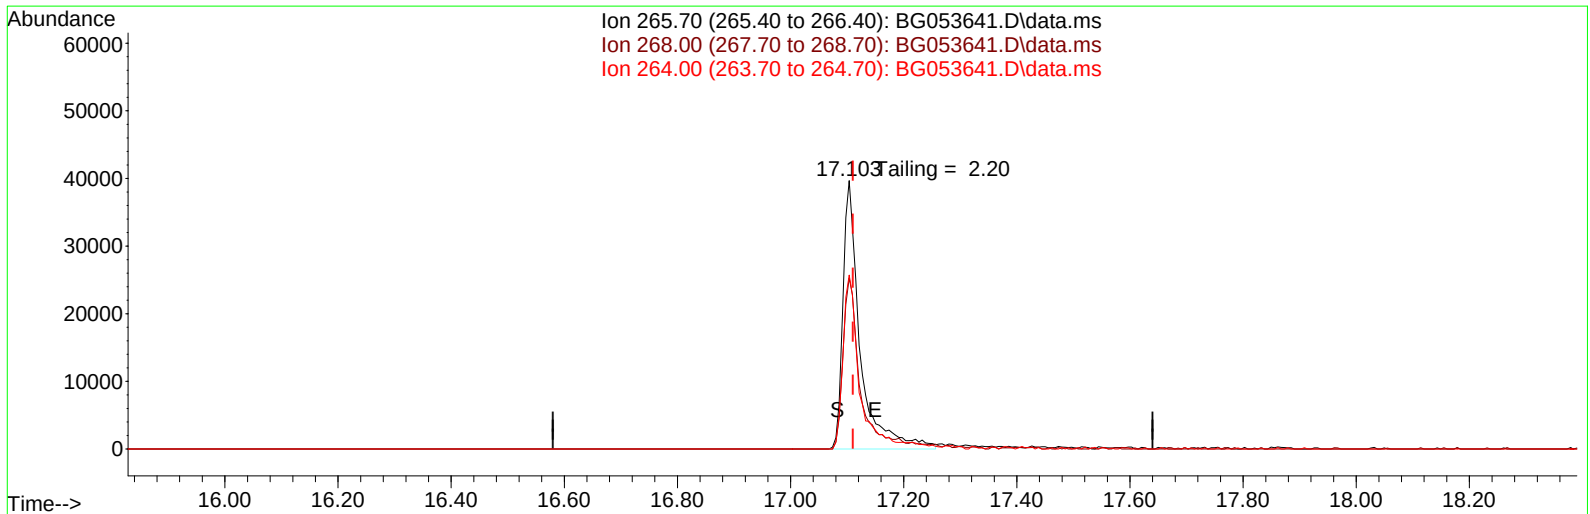

TIC: BG053641.D\data.ms

(70) Pentachlorophenol (C)

17.103min (-0.006) 154739.95 ng




response 81476

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.75
264.00	66.20	64.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052022\
Data File : BG053641.D
Acq On : 20 May 2022 12:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 20 13:29:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 03:55:28 2022
Response via : Initial Calibration

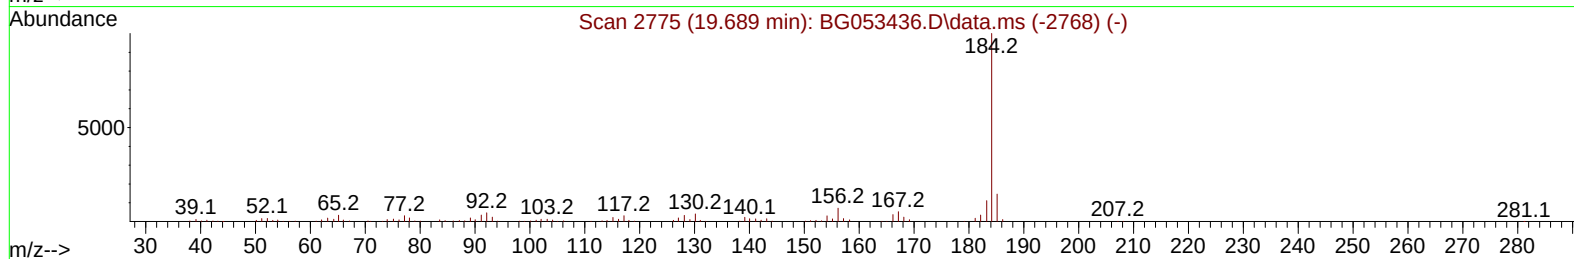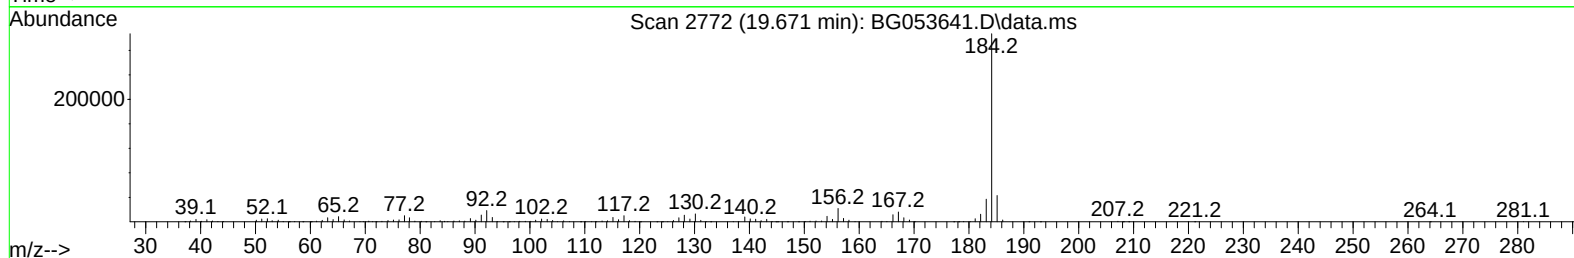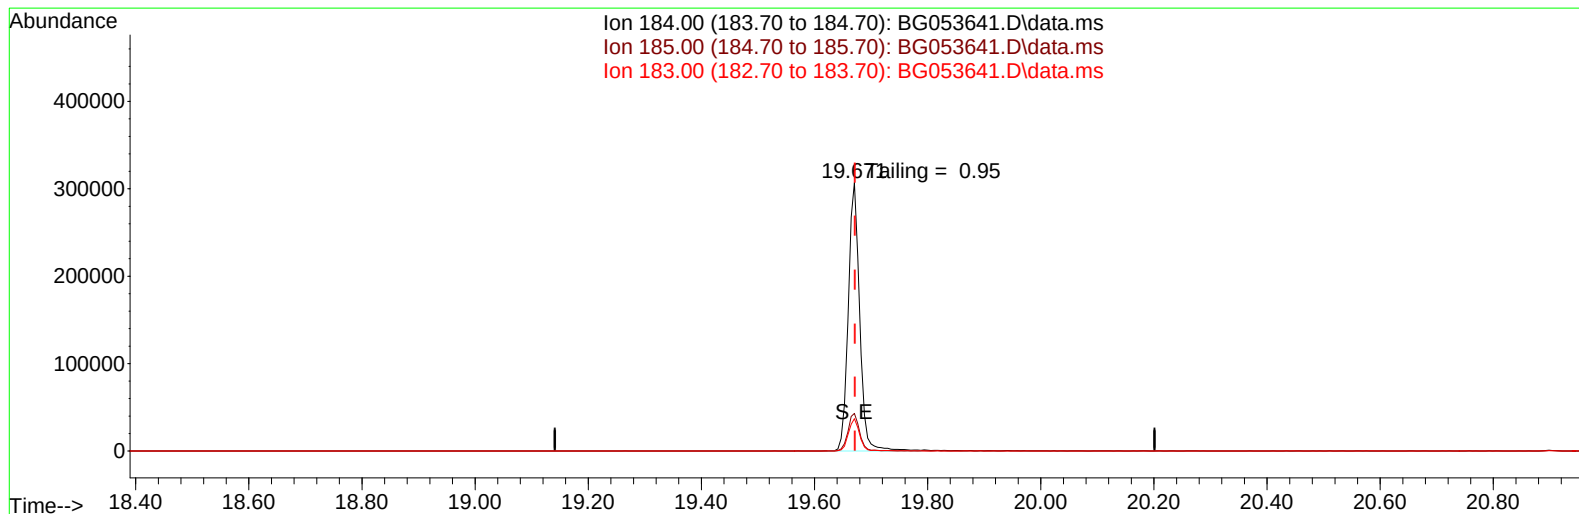

TIC: BG053641.D\data.ms

(77) Benzidine

19.671min (-0.000) 62976.84 ng

response 431648

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.03
183.00	11.10	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/20/2022	BNA_G	<u>BG053641.D</u>
Compound Name	Response	Retention Time
DDT	200542	20.904
DDD	2708	20.511
DDE	64	20.047
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2772	203314	1.36

Instrument :
BNA_G
ClientSampleId :
DFTPP