

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052116\
 Data File : BG021981.D
 Acq On : 21 May 2016 16:35
 Operator : UM/SJ
 Sample : PB90760BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.538	115	119	125	rBV3	7762	12414	1.07%	0.116%
2	3.667	139	141	145	rBV3	968	1242	0.11%	0.012%
3	4.296	246	248	256	rVB4	1860	3566	0.31%	0.033%
4	6.511	621	625	627	rBV3	825	1308	0.11%	0.012%
5	7.310	754	761	775	rBV	124218	251816	21.70%	2.348%
6	7.480	782	790	799	rBV	109430	214494	18.48%	2.000%
7	7.692	818	826	839	rBV	139754	283265	24.41%	2.642%
8	7.933	864	867	869	rBV3	1013	1583	0.14%	0.015%
9	8.162	898	906	917	rBV	88188	181007	15.60%	1.688%
10	8.861	1018	1025	1043	rBV	176472	369863	31.87%	3.449%
11	9.043	1052	1056	1058	rBV4	1091	1723	0.15%	0.016%
12	9.331	1097	1105	1121	rVV	124762	270601	23.32%	2.524%
13	9.448	1123	1125	1130	rVB3	929	1182	0.10%	0.011%
14	9.807	1181	1186	1188	rVB2	835	1413	0.12%	0.013%
15	10.054	1221	1228	1242	rBV2	100790	216342	18.64%	2.018%
16	10.594	1310	1320	1334	rBV	170546	359843	31.01%	3.356%
17	10.982	1376	1386	1400	rBV	161313	328709	28.32%	3.065%
18	11.111	1400	1408	1427	rBV	156200	368588	31.76%	3.437%
19	12.562	1650	1655	1659	rBV3	1998	4267	0.37%	0.040%
20	13.127	1747	1751	1754	rVB	888	1199	0.10%	0.011%
21	14.067	1909	1911	1916	rVB2	899	1486	0.13%	0.014%
22	14.178	1921	1930	1942	rVV	354170	587339	50.61%	5.477%
23	14.261	1942	1944	1947	rVV2	1025	1213	0.10%	0.011%
24	14.478	1974	1981	1996	rBV	465331	820932	70.74%	7.656%
25	14.783	2025	2033	2041	rBV2	256966	457259	39.40%	4.264%
26	14.842	2041	2043	2047	rVB3	1082	1439	0.12%	0.013%
27	14.983	2059	2067	2081	rBV2	66407	186657	16.08%	1.741%
28	15.776	2194	2202	2214	rBV	580227	988041	85.14%	9.214%
29	15.888	2216	2221	2236	rVV	94604	171025	14.74%	1.595%
30	16.006	2237	2241	2249	rVB4	5335	10014	0.86%	0.093%
31	16.346	2295	2299	2302	rBV	768	1324	0.11%	0.012%
32	17.527	2493	2500	2509	rVV	286449	488846	42.12%	4.559%
33	17.627	2509	2517	2532	rVV2	575544	1001013	86.26%	9.335%
34	18.796	2712	2716	2719	rVB3	934	1501	0.13%	0.014%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052116\
Data File : BG021981.D
Acq On : 21 May 2016 16:35
Operator : UM/SJ
Sample : PB90760BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK60

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Title : SVOA CALIBRATION

35	18.931	2735	2739	2743	rBV2	848	1212	0.10%	0.011%
36	19.372	2811	2814	2815	rBV2	1167	1364	0.12%	0.013%
37	19.402	2818	2819	2822	rVV3	1553	1368	0.12%	0.013%
38	19.425	2822	2823	2827	rVV3	1402	1579	0.14%	0.015%
39	19.466	2827	2830	2832	rVV2	1385	1593	0.14%	0.015%
40	19.490	2832	2834	2837	rVV2	1811	1460	0.13%	0.014%
41	19.543	2837	2843	2848	rVV	7326	12210	1.05%	0.114%
42	19.607	2852	2854	2856	rBV2	1648	1220	0.11%	0.011%
43	19.701	2868	2870	2873	rBV3	980	1225	0.11%	0.011%
44	19.801	2881	2887	2891	rVB4	5088	9739	0.84%	0.091%
45	19.907	2898	2905	2917	rBV	743440	1160499	100.00%	10.823%
46	20.036	2925	2927	2932	rVB6	1963	1826	0.16%	0.017%
47	20.083	2933	2935	2938	rVB4	1863	1189	0.10%	0.011%
48	20.277	2964	2968	2969	rBV4	2580	2314	0.20%	0.022%
49	20.371	2982	2984	2986	rBV3	1925	1686	0.15%	0.016%
50	20.406	2986	2990	2991	rBV3	1759	2285	0.20%	0.021%
51	20.483	3001	3003	3004	rBV2	2587	1366	0.12%	0.013%
52	20.571	3015	3018	3019	rBV3	2572	3030	0.26%	0.028%
53	20.747	3046	3048	3051	rBV4	2269	2977	0.26%	0.028%
54	20.959	3082	3084	3086	rBV3	2441	2549	0.22%	0.024%
55	21.810	3222	3229	3248	rBV	255829	533100	45.94%	4.972%
56	24.913	3746	3757	3771	rBV	285161	890200	76.71%	8.302%
57	25.142	3785	3796	3810	rVB	149534	492332	42.42%	4.591%
58	28.532	4371	4373	4374	rBV2	3948	2026	0.17%	0.019%


Sum of corrected areas: 10722863

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052116\
Data File : BG021981.D
Acq On : 21 May 2016 16:35
Operator : UM/SJ
Sample : PB90760BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK60

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

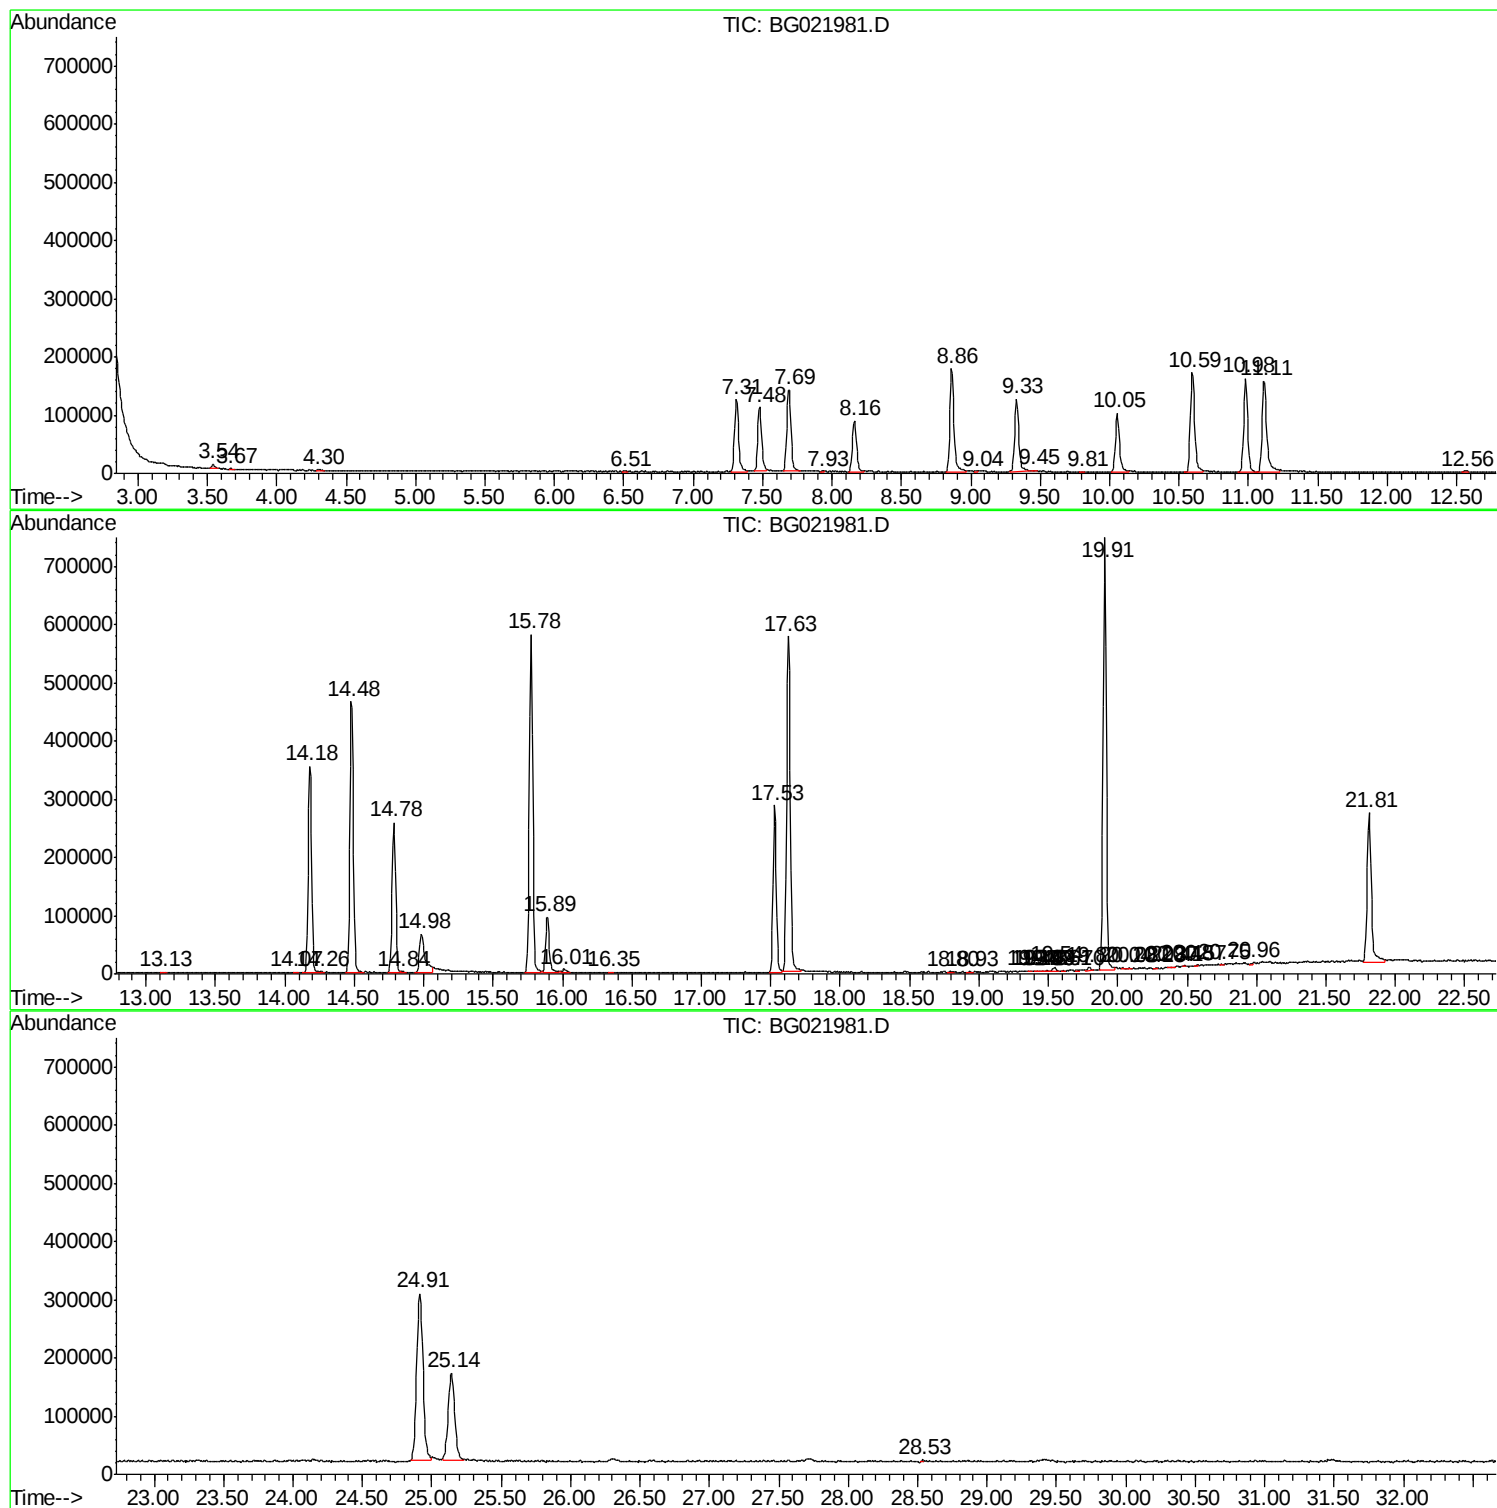

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052116\
Data File : BG021981.D
Acq On : 21 May 2016 16:35
Operator : UM/SJ
Sample : PB90760BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK60

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052116\
Data File : BG021981.D
Acq On : 21 May 2016 16:35
Operator : UM/SJ
Sample : PB90760BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK60

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc