
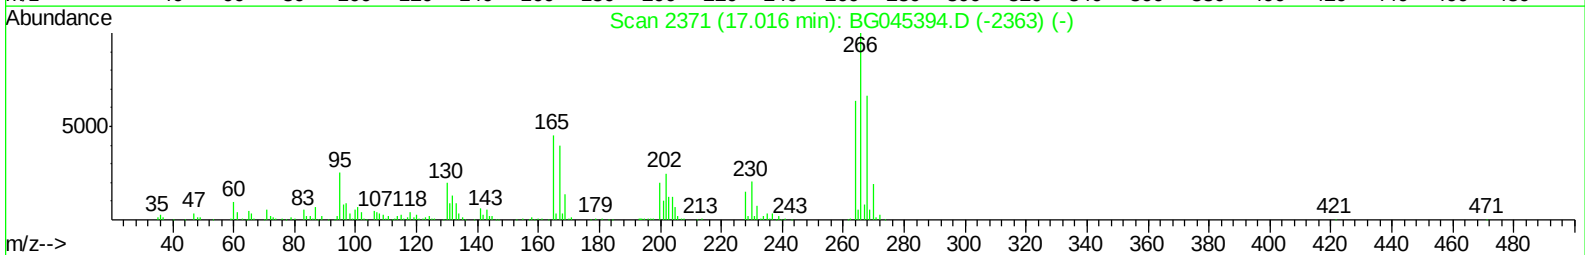
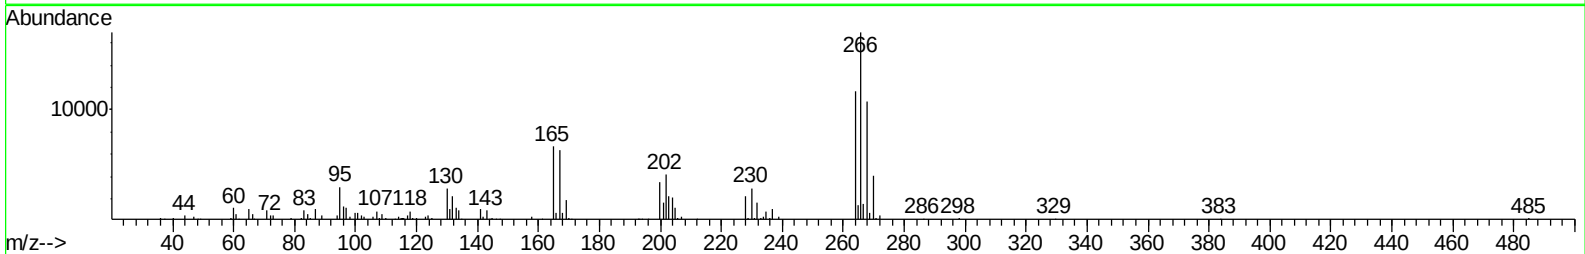


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG052120\
Data File : BG045437.D
Acq On : 21 May 2020 12:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 01:19:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 20 14:43:36 2020
Response via : Initial Calibration

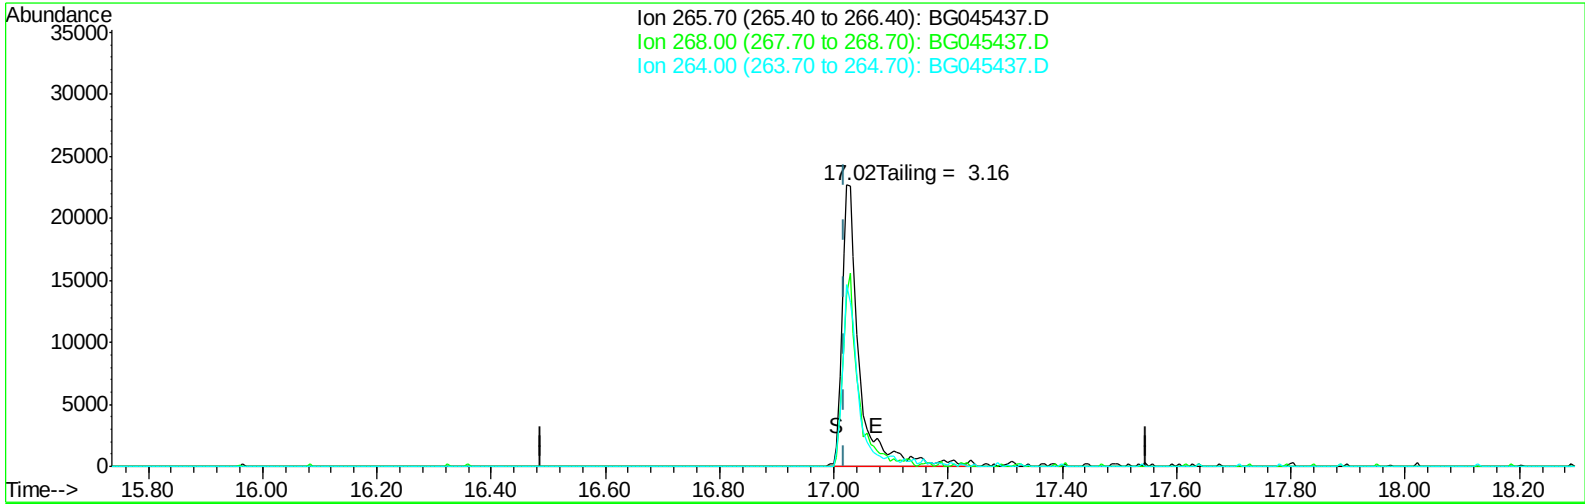

TIC: BG045437.D

(70) Pentachlorophenol (C)




17.022min (+0.004) 19756.87ng

response 43569

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	60.72
264.00	63.70	64.37
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG052120\
 Data File : BG045437.D
 Acq On : 21 May 2020 12:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 01:19:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 20 14:43:36 2020
 Response via : Initial Calibration

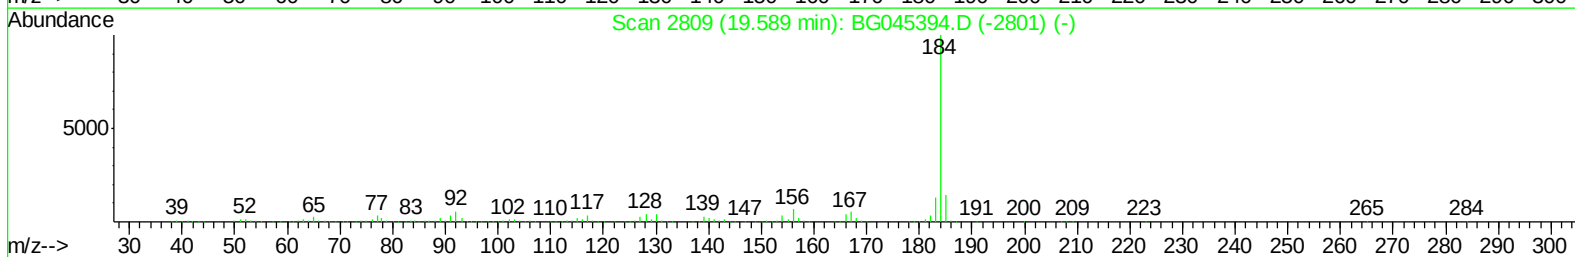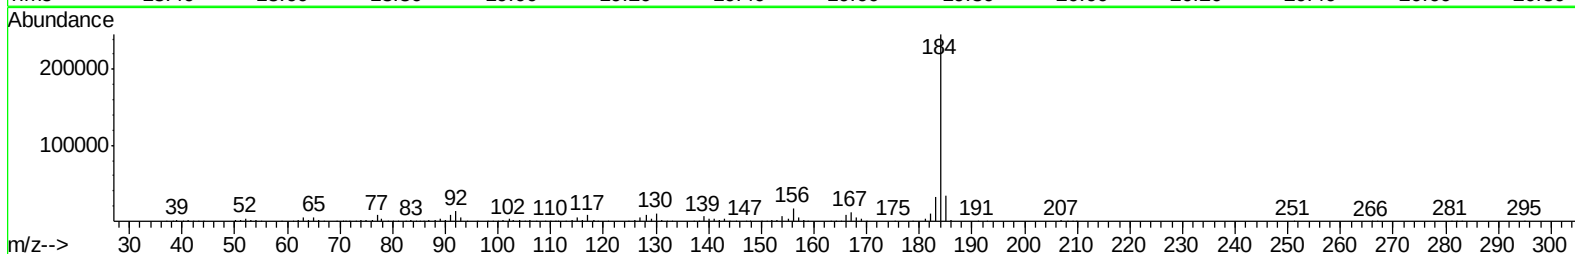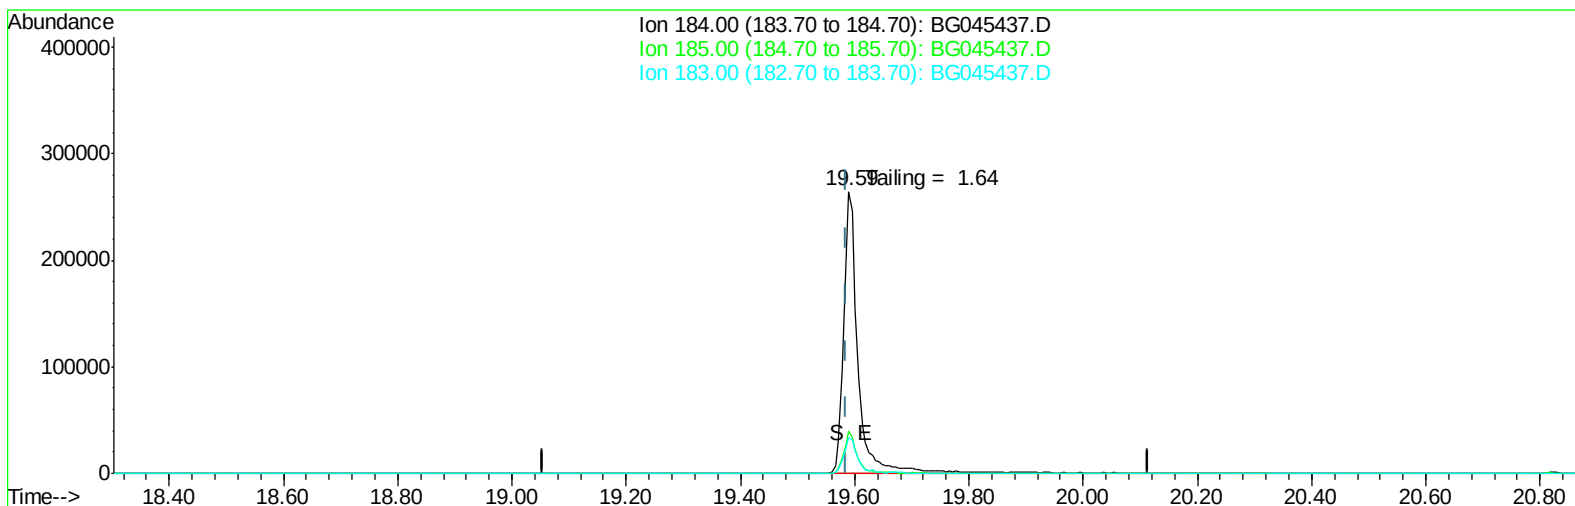

TIC: BG045437.D

(77) Benzidine

19.590min (+0.004) 301237.55ng m

response 482243

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	14.87
183.00	12.80	12.61
0.00	0.00	0.00