


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG052120\
 Data File : BG045437.D
 Acq On : 21 May 2020 12:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 20 14:43:36 2020

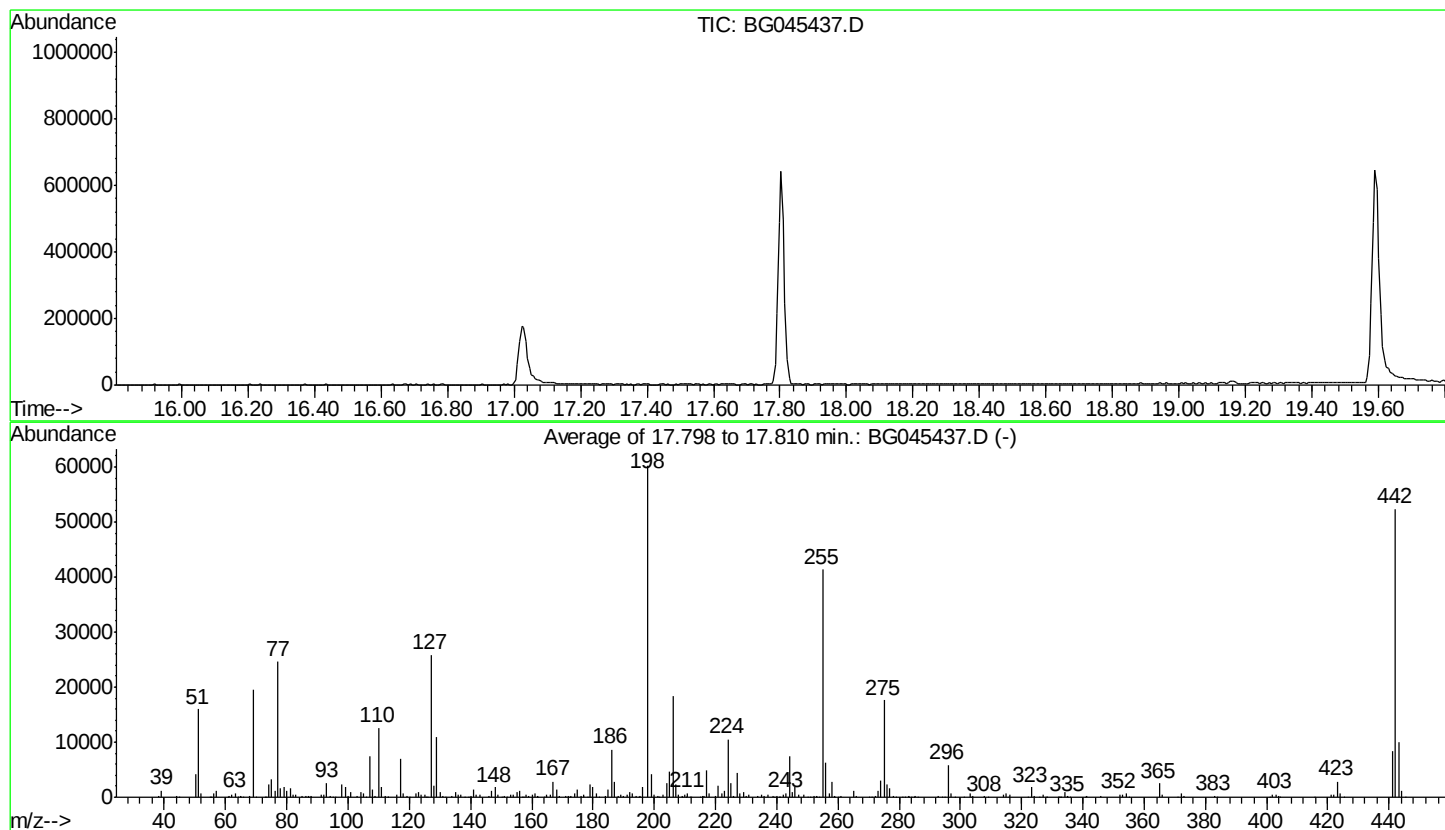

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	15991	PASS
68	69	0.00	2	1.5	294	PASS
69	198	0.00	100	32.5	19587	PASS
70	69	0.00	2	0.5	91	PASS
127	198	10	80	42.9	25869	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60232	PASS
199	198	5	9	6.8	4099	PASS
275	198	10	60	29.2	17564	PASS
365	198	1	100	4.2	2542	PASS
441	198	0.01	100	13.9	8367	PASS
442	198	50	100	87.1	52437	PASS
443	442	15	24	19.3	10095	PASS