


Data Path : Z:\HPCHEM1\BNA_G\Data\BG052215\
 Data File : BG017241.D
 Acq On : 22 May 2015 10:39
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 16:12:13 2015

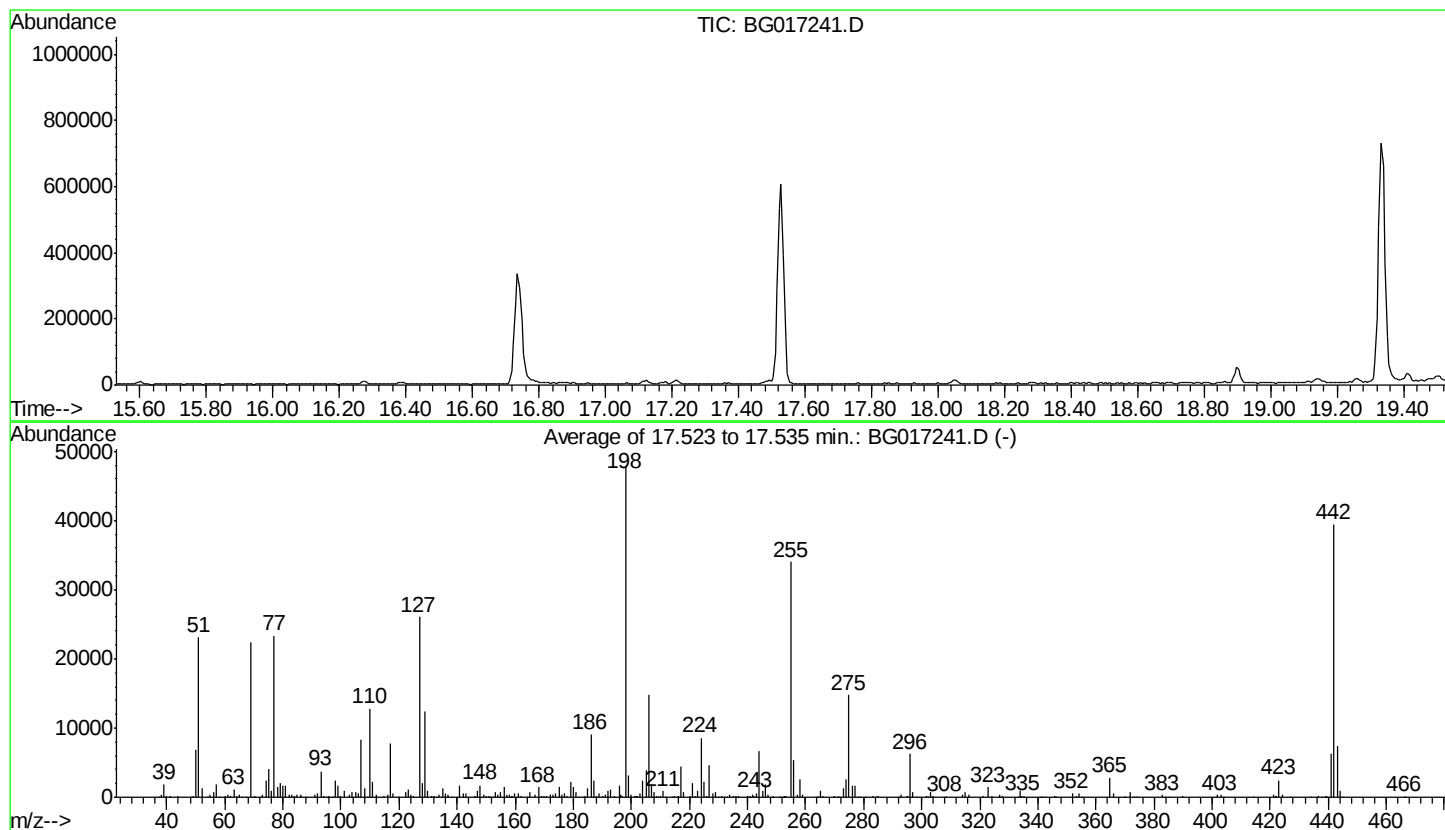

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	23096	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.7	22353	PASS
70	69	0.00	2	0.5	117	PASS
127	198	10	80	54.3	26008	PASS
197	198	0.00	2	0.3	151	PASS
198	198	100	100	100.0	47914	PASS
199	198	5	9	6.7	3214	PASS
275	198	10	60	30.8	14779	PASS
365	198	1	100	5.8	2798	PASS
441	442	0.01	24	15.8	6239	PASS
442	198	50	100	82.2	39378	PASS
443	442	15	24	18.9	7444	PASS