
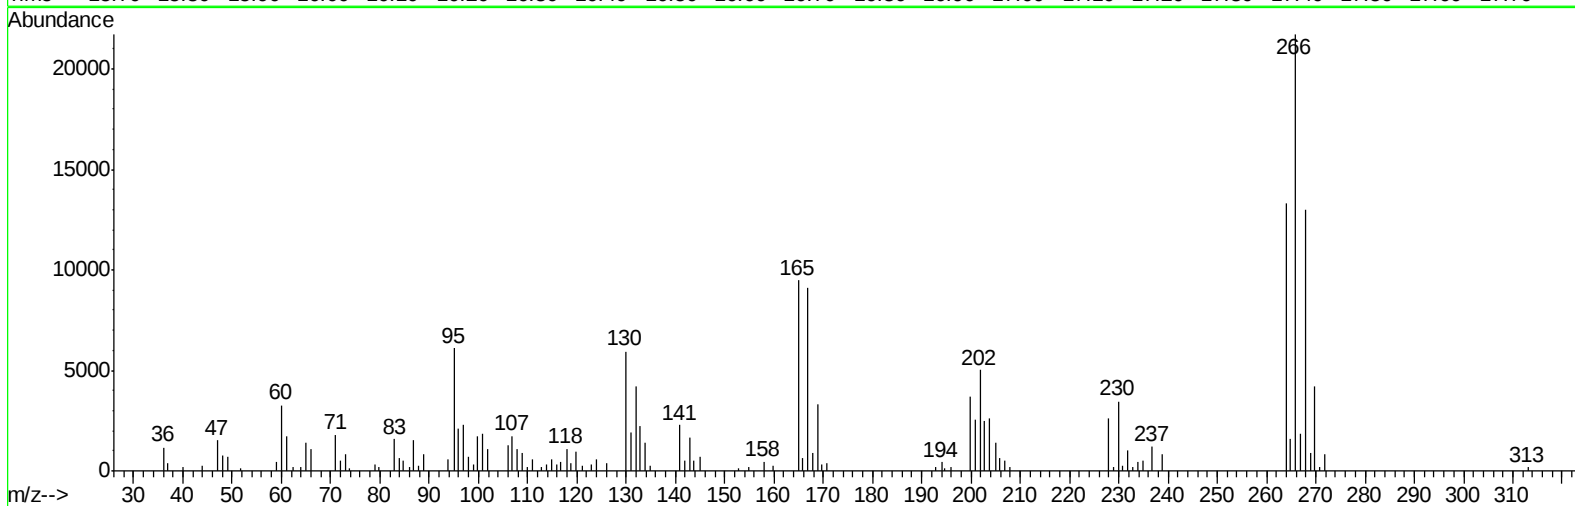


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
Data File : BG017257.D
Acq On : 22 May 2015 23:52
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 01:35:26 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

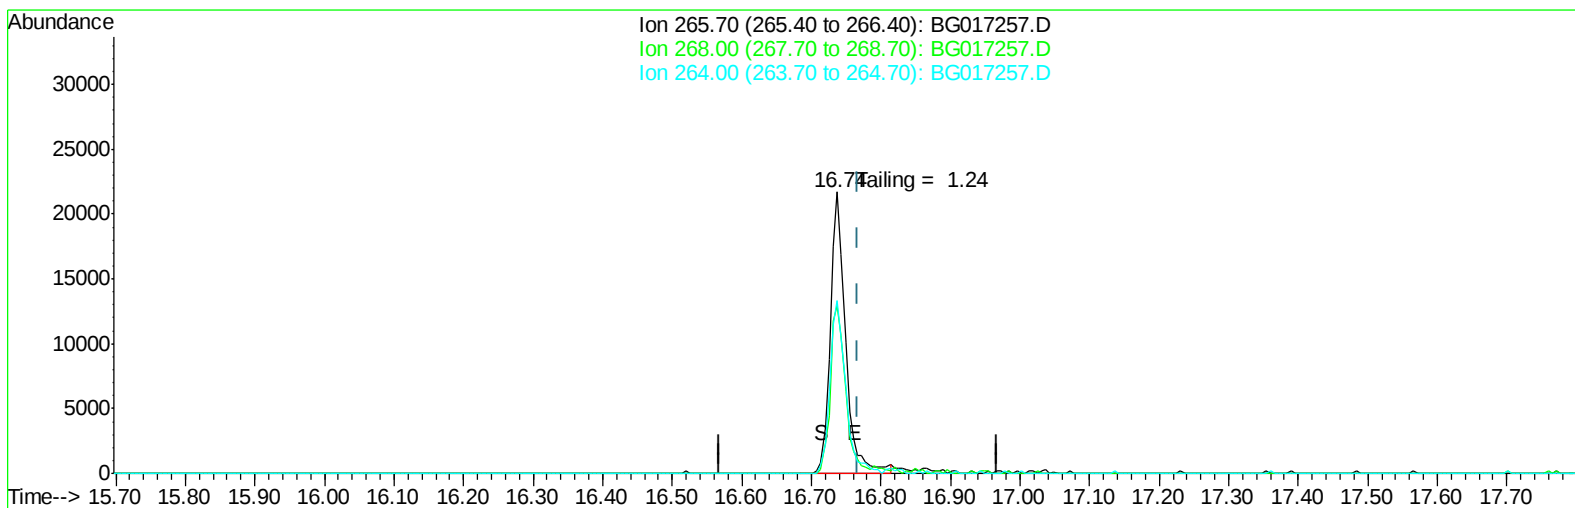

TIC: BG017257.D

(69) Pentachlorophenol (C)



16.737min (-0.031) 2586.16ng

response 32664

Ion	Exp%	Act%
265.70	100	100
268.00	70.70	59.74
264.00	61.70	61.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
Data File : BG017257.D
Acq On : 22 May 2015 23:52
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 01:35:26 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

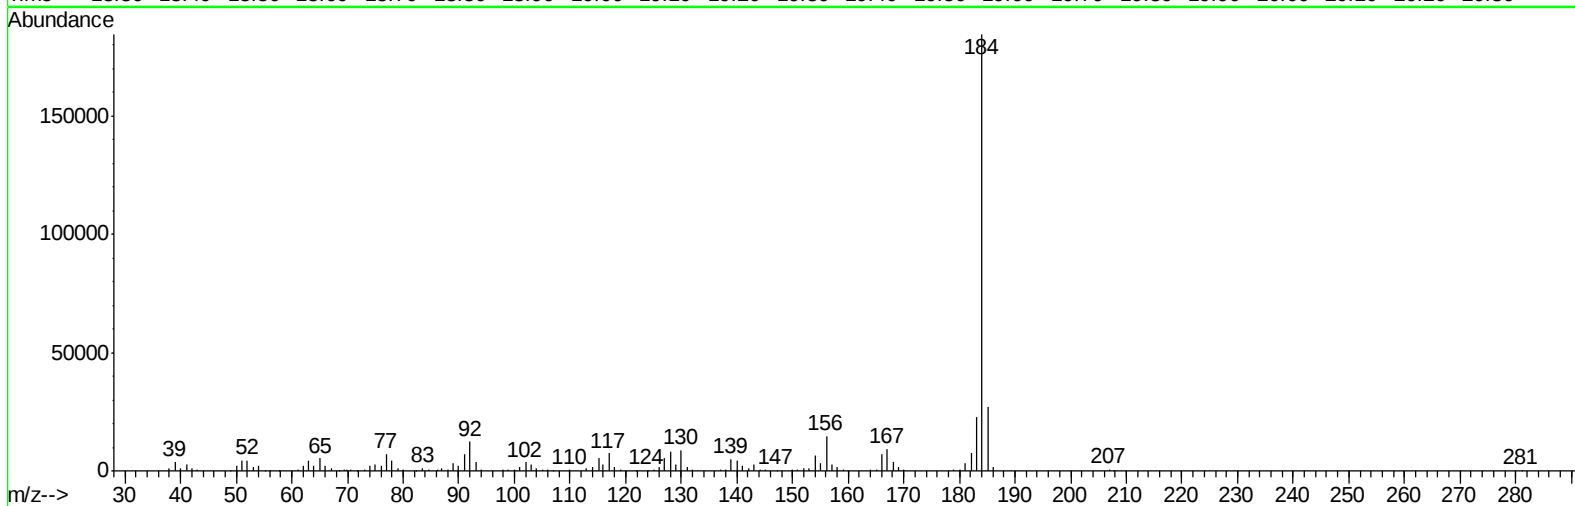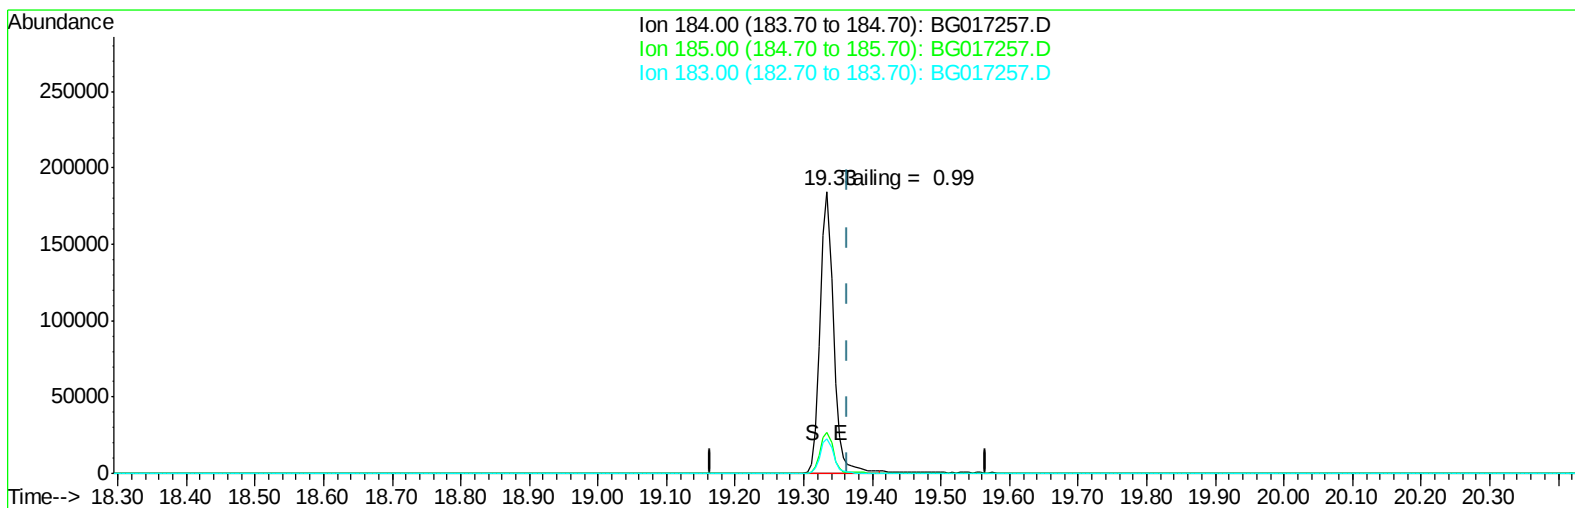

TIC: BG017257.D

(76) Benzidine

19.334min (-0.031) 134096.22ng

response 249558

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.73
183.00	14.30	12.31
0.00	0.00	0.00