

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
 Data File : BG017265.D
 Acq On : 23 May 2015 4:29
 Operator : TP/IZ
 Sample : G2357-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-H2O-05

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.767	9	13	23	rVV2	46959	95581	1.37%	0.269%
2	2.856	23	28	44	rVB	274468	445574	6.38%	1.256%
3	4.806	351	360	367	rBV	485390	716613	10.26%	2.020%
4	5.306	434	445	452	rBV	619735	1096482	15.70%	3.091%
5	5.582	487	492	500	rVB	94336	167128	2.39%	0.471%
6	5.746	508	520	523	rBV	2215002	3862756	55.30%	10.890%
7	5.805	523	530	534	rVB	3377010	6985299	100.00%	19.693%
8	6.898	710	716	725	rBV	764392	1164458	16.67%	3.283%
9	7.145	753	758	764	rVB	276726	368436	5.27%	1.039%
10	7.233	764	773	781	rVV	833285	1382987	19.80%	3.899%
11	7.309	781	786	796	rVB3	41301	82871	1.19%	0.234%
12	7.685	841	850	856	rVB2	150771	338532	4.85%	0.954%
13	7.756	856	862	871	rBV2	564974	1207565	17.29%	3.404%
14	7.850	871	878	887	rVV3	297717	820154	11.74%	2.312%
15	7.938	887	893	896	rVV	109573	170983	2.45%	0.482%
16	8.002	896	904	910	rVV2	561336	1079114	15.45%	3.042%
17	8.226	937	942	952	rVB3	56281	95752	1.37%	0.270%
18	8.320	952	958	964	rBV	130829	226224	3.24%	0.638%
19	8.425	971	976	980	rBV	93845	140222	2.01%	0.395%
20	8.519	980	992	999	rVV4	112131	384669	5.51%	1.084%
21	8.631	1006	1011	1015	rBV	86682	140264	2.01%	0.395%
22	8.684	1015	1020	1026	rVB2	78228	136791	1.96%	0.386%
23	8.784	1032	1037	1041	rBV	136050	208205	2.98%	0.587%
24	8.848	1041	1048	1059	rVB	485612	842142	12.06%	2.374%
25	9.119	1076	1094	1096	rBV4	235314	857831	12.28%	2.418%
26	9.242	1105	1115	1119	rVB2	167956	410352	5.87%	1.157%
27	9.307	1119	1126	1129	rVV	77064	121558	1.74%	0.343%
28	9.366	1129	1136	1141	rVV2	162108	312653	4.48%	0.881%
29	9.454	1141	1151	1155	rVV4	172405	449375	6.43%	1.267%
30	9.724	1192	1197	1205	rVB	62051	105779	1.51%	0.298%
31	9.877	1216	1223	1231	rVB2	166639	307214	4.40%	0.866%
32	10.470	1317	1324	1329	rBV	229351	422290	6.05%	1.191%
33	10.523	1329	1333	1339	rVB	360534	561470	8.04%	1.583%
34	10.652	1346	1355	1358	rBV7	42392	107997	1.55%	0.304%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
Data File : BG017265.D
Acq On : 23 May 2015 4:29
Operator : TP/IZ
Sample : G2357-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-H2O-05

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.693	1358	1362	1370	rVB4	43234	81803	1.17%	0.231%
36	11.316	1463	1468	1474	rVB5	37564	74258	1.06%	0.209%
37	12.955	1740	1747	1754	rBV	1091222	1611172	23.07%	4.542%
38	14.336	1976	1982	1990	rVB2	267694	402997	5.77%	1.136%
39	14.724	2040	2048	2055	rBV	130998	183616	2.63%	0.518%
40	15.165	2118	2123	2128	rVB	76020	102899	1.47%	0.290%
41	15.829	2230	2236	2251	rBV2	246407	393234	5.63%	1.109%
42	17.080	2444	2449	2458	rVB2	342723	475094	6.80%	1.339%
43	19.348	2828	2835	2842	rBV	2307854	3286451	47.05%	9.265%
44	19.712	2891	2897	2904	rBV	1357359	1660701	23.77%	4.682%
45	19.965	2935	2940	2948	rBV	147639	189091	2.71%	0.533%
46	20.458	3020	3024	3029	rVB	82823	105546	1.51%	0.298%
47	21.263	3156	3161	3168	rBV	436800	570194	8.16%	1.607%
48	23.514	3538	3544	3555	rVB2	269580	518783	7.43%	1.463%


Sum of corrected areas: 35471160

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
Data File : BG017265.D
Acq On : 23 May 2015 4:29
Operator : TP/IZ
Sample : G2357-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-H2O-05

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

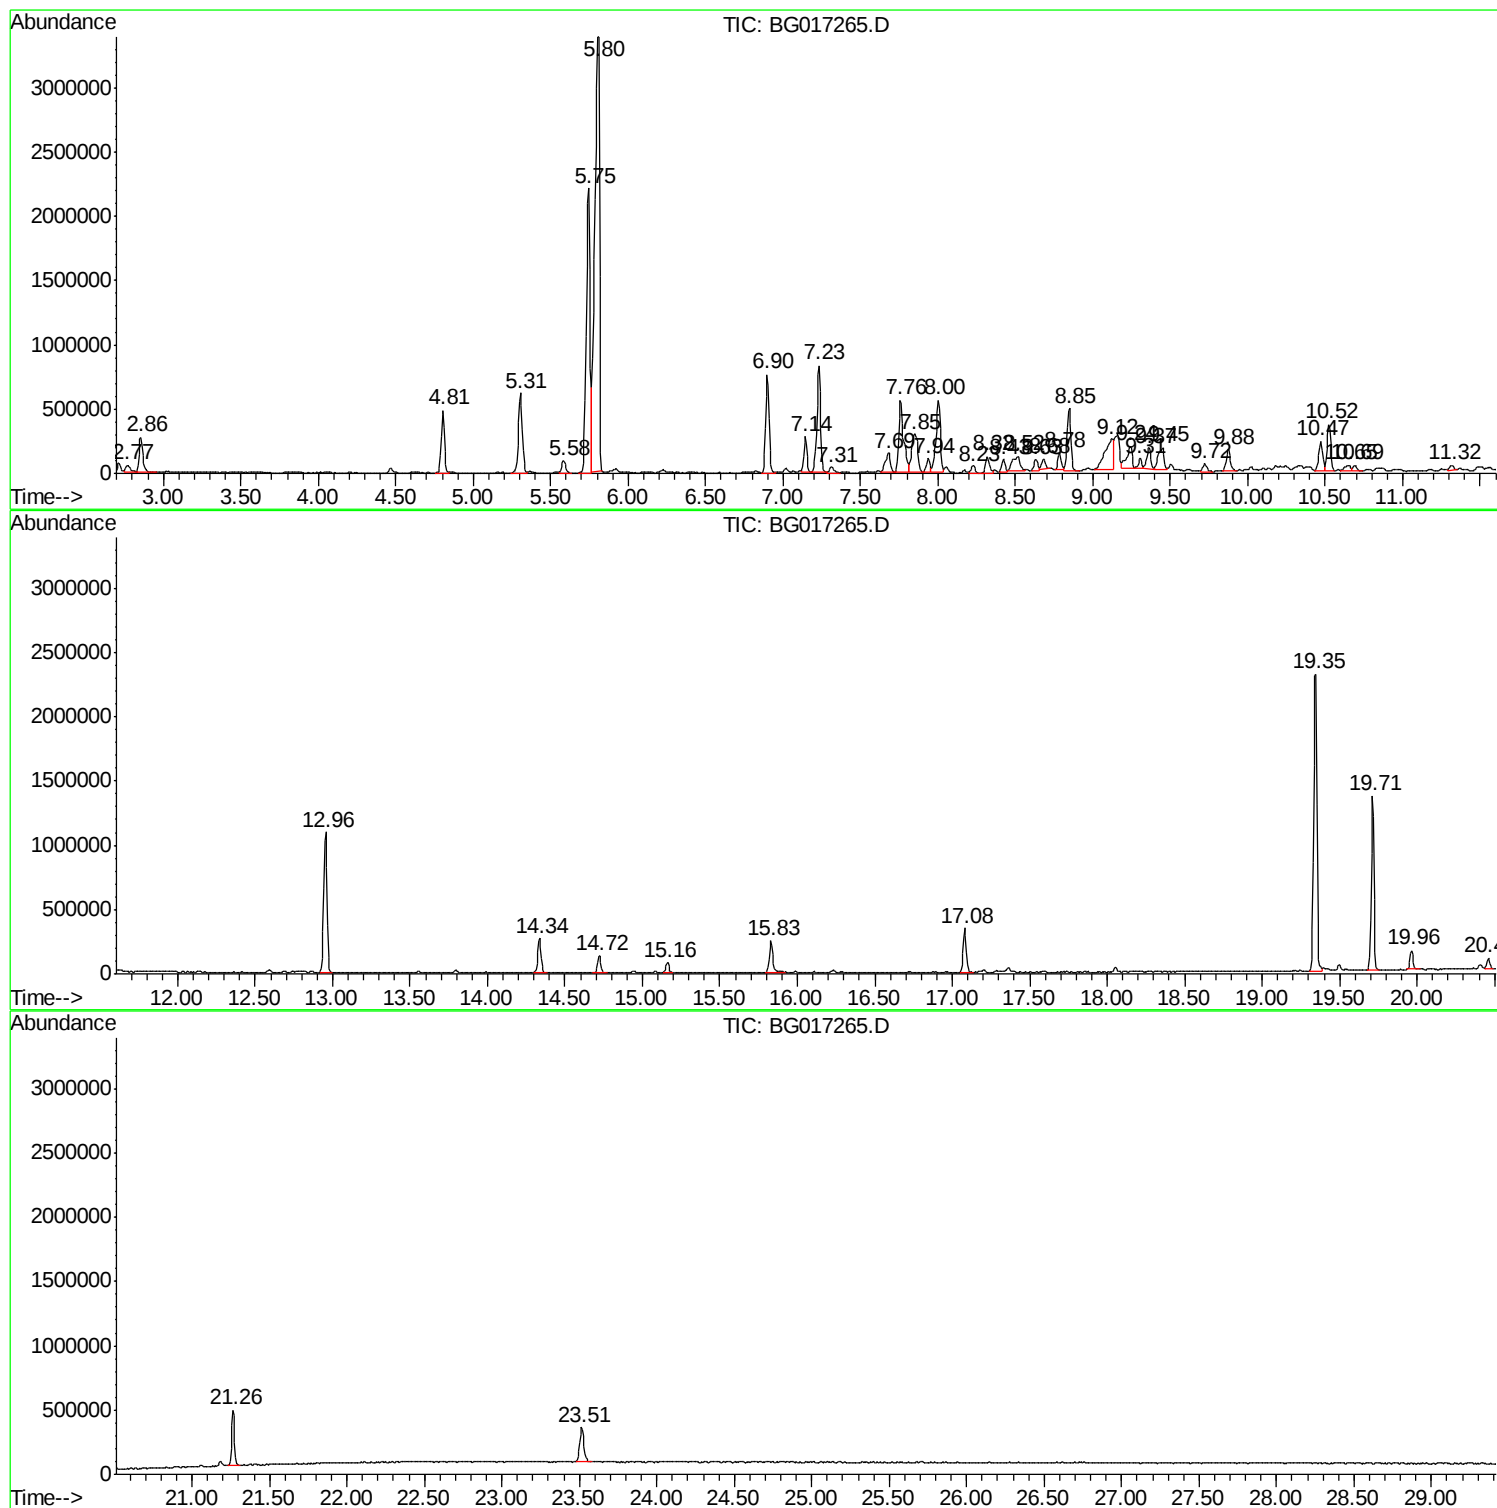

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
Data File : BG017265.D
Acq On : 23 May 2015 4:29
Operator : TP/IZ
Sample : G2357-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-H2O-05

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
Data File : BG017265.D
Acq On : 23 May 2015 4:29
Operator : TP/IZ
Sample : G2357-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-H2O-05

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc