

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
 Data File : BG017267.D
 Acq On : 23 May 2015 5:38
 Operator : TP/IZ
 Sample : G2355-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FRACTANKSAMPLE1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.772	9	14	20	rBV	52101	105545	4.34%	0.814%
2	2.854	23	28	38	rVB	312898	470219	19.32%	3.627%
3	3.818	179	192	197	rBV3	25831	54177	2.23%	0.418%
4	4.047	226	231	240	rBV2	18120	36356	1.49%	0.280%
5	4.799	354	359	366	rVB	142440	195590	8.04%	1.509%
6	5.205	420	428	434	rBV3	17336	37433	1.54%	0.289%
7	5.287	434	442	450	rVV	700923	992305	40.77%	7.655%
8	6.891	709	715	727	rBV	676781	1038943	42.68%	8.014%
9	7.226	764	772	781	rBV	740973	1146544	47.10%	8.845%
10	7.684	841	850	856	rBV	132322	209348	8.60%	1.615%
11	8.001	896	904	913	rVB	547208	847107	34.80%	6.535%
12	8.448	975	980	986	rBV5	14135	31042	1.28%	0.239%
13	8.842	1039	1047	1055	rBV	452621	734165	30.16%	5.663%
14	9.006	1067	1075	1080	rBV3	10515	25632	1.05%	0.198%
15	9.106	1087	1092	1100	rVB4	19712	41578	1.71%	0.321%
16	9.253	1110	1117	1122	rBV3	21522	41949	1.72%	0.324%
17	9.329	1122	1130	1139	rVB5	21740	53801	2.21%	0.415%
18	9.829	1207	1215	1224	rBV7	11149	30233	1.24%	0.233%
19	10.475	1317	1325	1331	rBV	166641	275318	11.31%	2.124%
20	12.954	1739	1747	1759	rBV	1022109	1512960	62.15%	11.671%
21	13.759	1877	1884	1891	rBV2	21678	33014	1.36%	0.255%
22	14.335	1974	1982	1990	rBV2	237624	355402	14.60%	2.742%
23	15.828	2229	2236	2249	rBV	551805	795236	32.67%	6.135%
24	17.079	2443	2449	2458	rBV	307897	429027	17.62%	3.310%
25	18.048	2610	2614	2618	rBV	34396	46373	1.91%	0.358%
26	19.711	2890	2897	2903	rBV	1991775	2434201	100.00%	18.778%
27	21.262	3156	3161	3166	rBV	397055	514905	21.15%	3.972%
28	23.513	3538	3544	3554	rBV2	251781	474914	19.51%	3.664%


Sum of corrected areas: 12963317

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
Data File : BG017267.D
Acq On : 23 May 2015 5:38
Operator : TP/IZ
Sample : G2355-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FRACTANKSAMPLE1

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

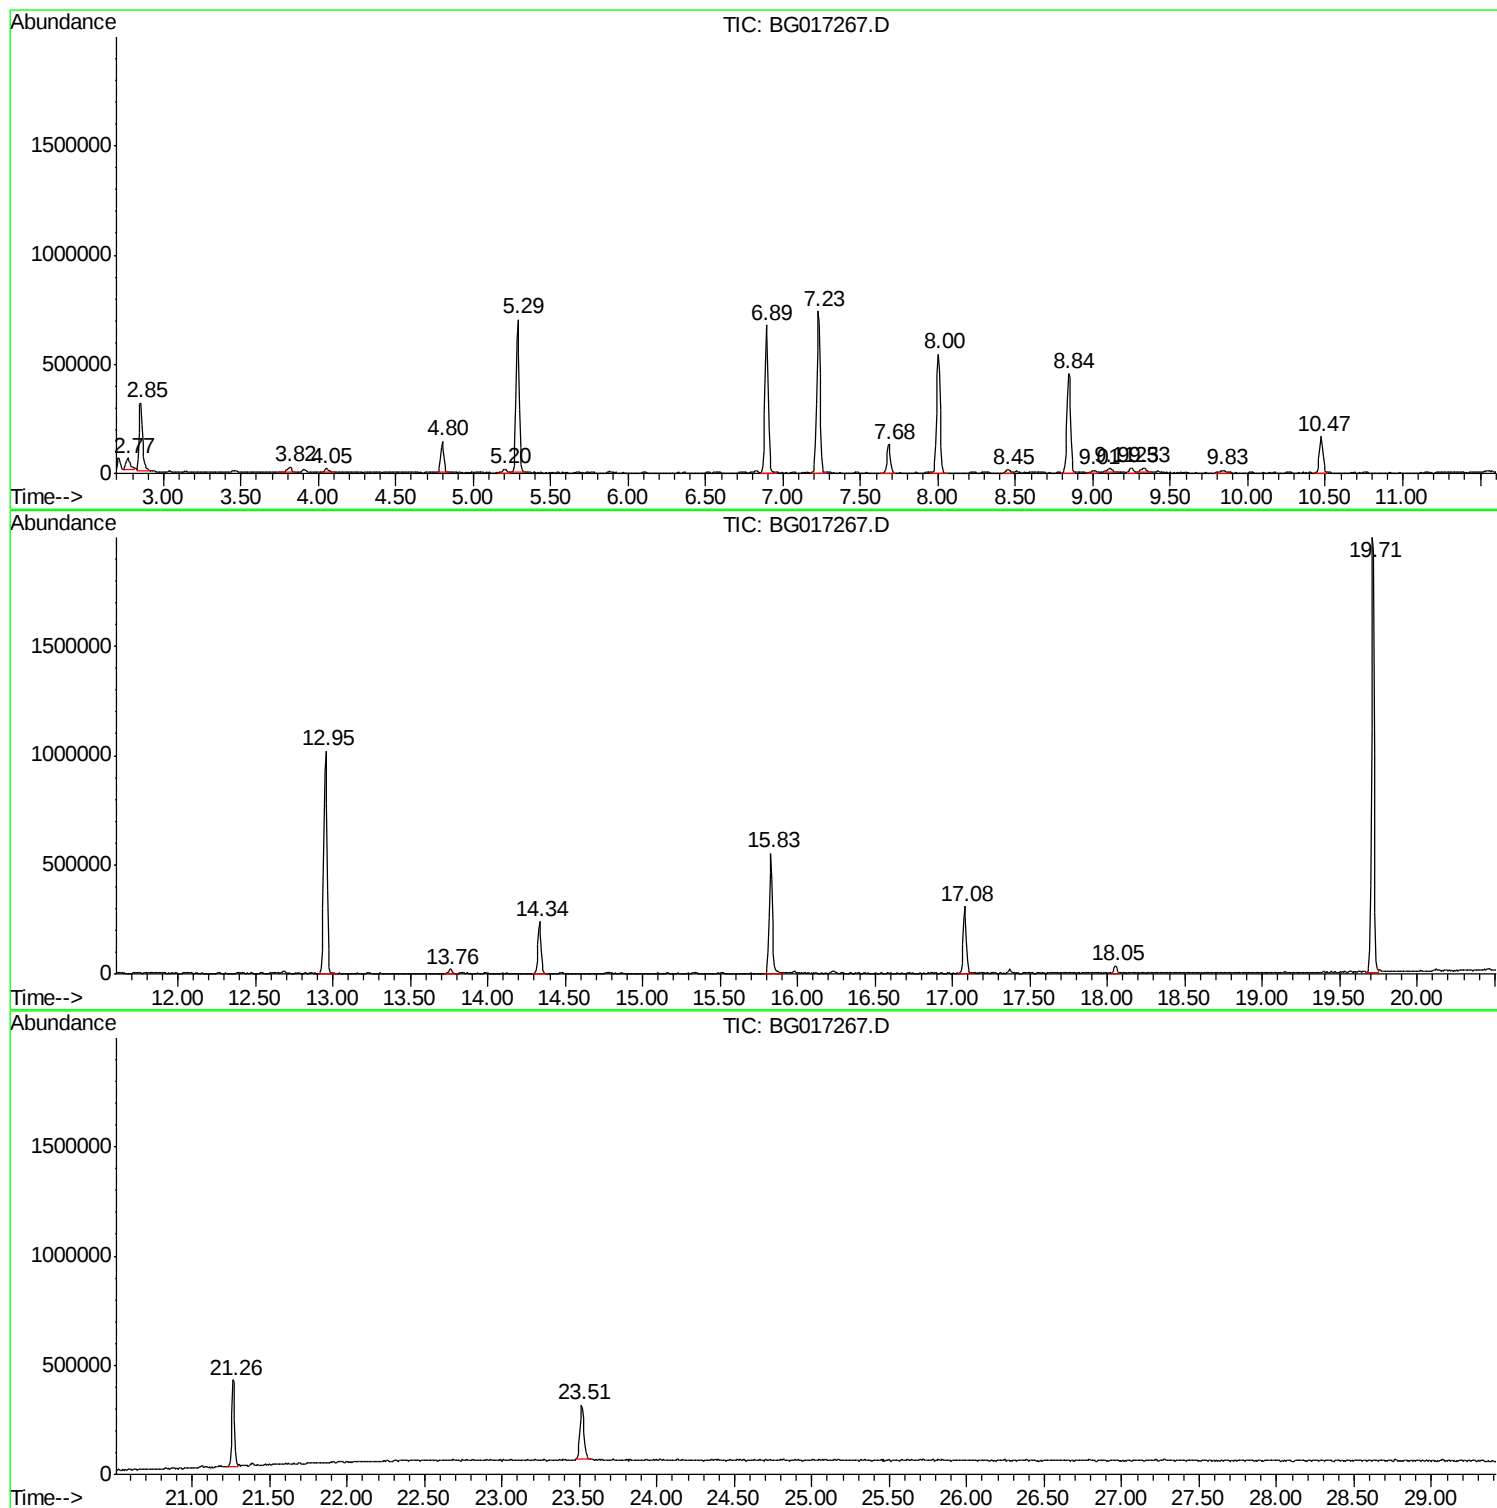

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
Data File : BG017267.D
Acq On : 23 May 2015 5:38
Operator : TP/IZ
Sample : G2355-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FRACTANKSAMPLE1

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
Data File : BG017267.D
Acq On : 23 May 2015 5:38
Operator : TP/IZ
Sample : G2355-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FRACTANKSAMPLE1

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc