


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052215\
 Data File : BG017257.D
 Acq On : 22 May 2015 23:52
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 23 00:52:32 2015

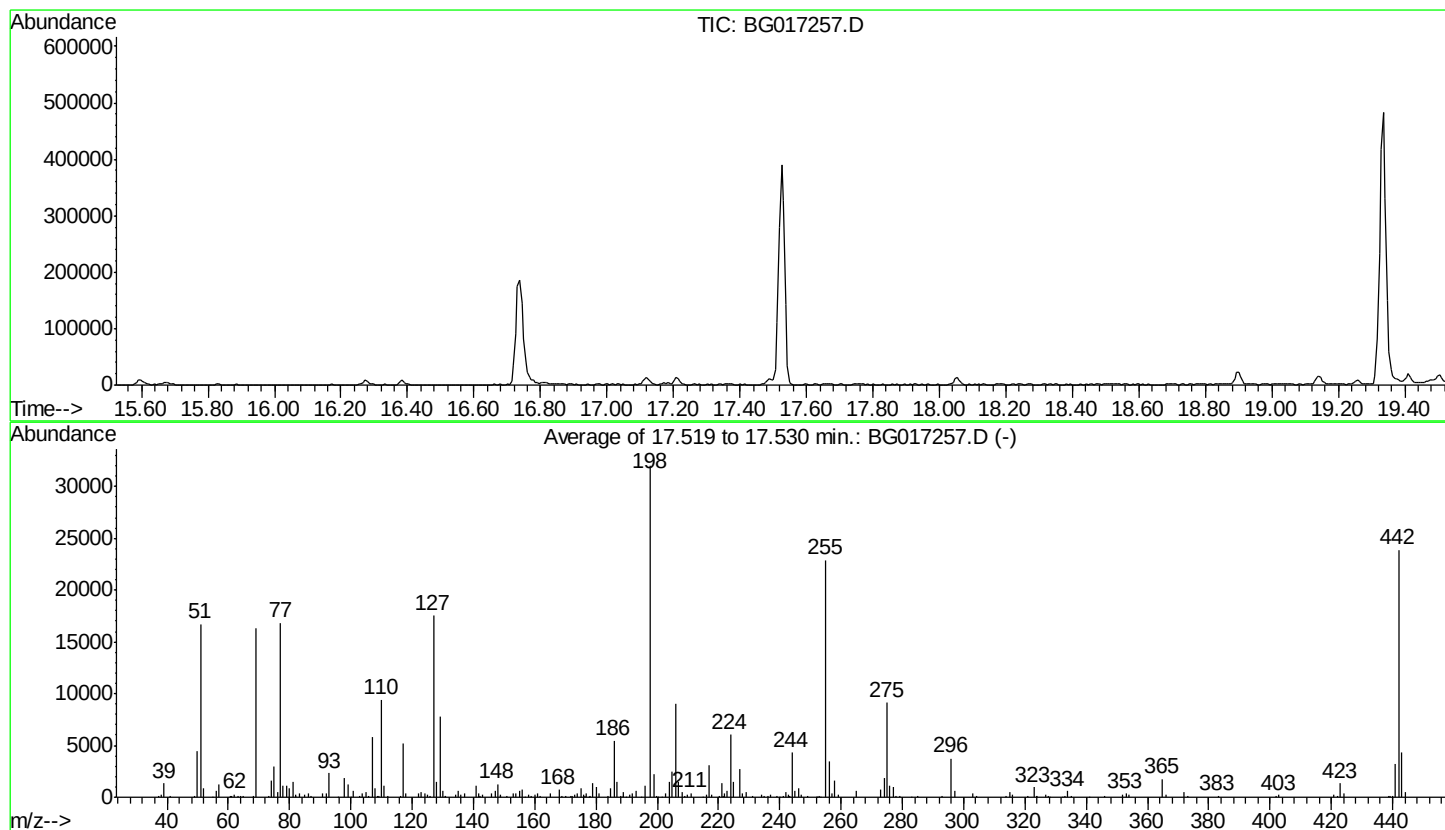

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	16750	PASS
68	69	0.00	2	0.6	101	PASS
69	198	0.00	100	51.1	16352	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.7	17526	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32018	PASS
199	198	5	9	7.1	2284	PASS
275	198	10	60	28.5	9141	PASS
365	198	1	100	5.4	1737	PASS
441	442	0.01	24	13.6	3248	PASS
442	198	50	100	74.5	23864	PASS
443	442	15	24	18.2	4353	PASS