
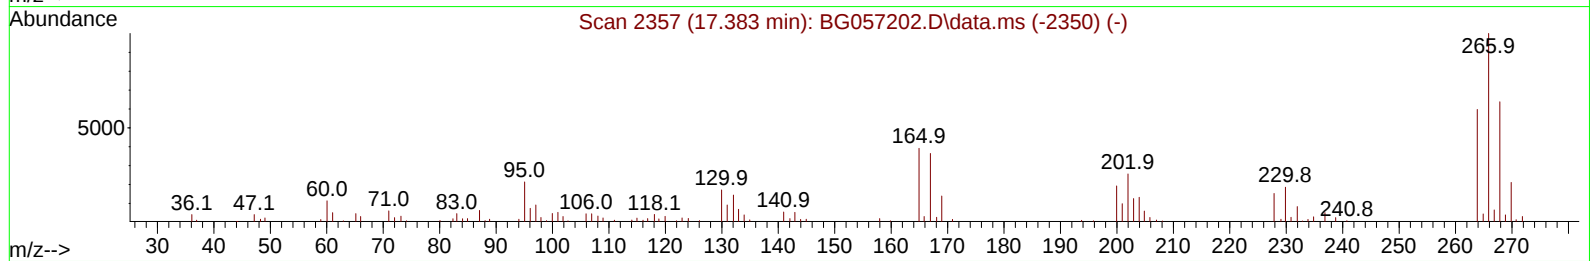
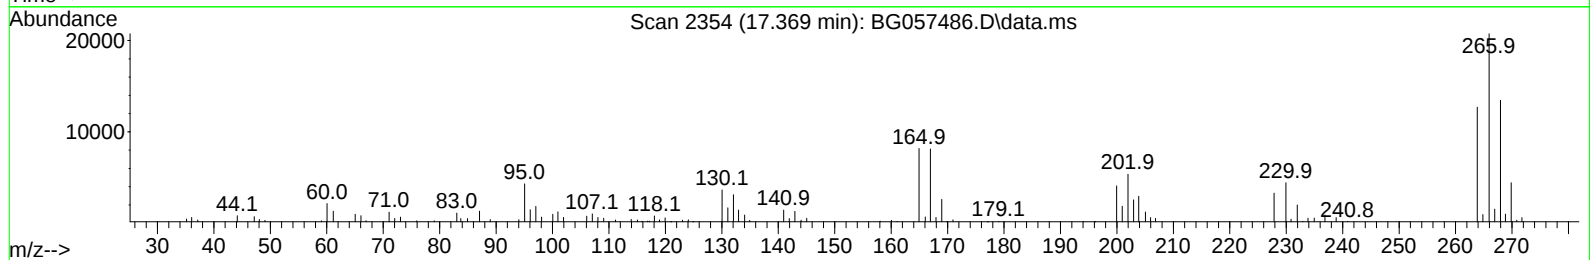


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052223\  
Data File : BG057486.D  
Acq On : 22 May 2023 9:42  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 11:55:14 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG042723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat May 20 04:19:55 2023  
Response via : Initial Calibration

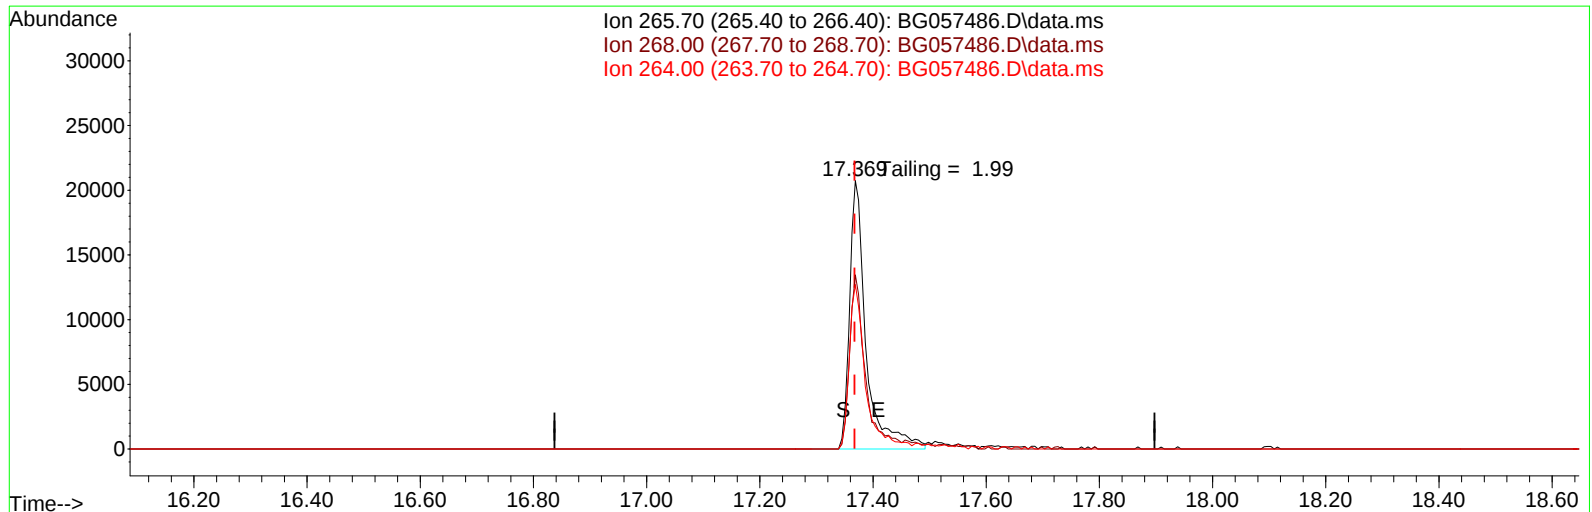

TIC: BG057486.D\data.ms

**(70) Pentachlorophenol (C)**




17.369min (+ 0.001) 23898.08 ng

response 42317

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 64.85  |
| 264.00 | 59.70  | 61.22  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052223\  
Data File : BG057486.D  
Acq On : 22 May 2023 9:42  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 11:55:14 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG042723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat May 20 04:19:55 2023  
Response via : Initial Calibration

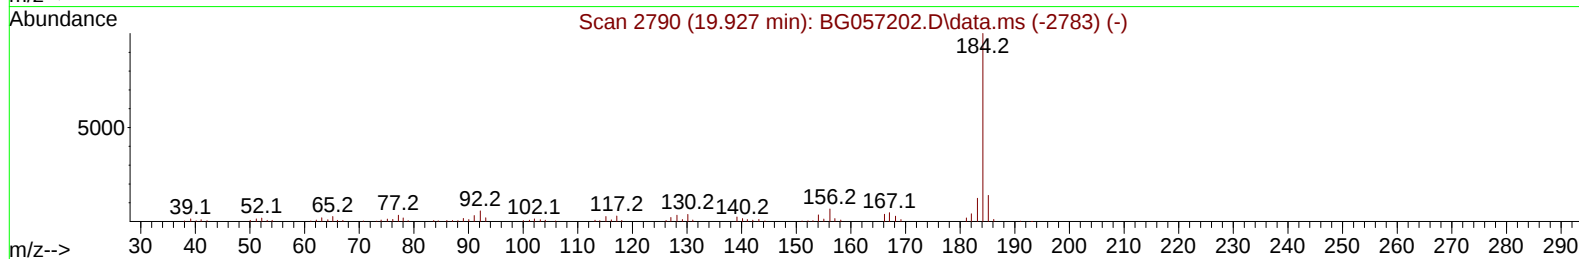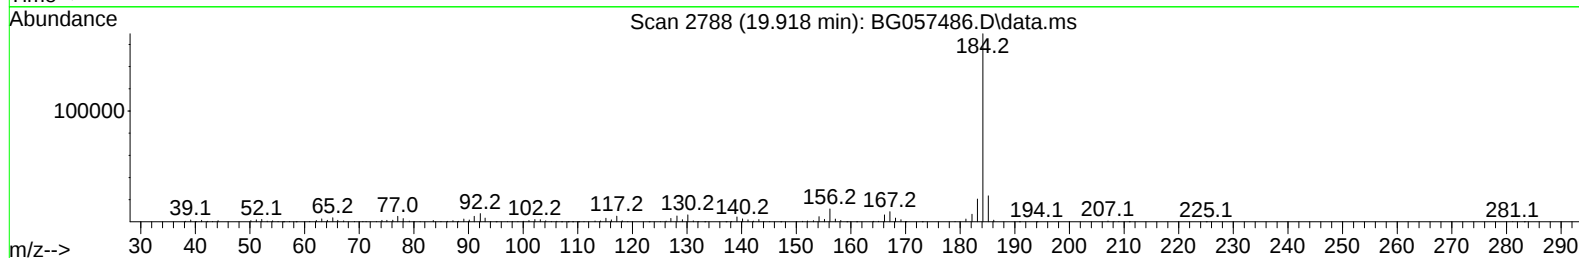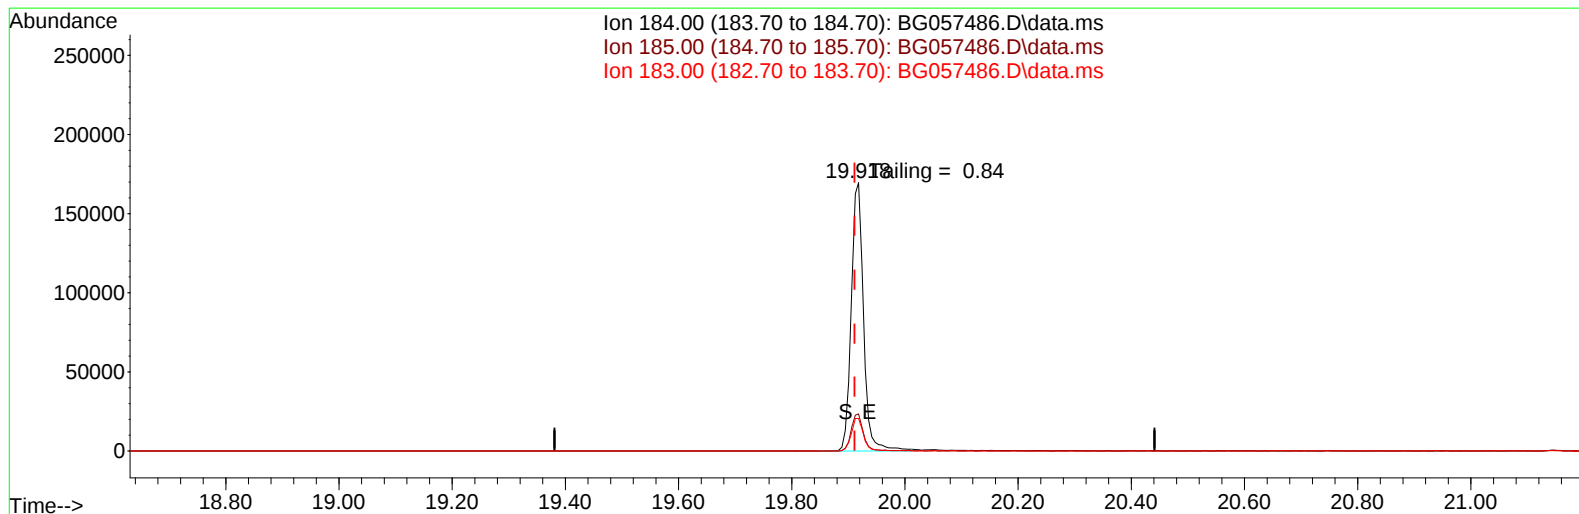

TIC: BG057486.D\data.ms

**(77) Benzidine****19.918min (+ 0.007) 0.00 ng****response 256447**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 13.84  |
| 183.00 | 12.40  | 12.13  |
| 0.00   | 0.00   | 0.00   |