
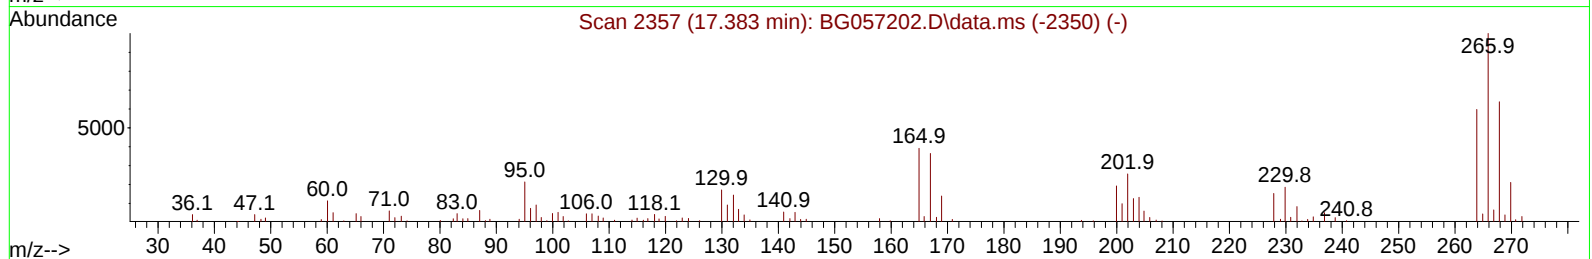
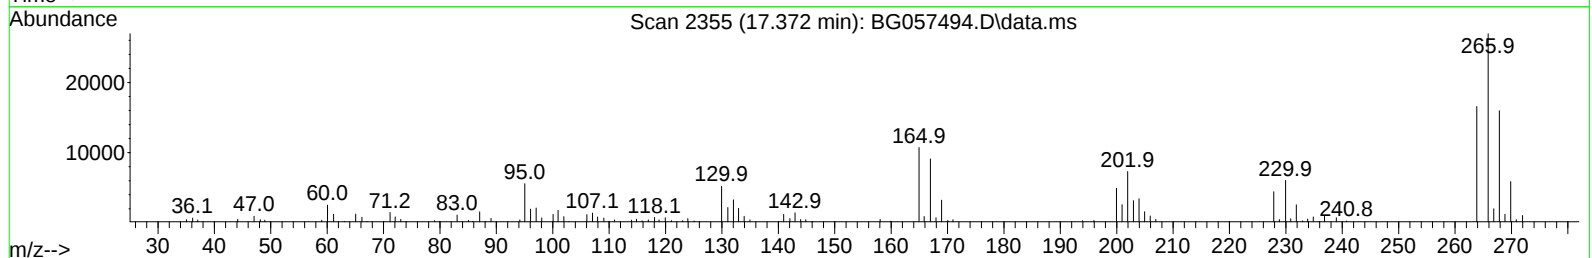


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052223\
Data File : BG057494.D
Acq On : 22 May 2023 15:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 15:47:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

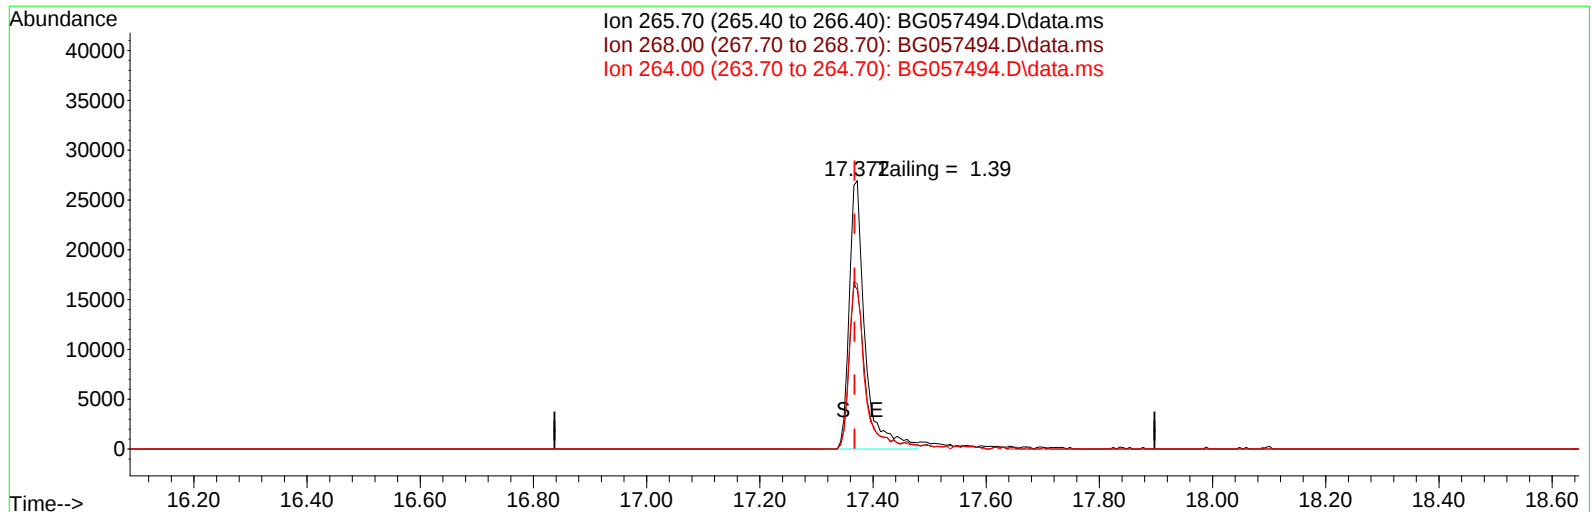

TIC: BG057494.D\data.ms

(70) Pentachlorophenol (C)




17.372min (+ 0.005) 38084.58 ng

response 52596

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	59.31
264.00	59.70	61.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052223\
Data File : BG057494.D
Acq On : 22 May 2023 15:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 15:47:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

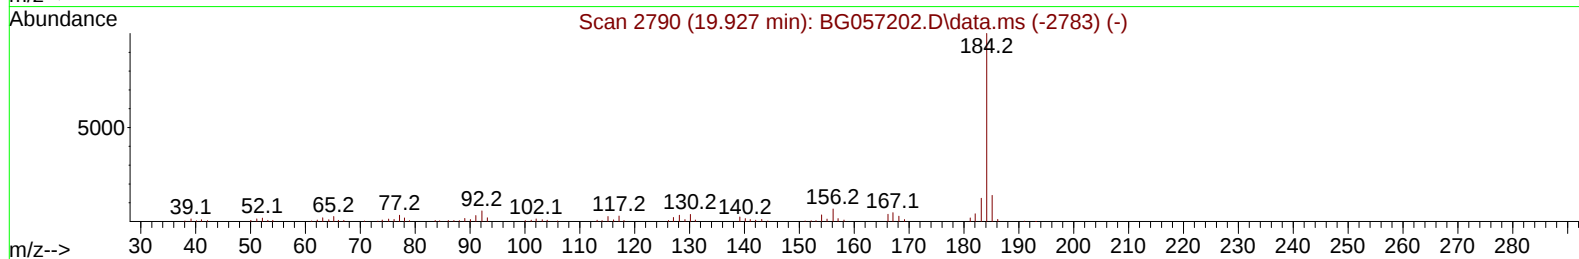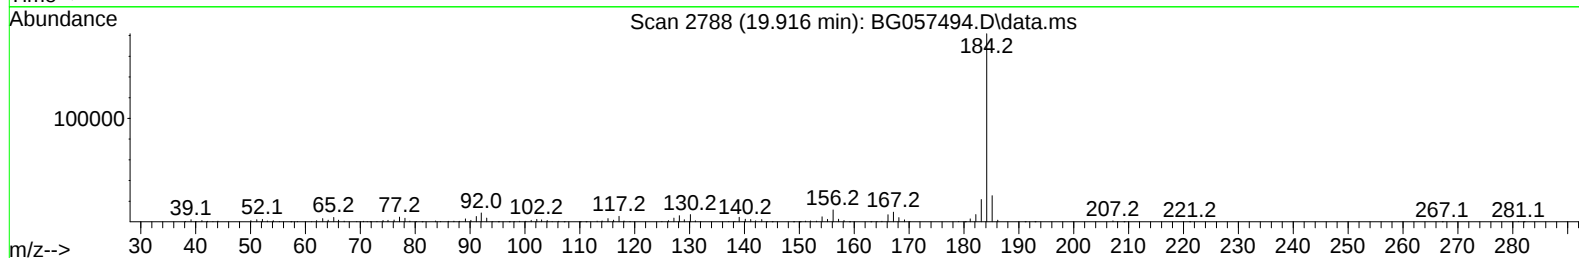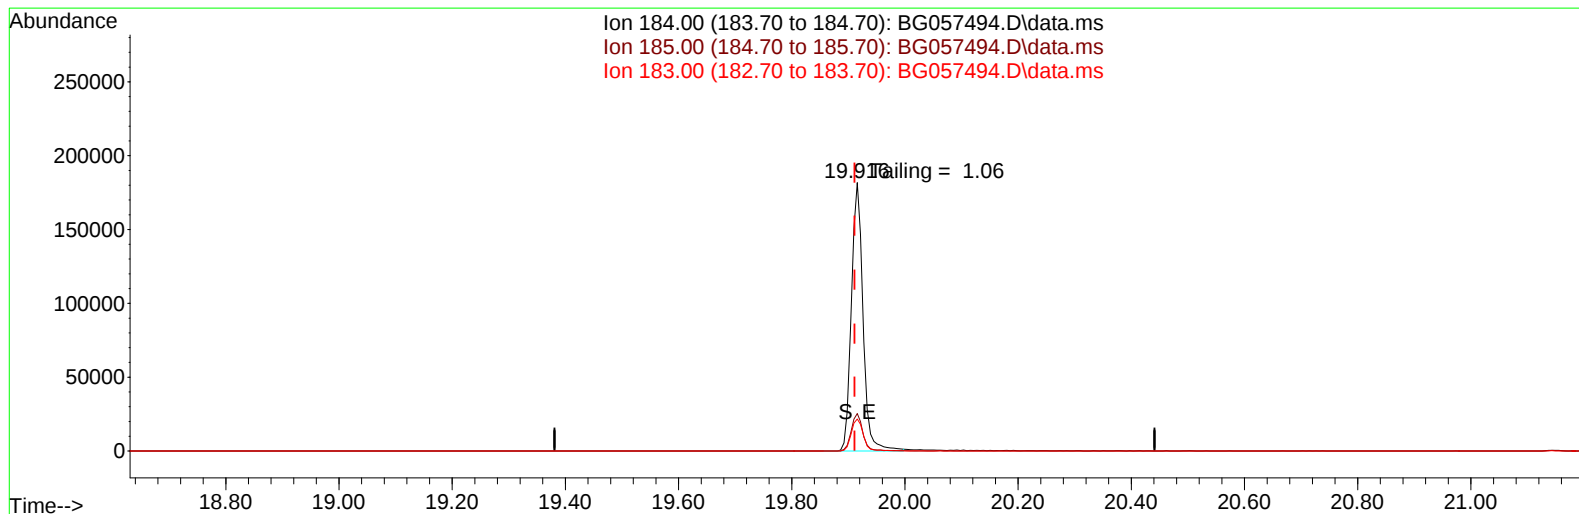

TIC: BG057494.D\data.ms

(77) Benzidine

19.916min (+ 0.005) 0.00 ng

response 262289

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.95
183.00	12.40	11.94
0.00	0.00	0.00