
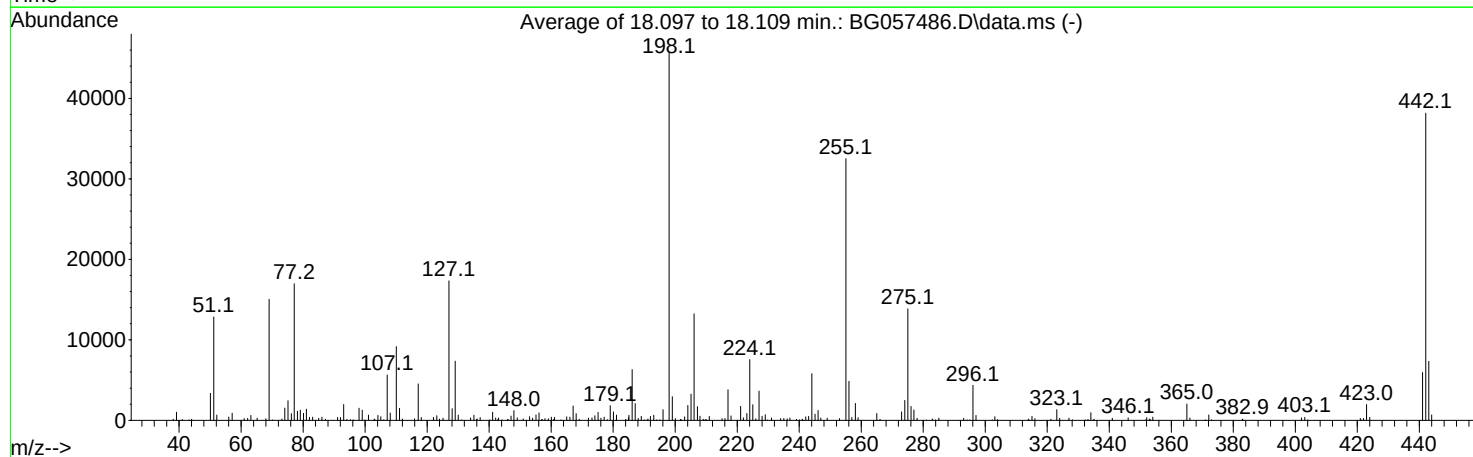


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052223\
 Data File : BG057486.D
 Acq On : 22 May 2023 9:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 20 04:19:55 2023

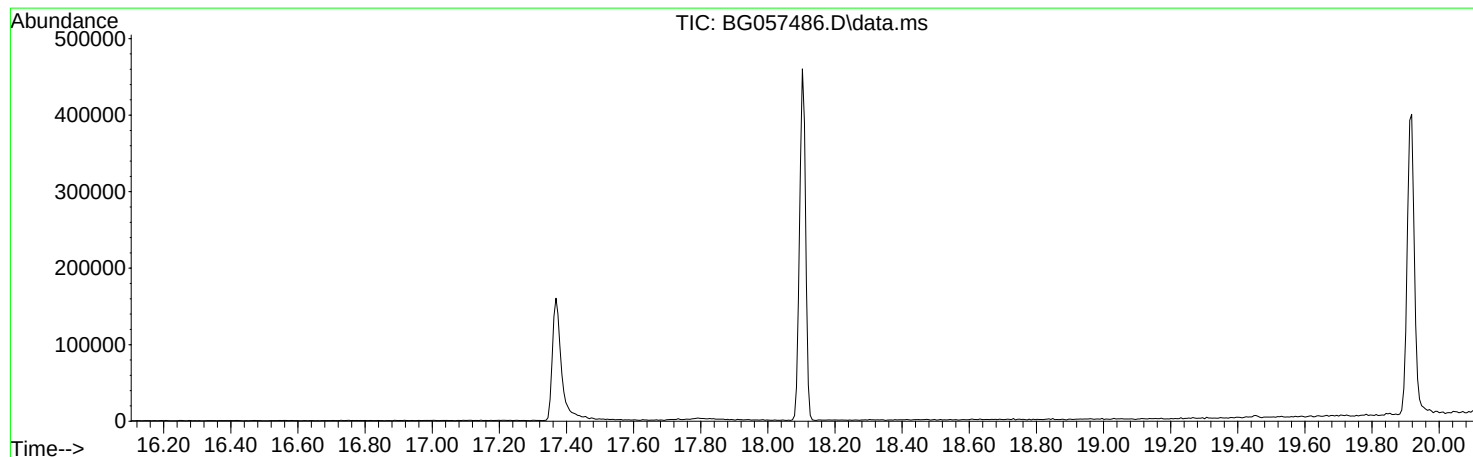

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	12845	PASS
68	69	0.00	2	1.3	192	PASS
69	198	0.00	100	32.9	15053	PASS
70	69	0.00	2	0.5	70	PASS
127	198	10	80	37.9	17329	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45696	PASS
199	198	5	9	6.4	2947	PASS
275	198	10	60	30.3	13853	PASS
365	198	1	100	4.4	2023	PASS
441	198	0.01	100	13.0	5941	PASS
442	442	50	100	100.0	38160	PASS
443	442	15	24	19.2	7337	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/22/2023	BNA_G	<u>BG057486.D</u>
Compound Name	Response	Retention Time
DDT	128756	21.144
DDD	4055	20.746
DDE	185	20.188
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4240	132996	3.19

Instrument :
BNA_G
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052223\  
Data File : BG057486.D  
Acq On    : 22 May 2023    9:42  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 22 11:55:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

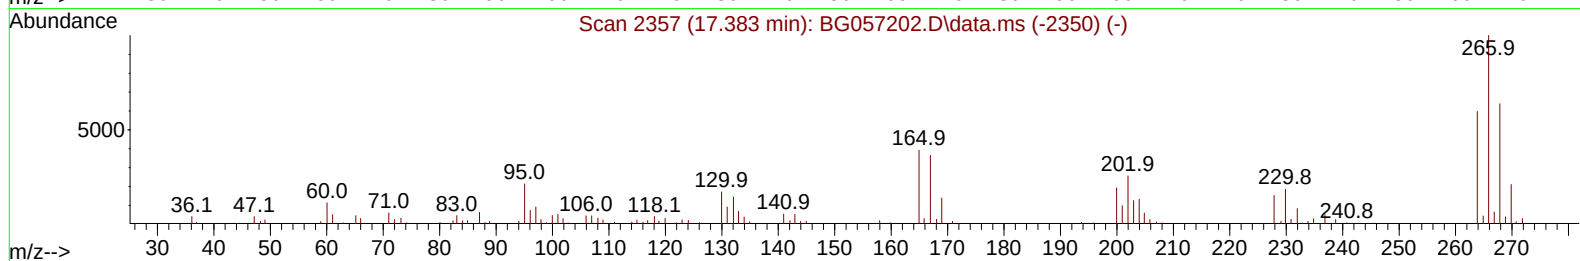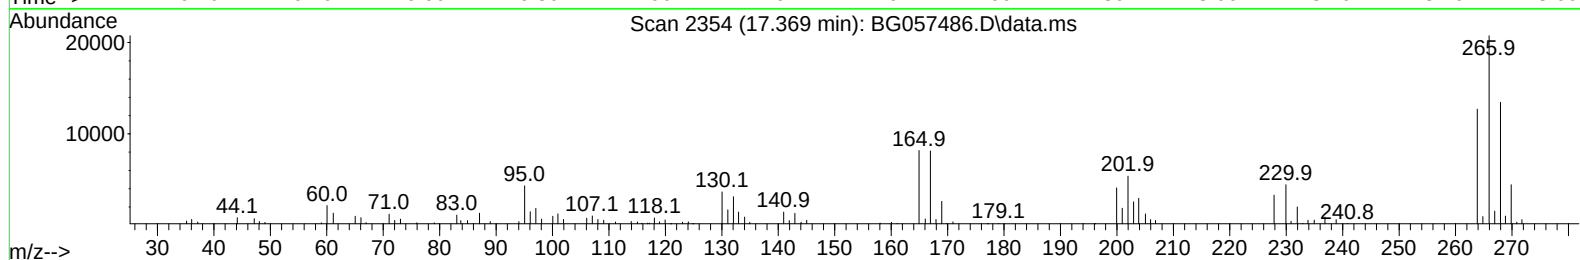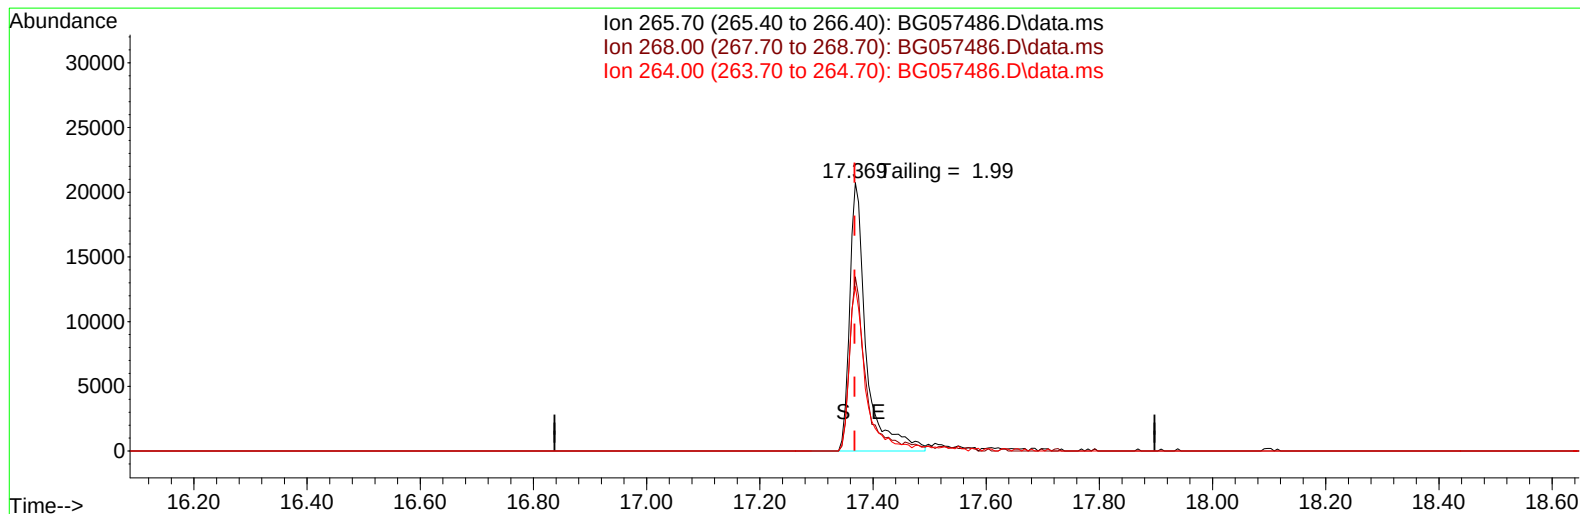

TIC: BG057486.D\data.ms

(70) Pentachlorophenol (C)

17.369min (+ 0.001) 23898.08 ng




response 42317

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.85
264.00	59.70	61.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052223\
Data File : BG057486.D
Acq On : 22 May 2023 9:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 22 11:55:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

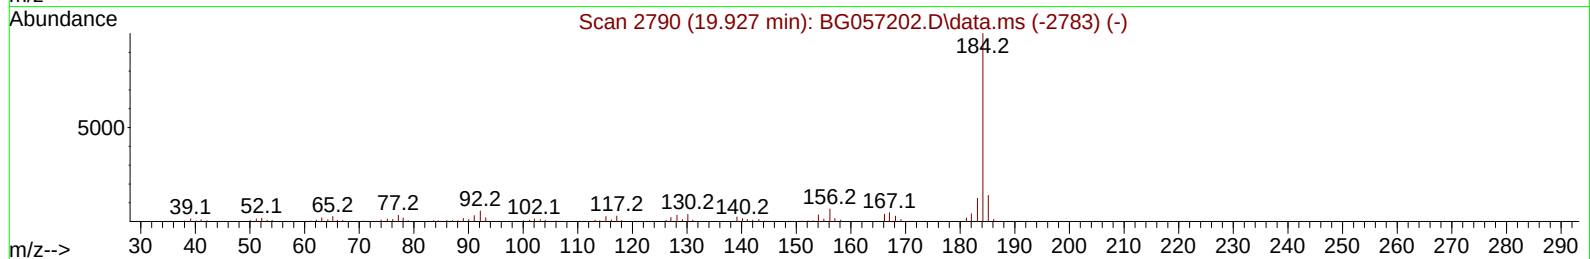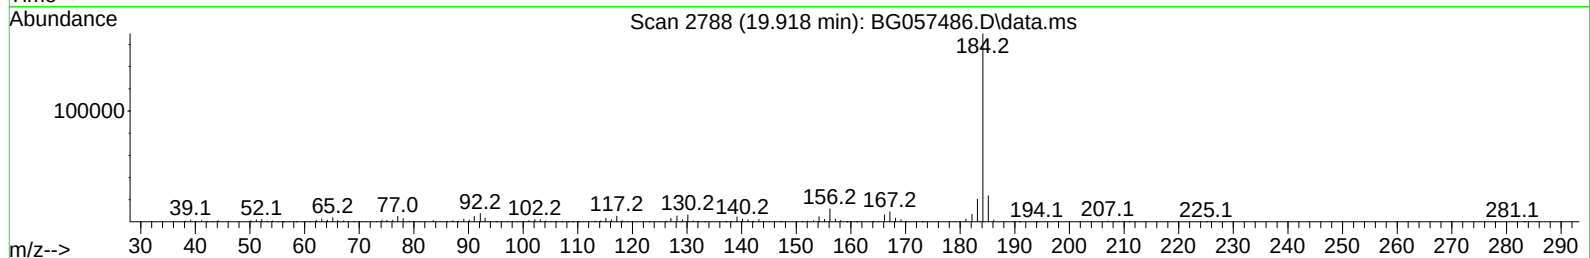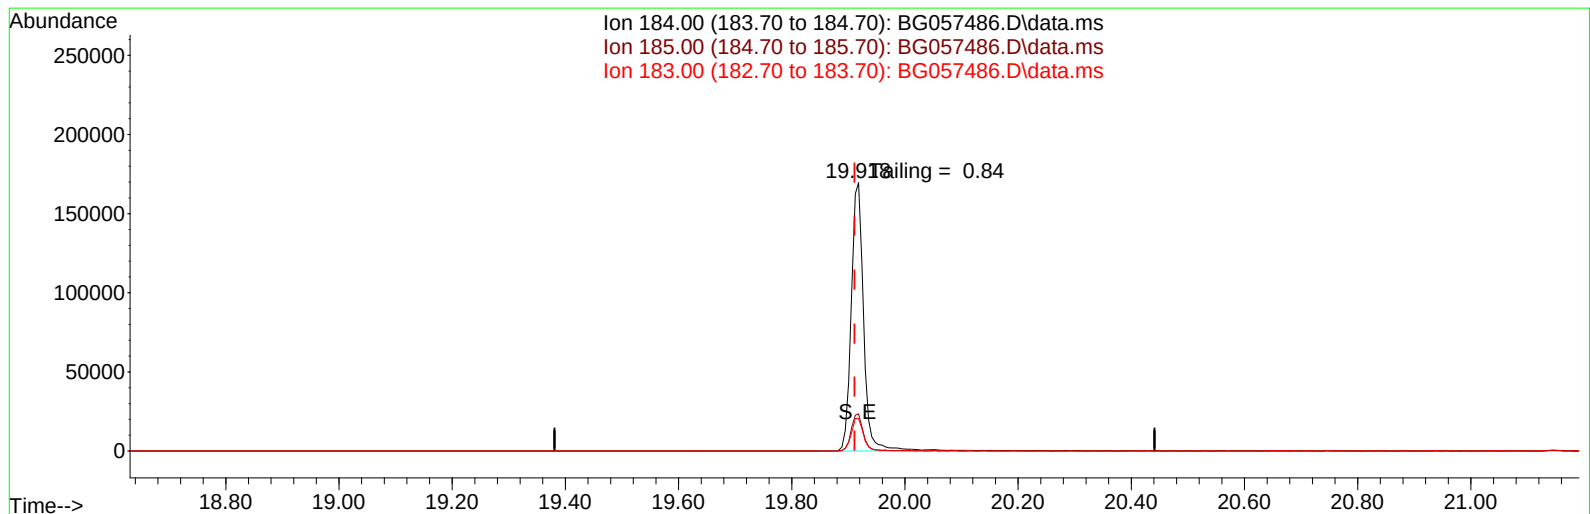

TIC: BG057486.D\data.ms

(77) Benzidine

19.918min (+ 0.007) 0.00 ng

response 256447

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.84
183.00	12.40	12.13
0.00	0.00	0.00