
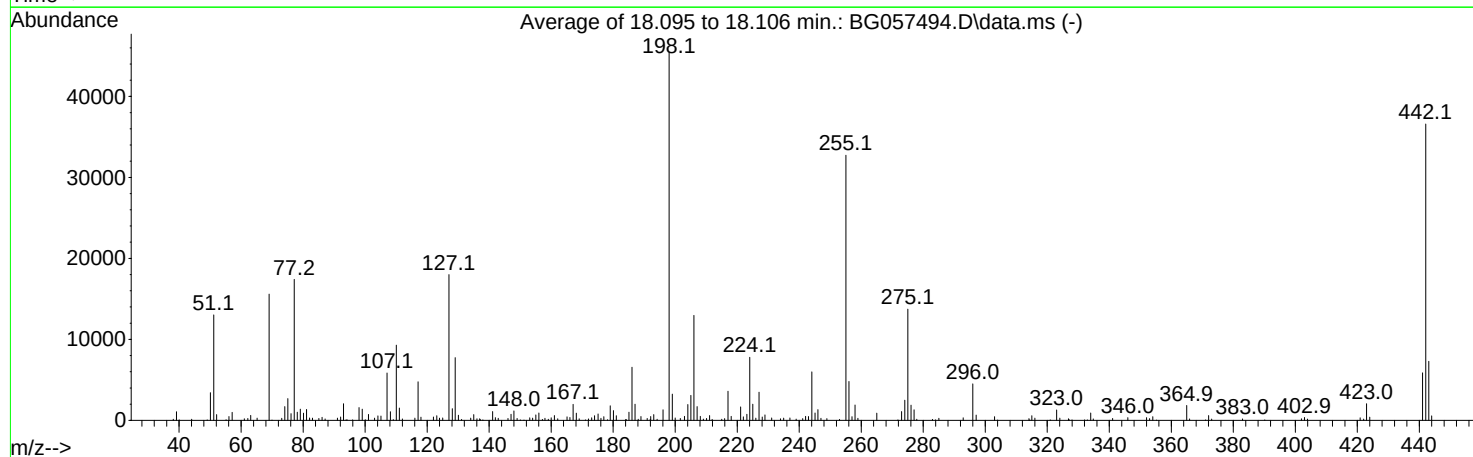


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052223\
Data File : BG057494.D
Acq On : 22 May 2023 15:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat May 20 04:19:55 2023

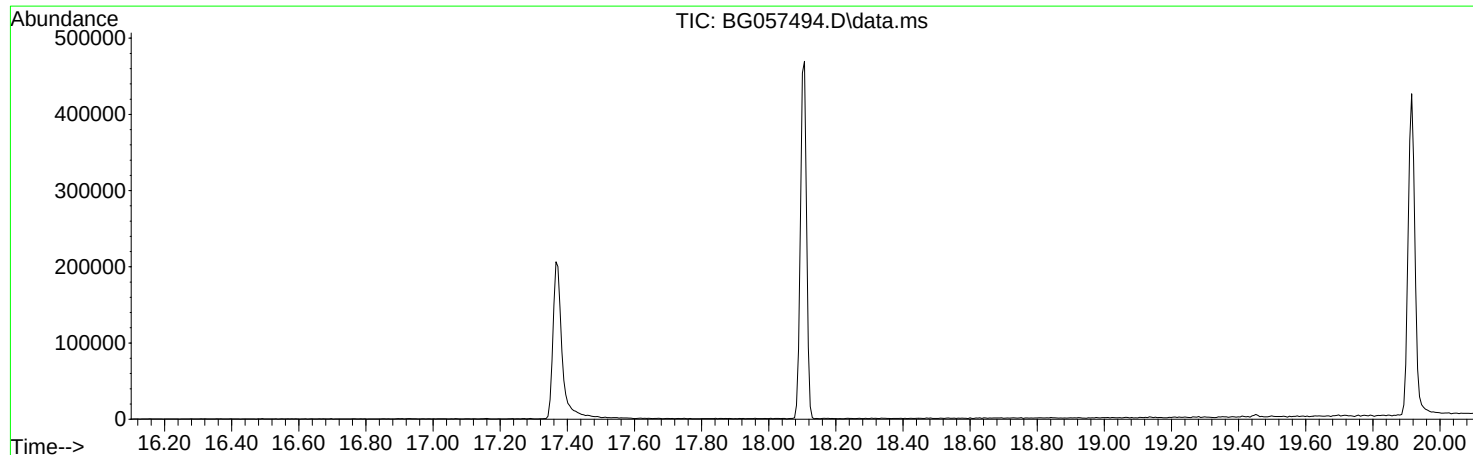

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	13022	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.3	15591	PASS
70	69	0.00	2	0.3	50	PASS
127	198	10	80	39.6	17996	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45421	PASS
199	198	5	9	7.2	3249	PASS
275	198	10	60	30.2	13732	PASS
365	198	1	100	4.1	1842	PASS
441	198	0.01	100	12.9	5863	PASS
442	442	50	100	100.0	36589	PASS
443	442	15	24	20.0	7301	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/22/2023	BNA_G	<u>BG057494.D</u>
Compound Name	Response	Retention Time
DDT	140845	21.149
DDD	3528	20.691
DDE	190	20.192
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3718	144563	2.57

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052223\
Data File : BG057494.D
Acq On : 22 May 2023 15:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 22 15:47:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

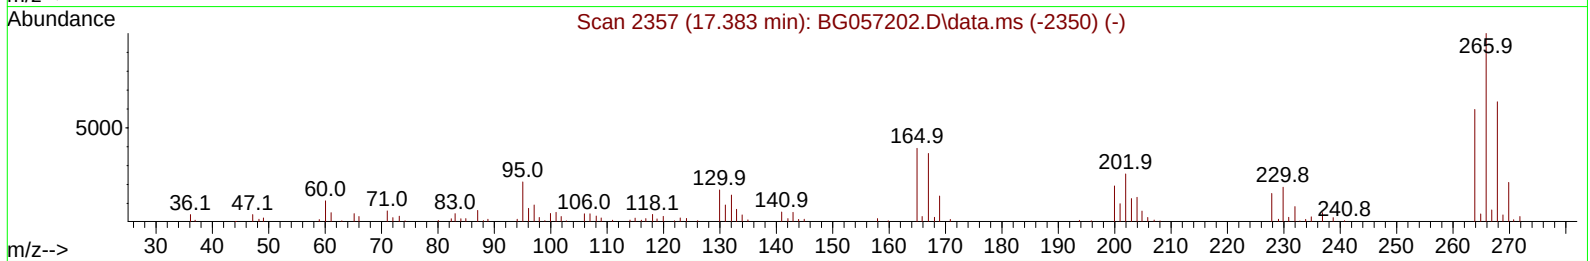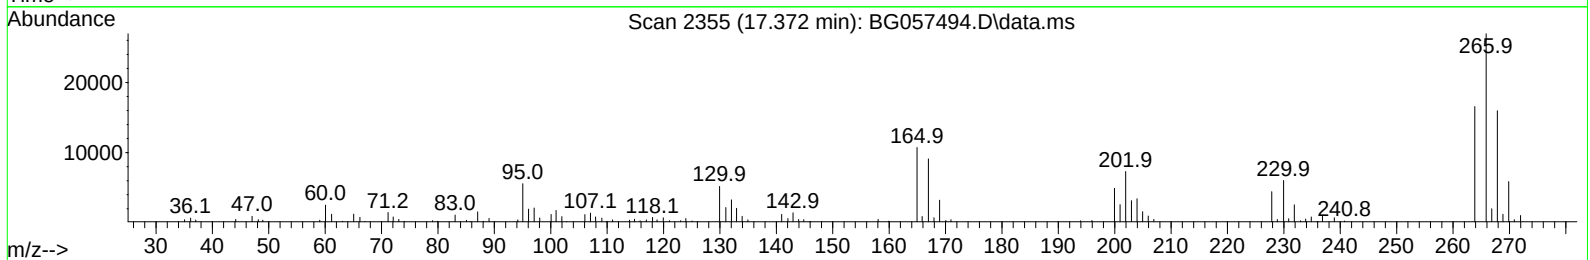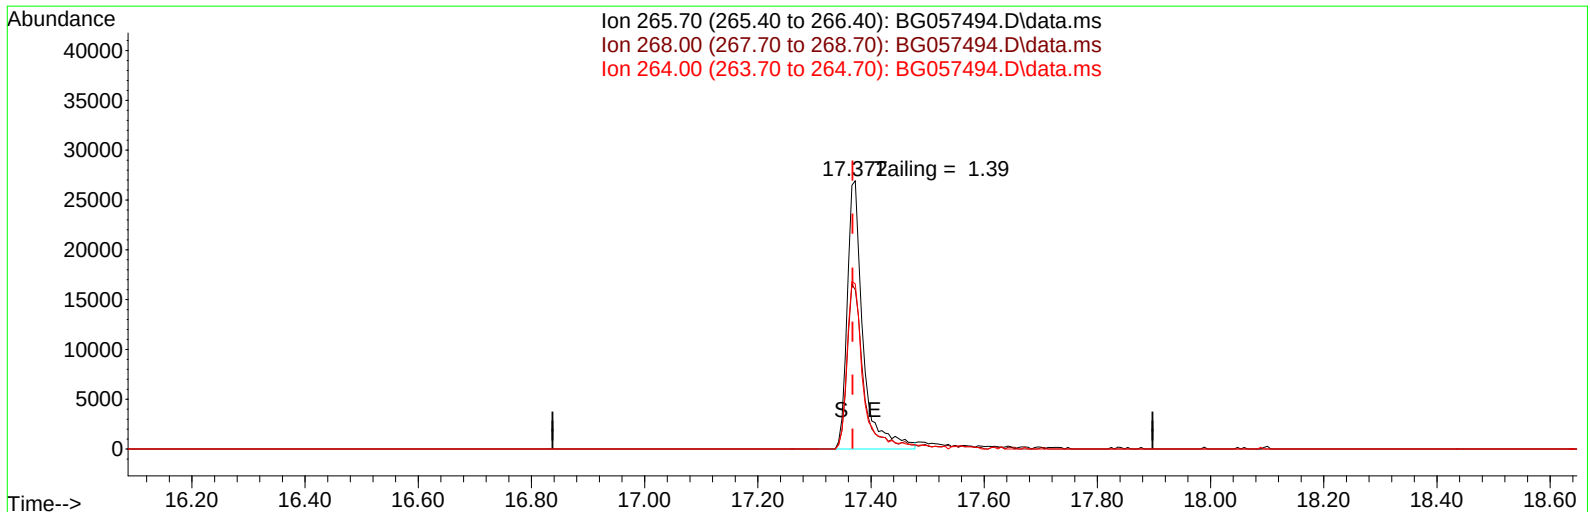

TIC: BG057494.D\data.ms

(70) Pentachlorophenol (C)

17.372min (+ 0.005) 38084.58 ng




response 52596

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	59.31
264.00	59.70	61.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052223\
Data File : BG057494.D
Acq On : 22 May 2023 15:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 22 15:47:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

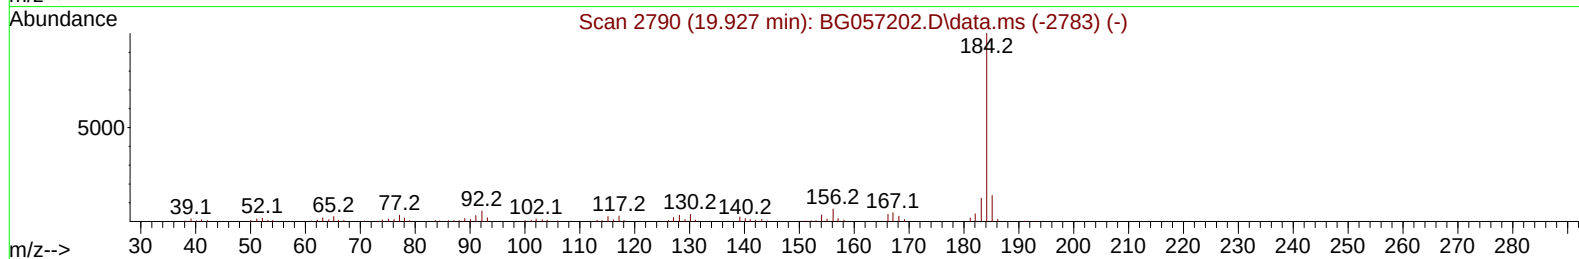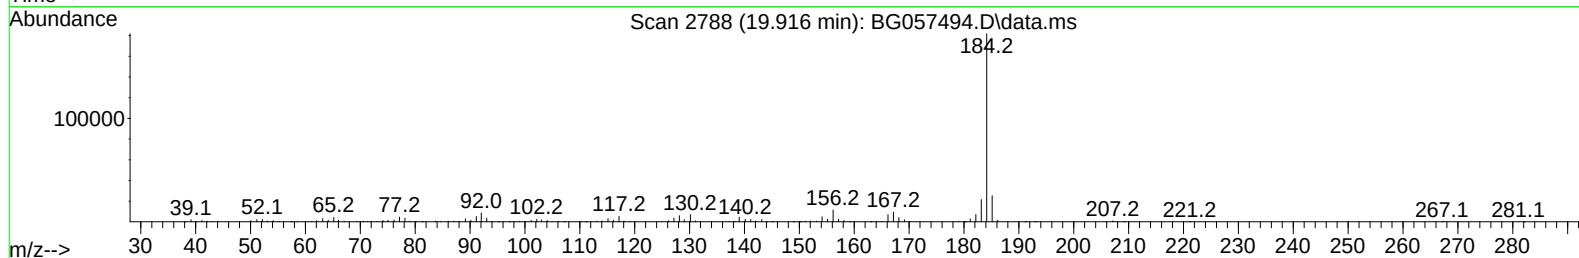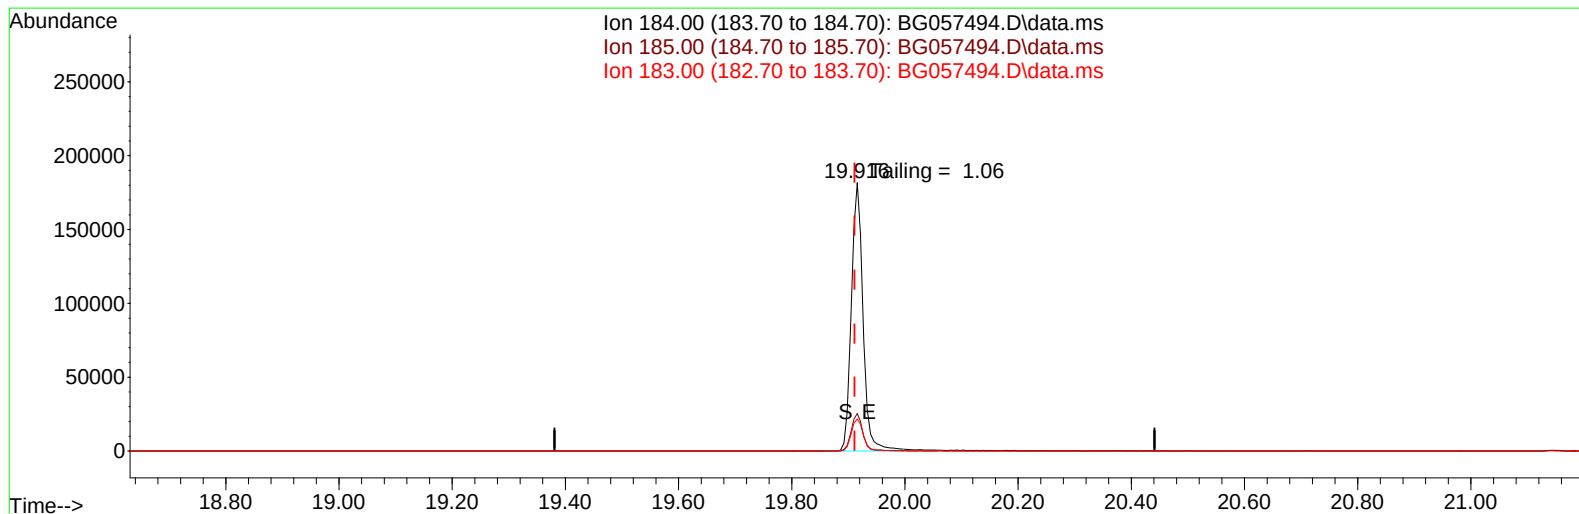

TIC: BG057494.D\data.ms

(77) Benzidine

19.916min (+ 0.005) 0.00 ng

response 262289

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.95
183.00	12.40	11.94
0.00	0.00	0.00