

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052316\
 Data File : BG022048.D
 Acq On : 23 May 2016 15:56
 Operator : UM/SJ
 Sample : H3124-15
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHGF7

Manual Integrations
 APPROVED

umangi
 5/24/2016 7:37:06 PM

Quant Time: May 24 07:31:22 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:44:46 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	43280	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	227548	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	122102	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.53	188	216073	20.00	ng/ul	0.00
75) Chrysene-d12	21.82	240	179412	20.00	ng/ul	0.00
83) Perylene-d12	25.15	264	173365	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	1853	2.23	ng/uL	0.00
5) Phenol-d5	7.31	99	47386	12.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	24001	11.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	42217	12.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	40356	12.17	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	19996	11.92	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	21429	11.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	39407	12.29	ng/ul	0.00
29) 4-Chloroaniline-d4	11.11	131	43058	12.33	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	126848	13.83	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	174215	13.60	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	8183m	5.18	ng/ul	0.02
57) Fluorene-d10	15.77	176	109278	12.72	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	6416	5.68	ng/ul	0.00
70) Anthracene-d10	17.63	188	145020	13.98	ng/ul	0.00
76) Pyrene-d10	19.91	212	138023	13.64	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.92	264	116647	14.50	ng/ul	0.00

Target Compounds

						Qvalue
44) Dimethylphthalate	14.23	163	34823	3.78	ng/ul#	94
47) Acenaphthylene	14.51	152	19683	1.51	ng/ul	99
58) Fluorene	15.83	166	16424	1.75	ng/ul	98
69) Phenanthrene	17.58	178	204192	16.99	ng/ul	99
71) Anthracene	17.66	178	42826	3.52	ng/ul	95
74) Fluoranthene	19.57	202	260057	21.17	ng/ul	99
77) Pyrene	19.94	202	293730	23.27	ng/ul	98
80) Benzo(a)anthracene	21.80	228	92680	8.81	ng/ul	97
82) Chrysene	21.87	228	96803	9.59	ng/ul	98
85) Benzo(b)fluoranthene	24.10	252	95020	9.37	ng/ul#	92
86) Benzo(k)fluoranthene	24.15	252	34722m	3.52	ng/ul	
88) Benzo(a)pyrene	25.00	252	88070	9.00	ng/ul#	93
89) Indeno(1,2,3-cd)pyrene	28.97	276	43522m	3.88	ng/ul	
91) Benzo(g,h,i)perylene	30.17	276	36984m	4.11	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052316\
Data File : BG022048.D
Acq On : 23 May 2016 15:56
Operator : UM/SJ
Sample : H3124-15
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
JHGF7

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:06 PM

Quant Time: May 24 07:31:22 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:44:46 2016
Response via : Initial Calibration

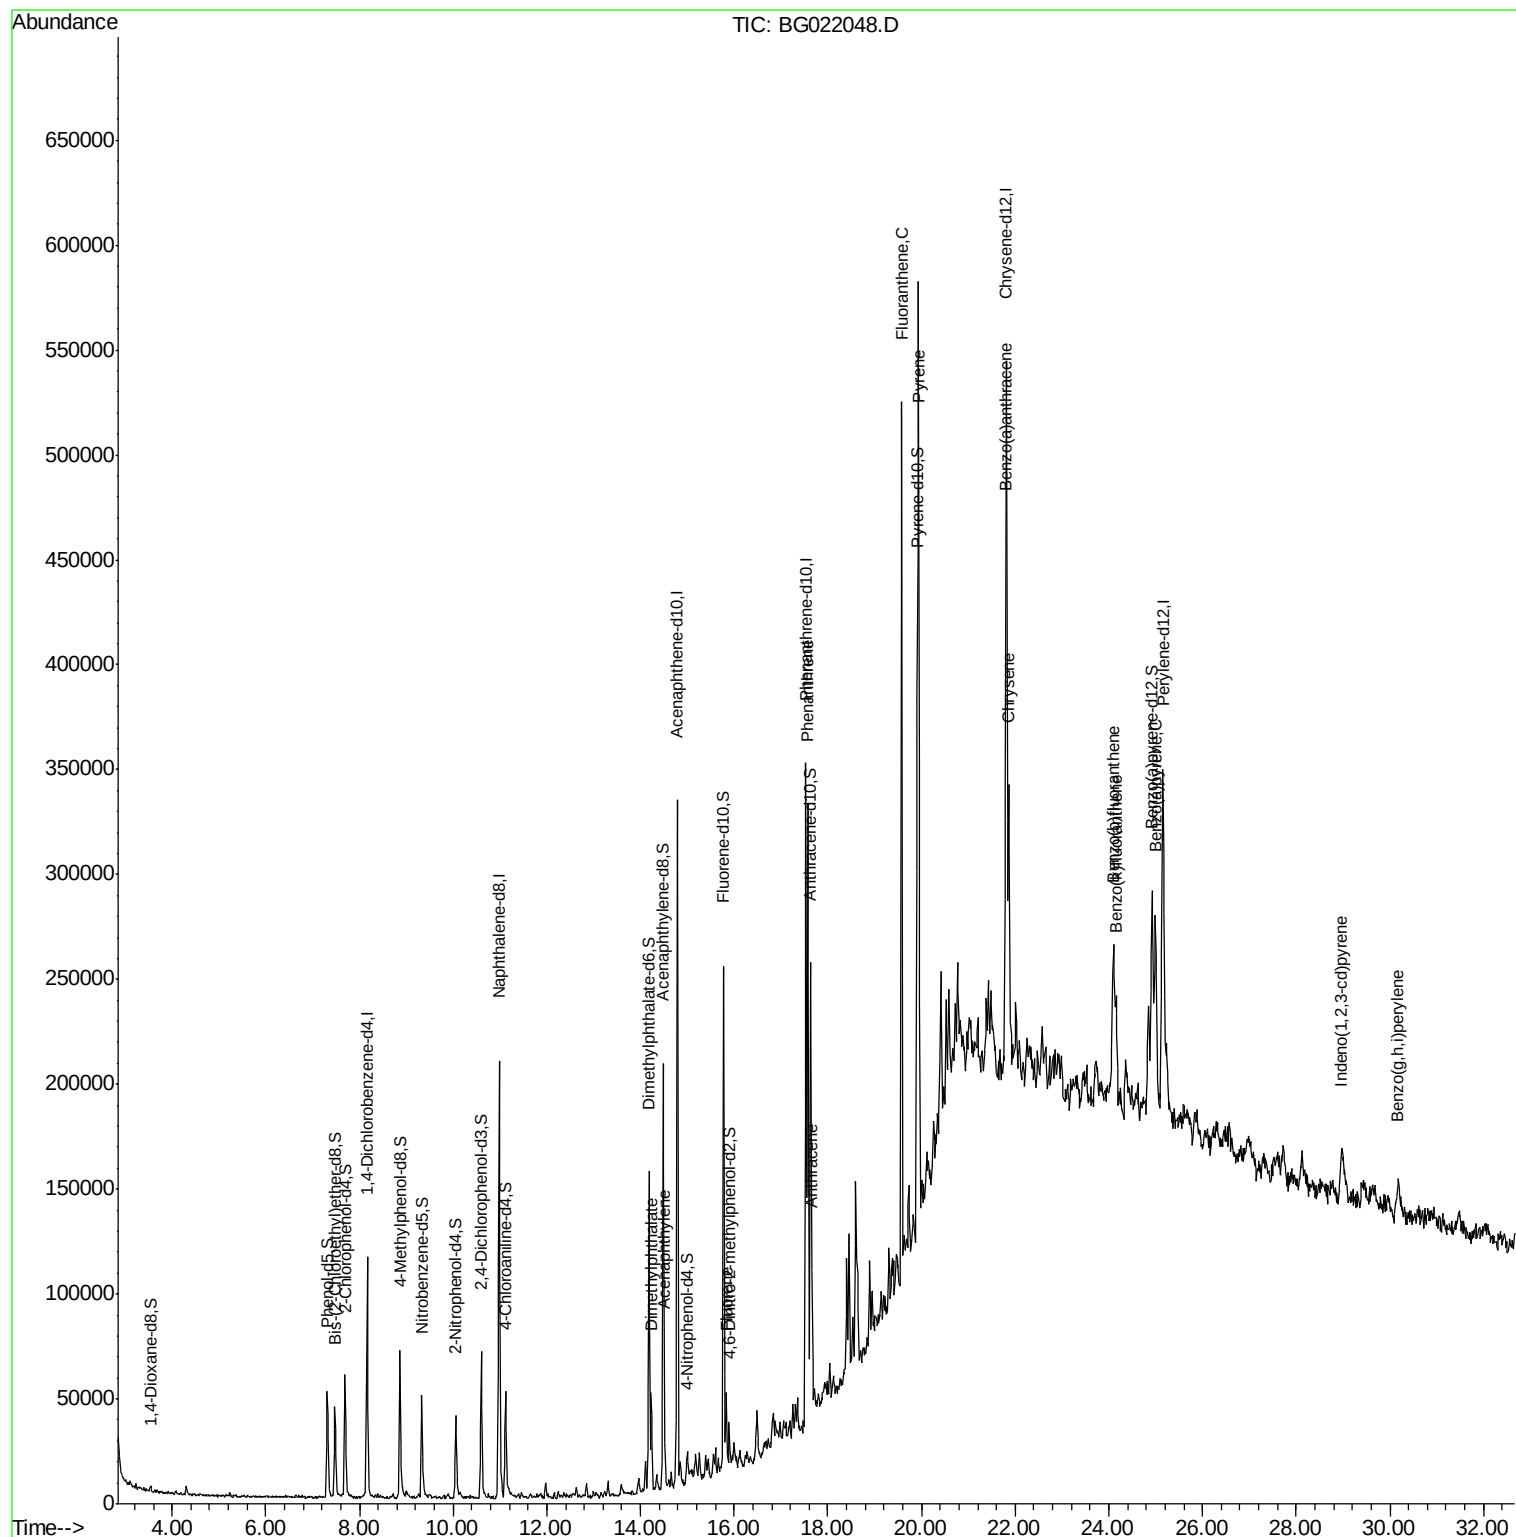

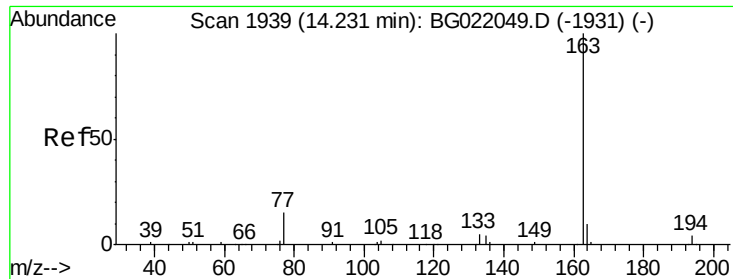





#44
Dimethylphthalate
Concen: 3.78 ng/ul
RT: 14.23 min Scan# 1938
Delta R.T. 0.00 min
Lab File: BG022048.D
Acq: 23 May 2016 15:56

Instrument :
BNA_G
ClientSampled :
JHGF7

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	34823		
194	3.8		3.4	5.2
164	8.3		8.8	13.2#




Manual Integrations
APPROVED


umangi
5/24/2016 7:37:06 PM

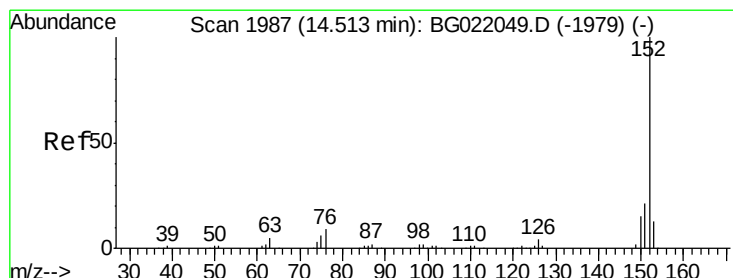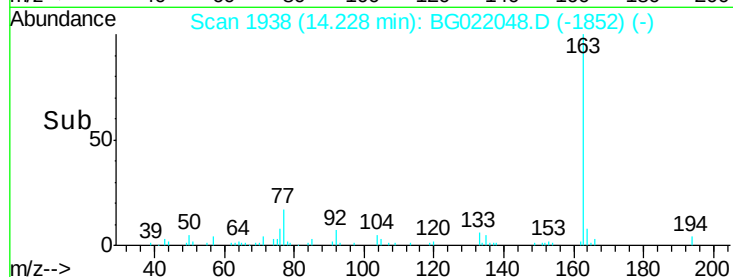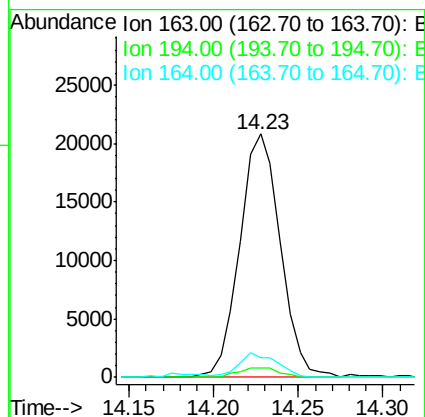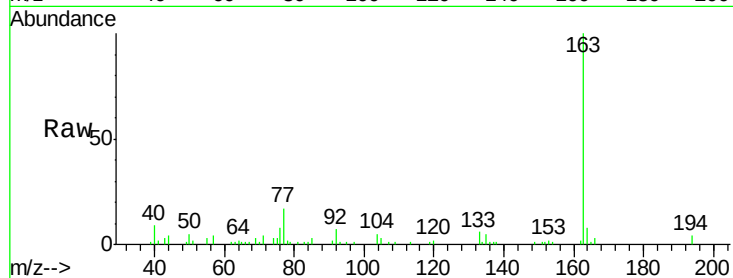

#47
Acenaphthylene
Concen: 1.51 ng/ul
RT: 14.51 min Scan# 1986
Delta R.T. 0.00 min
Lab File: BG022048.D
Acq: 23 May 2016 15:56

Tgt Ion	Ratio	Resp	Lower	Upper
152	100	19683		
151	21.8		17.5	26.3
153	14.8		11.1	16.7

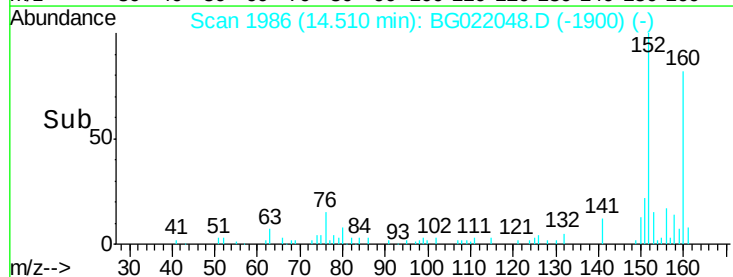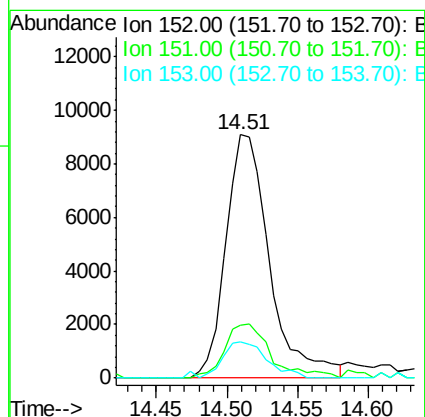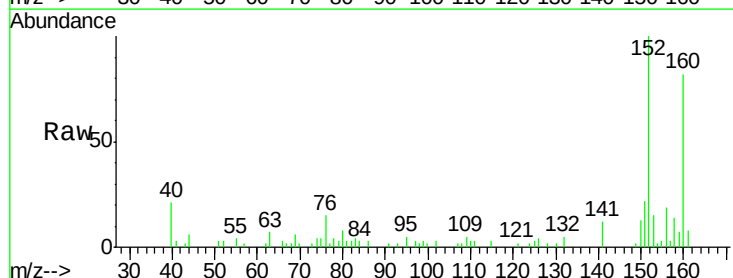

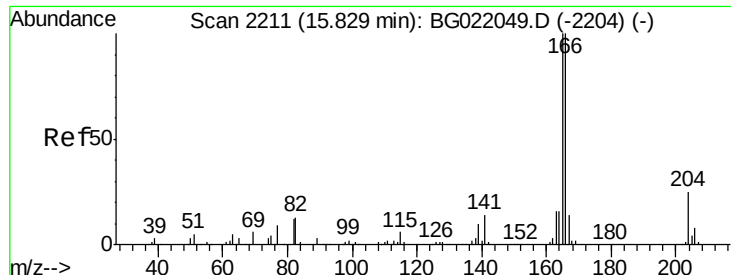





#58
 Fluorene
 Concen: 1.75 ng/ul
 RT: 15.83 min Scan# 2211
 Delta R.T. 0.00 min
 Lab File: BG022048.D
 Acq: 23 May 2016 15:56

Instrument :
 BNA_G
 ClientSampleId :
 JHGF7

Tgt Ion	Ratio	Resp	Lower	Upper
166	100	16424		
165	98.6	80.3	120.5	
167	13.2	10.3	15.5	




Manual Integrations
 APPROVED


umangi
 5/24/2016 7:37:06 PM

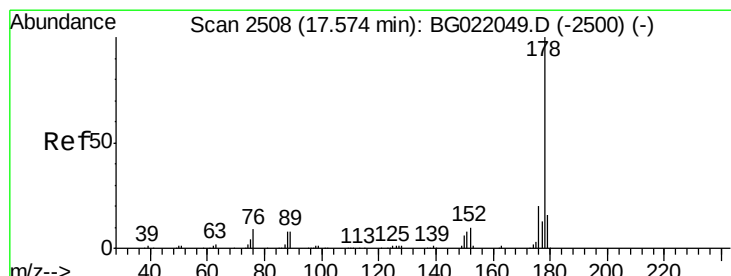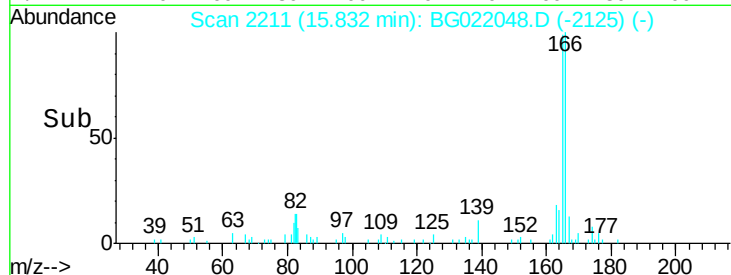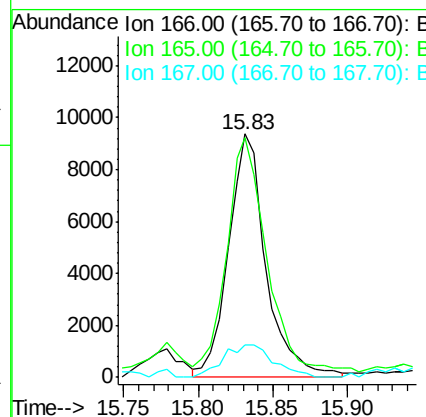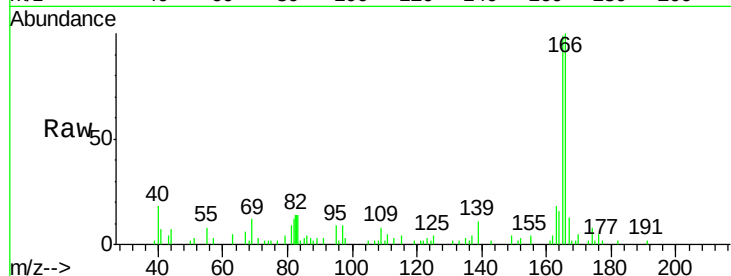

#69
 Phenanthrene
 Concen: 16.99 ng/ul
 RT: 17.58 min Scan# 2508
 Delta R.T. 0.00 min
 Lab File: BG022048.D
 Acq: 23 May 2016 15:56

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	204192		
179	15.4	12.9	19.3	
176	19.4	15.8	23.8	

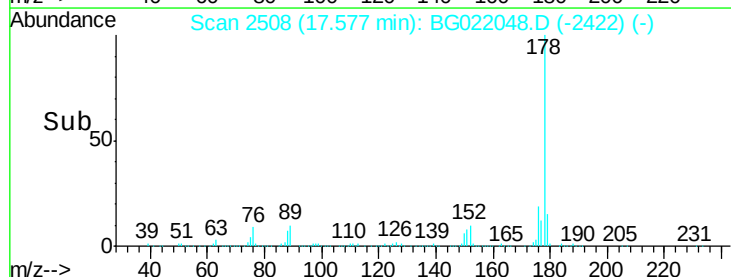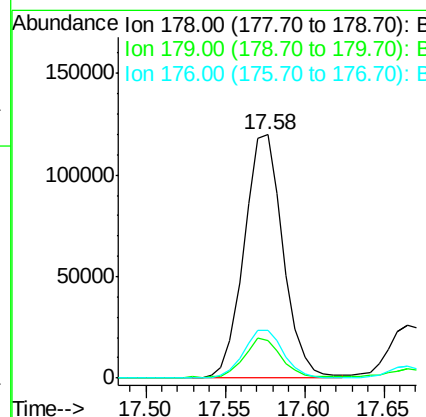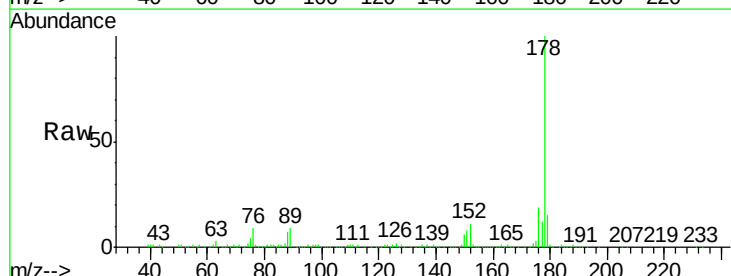

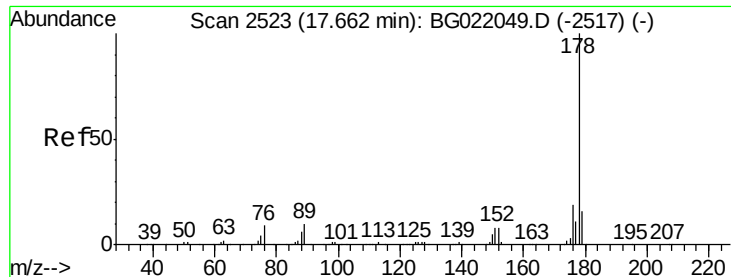


#71
 Anthracene
 Concen: 3.52 ng/ul
 RT: 17.66 min Scan# 2523
 Delta R.T. 0.00 min
 Lab File: BG022048.D
 Acq: 23 May 2016 15:56

Instrument :
 BNA_G
 ClientSampleId :
 JHGF7




Tgt Ion:	178	Resp:	42826
Ion Ratio	Lower	Upper	
178	100		
179	18.4	12.3	18.5
176	21.7	16.3	24.5

Manual Integrations
 APPROVED

umangi
 5/24/2016 7:37:06 PM

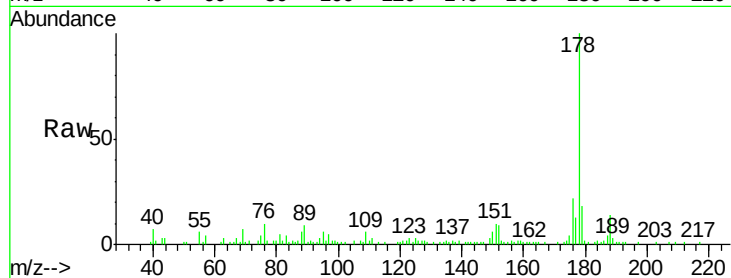




Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

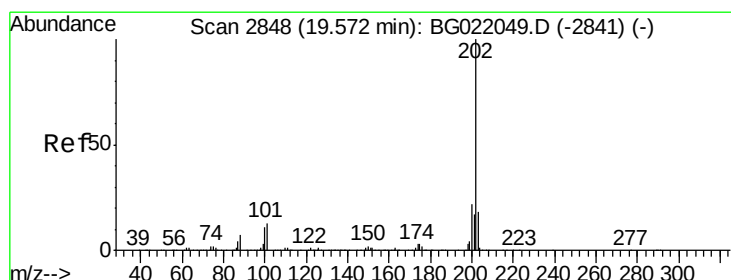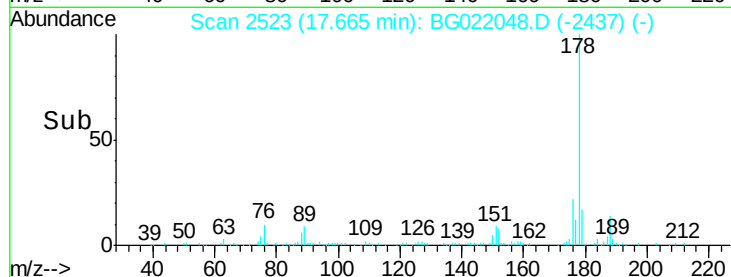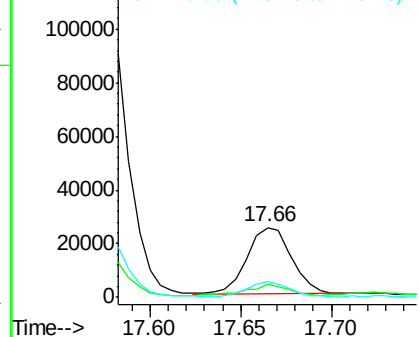


#74
 Fluoranthene
 Concen: 21.17 ng/ul
 RT: 19.57 min Scan# 2848
 Delta R.T. 0.00 min
 Lab File: BG022048.D
 Acq: 23 May 2016 15:56

Tgt Ion:	202	Resp:	260057
Ion Ratio	Lower	Upper	
202	100		
101	13.1	10.6	16.0
100	11.8	8.7	13.1

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

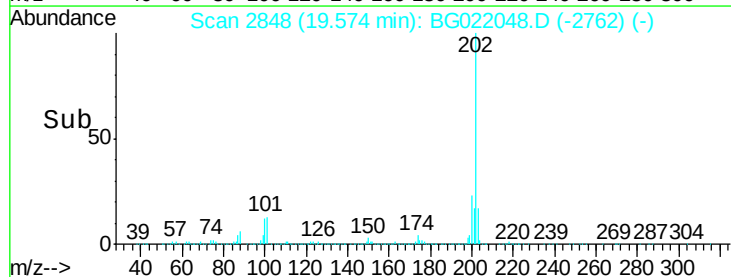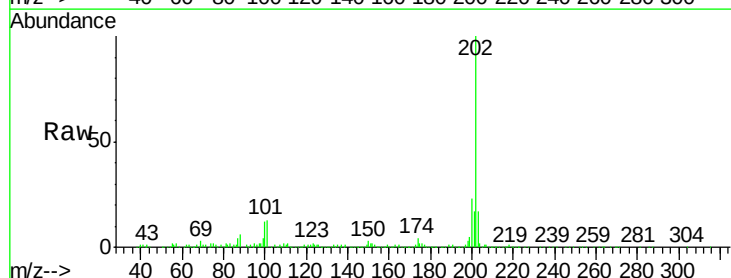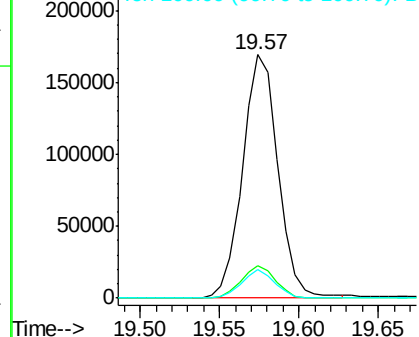

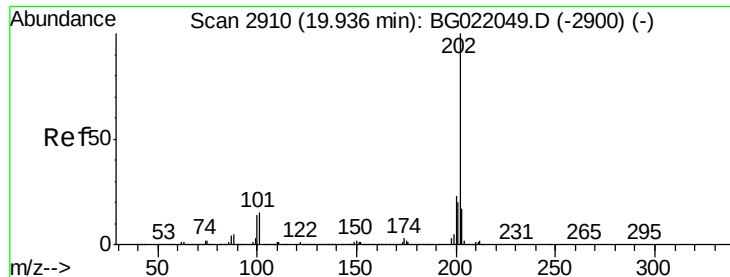





#77
Pyrene
 Concen: 23.27 ng/ul
 RT: 19.94 min Scan# 2910
 Delta R.T. 0.00 min
 Lab File: BG022048.D
 Acq: 23 May 2016 15:56

Instrument :
 BNA_G
 ClientSampleId :
 JHGF7

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	15.9	12.5	18.7
100	14.1	10.2	15.4




Manual Integrations
 APPROVED


umangi
 5/24/2016 7:37:06 PM

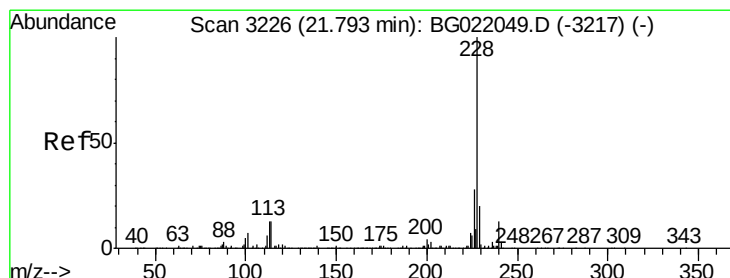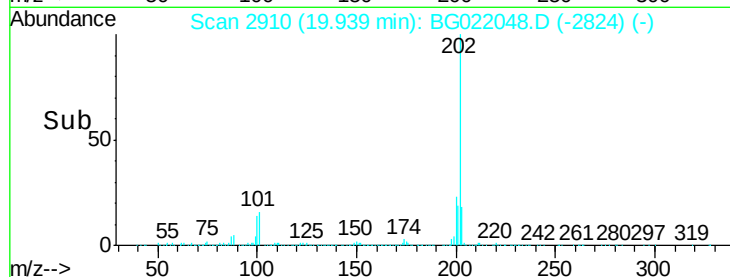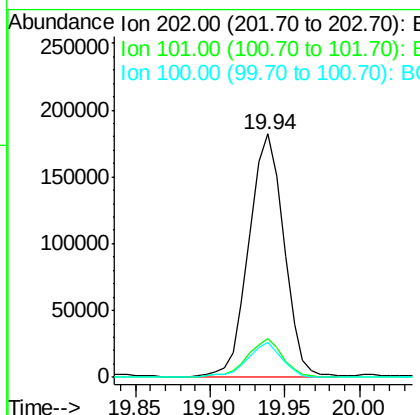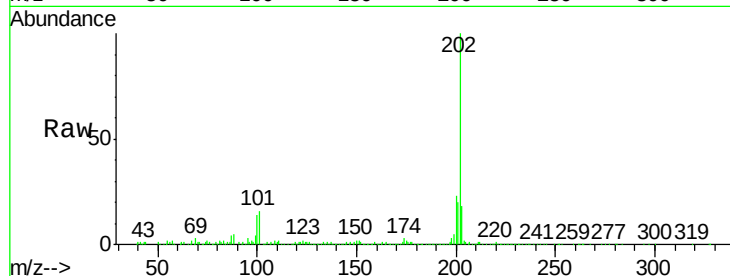

#80
Benzo(a)anthracene
 Concen: 8.81 ng/ul
 RT: 21.80 min Scan# 3226
 Delta R.T. 0.00 min
 Lab File: BG022048.D
 Acq: 23 May 2016 15:56

Tgt Ion	Ratio	Resp Lower	Resp Upper
228	100		
229	20.8	15.4	23.2
226	29.6	22.8	34.2

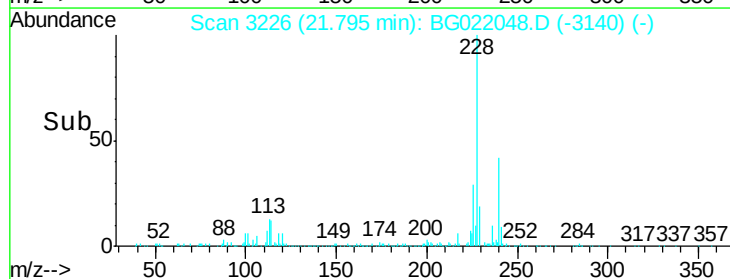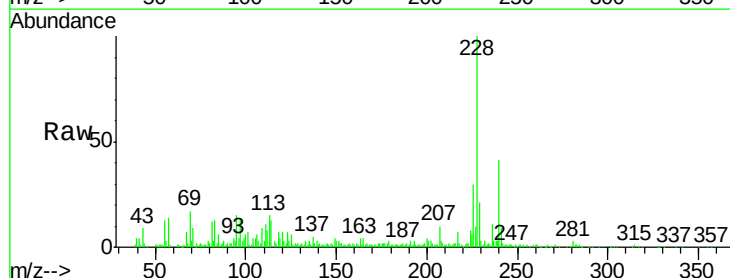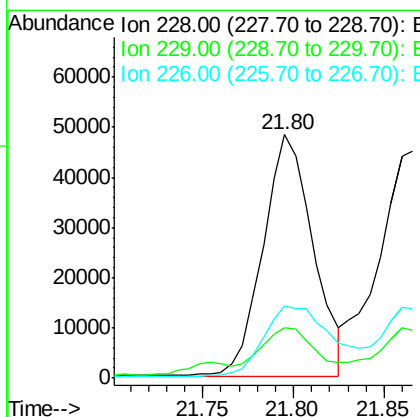

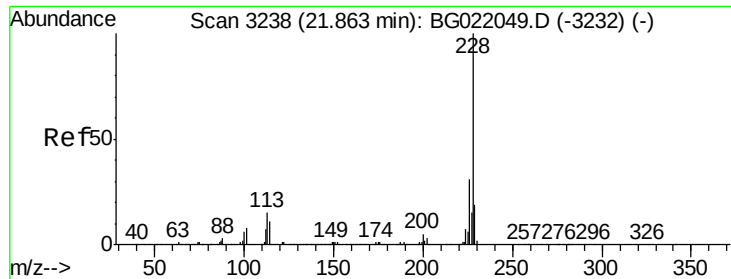

#82

Chrysene

Concen: 9.59 ng/ul

RT: 21.87 min Scan# 3238

Delta R.T. 0.00 min

Lab File: BG022048.D


Acq: 23 May 2016 15:56

Instrument :

BNA_G

ClientSampleId :




JHGF7

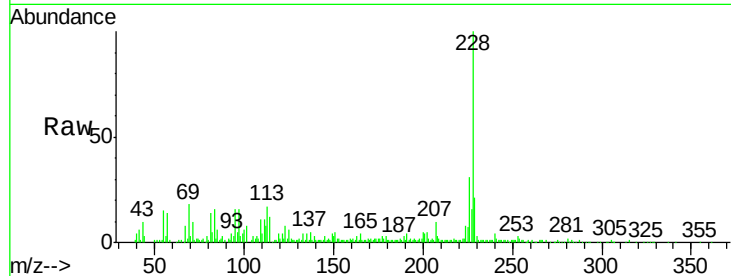

Tgt Ion:	228	Resp:	96803
Ion Ratio		Lower	Upper
228	100		
226	30.7	24.2	36.4
229	21.2	15.0	22.6

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:06 PM

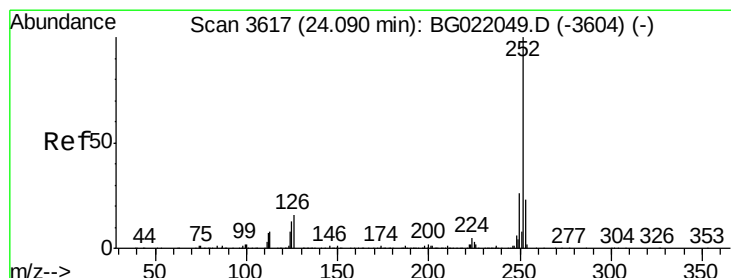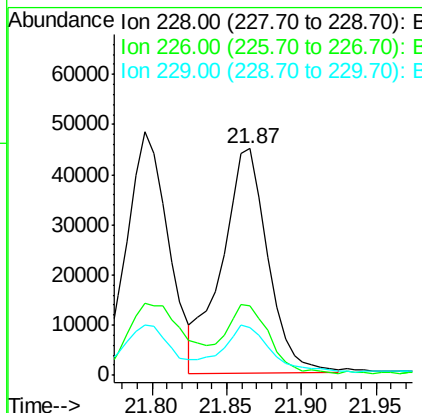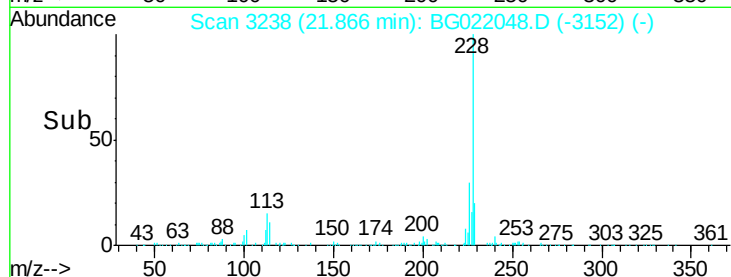

#85

Benzo(b)fluoranthene

Concen: 9.37 ng/ul




RT: 24.10 min Scan# 3618


Delta R.T. 0.02 min

Lab File: BG022048.D

Acq: 23 May 2016 15:56

Tgt Ion:	252	Resp:	95020
Ion Ratio		Lower	Upper
252	100		
253	22.5	18.2	27.2
125	22.0	10.8	16.2#

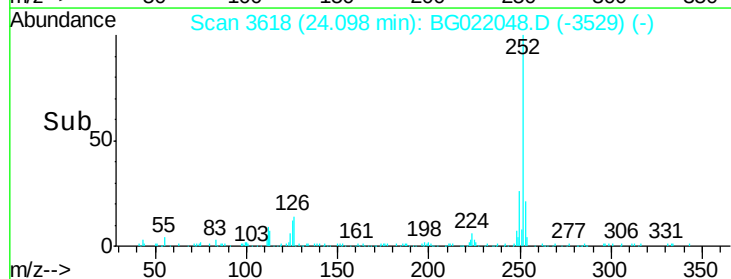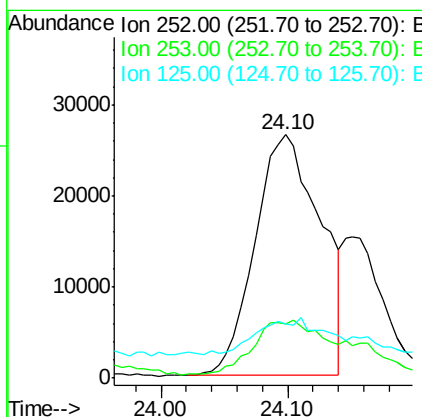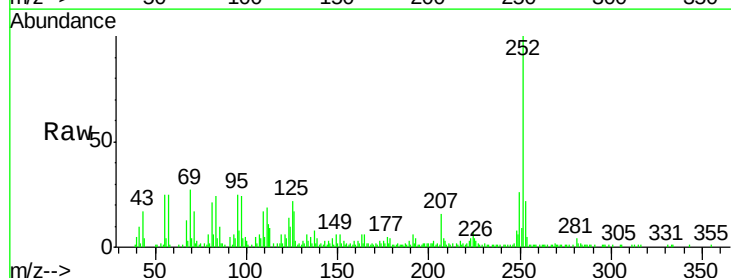

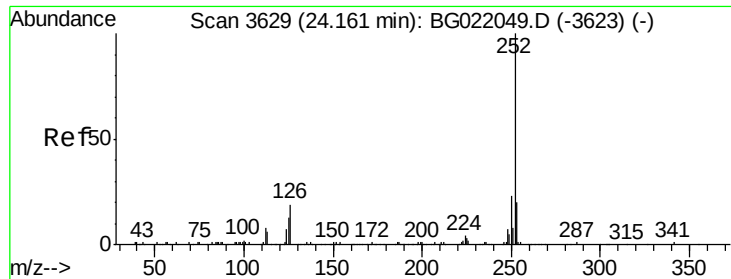

#86

Benzo(k)fluoranthene

Concen: 3.52 ng/ul m

RT: 24.15 min Scan# 3627

Delta R.T. 0.00 min

Lab File: BG022048.D

Acq: 23 May 2016 15:56

Instrument :

BNA_G





ClientSampleId :

JHGF7

Tgt Ion:	252	Resp:	34722
Ion Ratio	Lower	Upper	
252	100		
253	23.0	15.8	23.6
125	29.7	10.6	16.0

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:06 PM

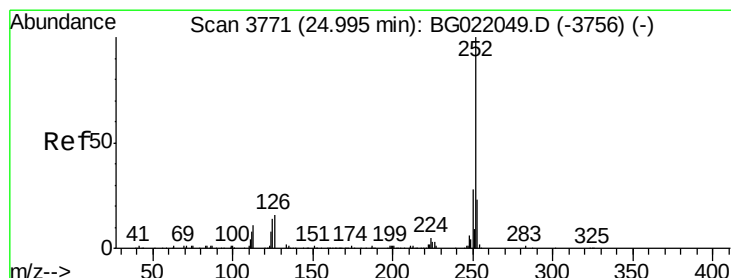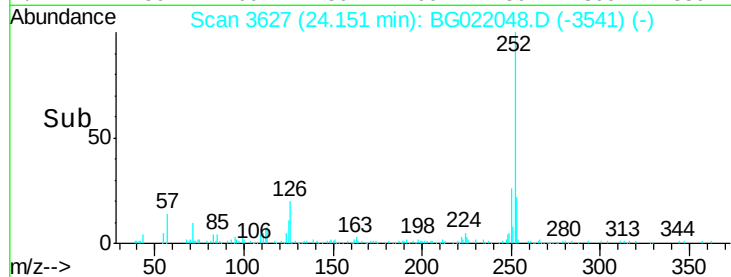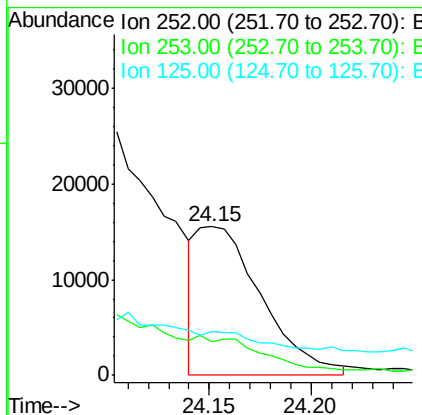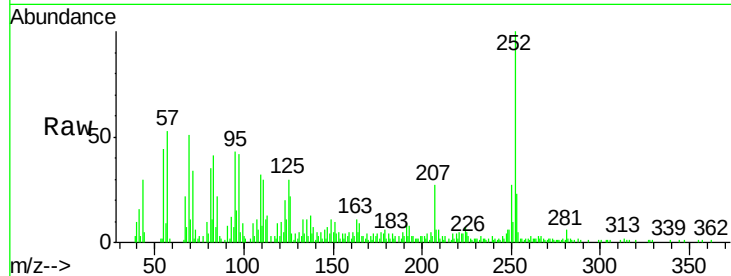

#88

Benzo(a)pyrene

Concen: 9.00 ng/ul




RT: 25.00 min Scan# 3771


Delta R.T. 0.01 min

Lab File: BG022048.D

Acq: 23 May 2016 15:56

Tgt Ion:	252	Resp:	88070
Ion Ratio	Lower	Upper	
252	100		
253	22.6	19.0	28.4
125	20.6	12.0	18.0

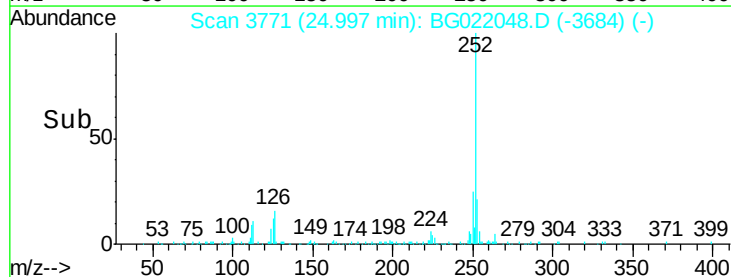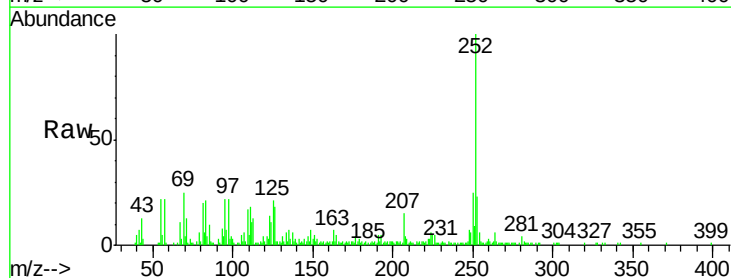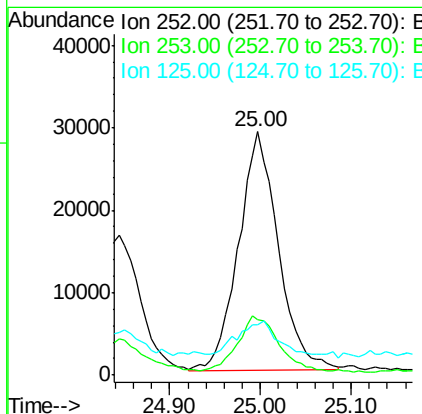

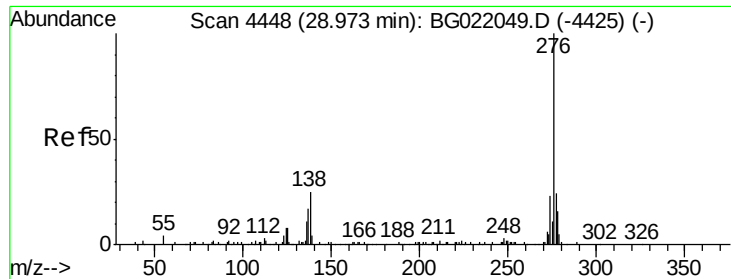

#89





Indeno(1,2,3-cd)pyrene
Concen: 3.88 ng/ul m
RT: 28.97 min Scan# 4447
Delta R.T. 0.01 min
Lab File: BG022048.D
Acq: 23 May 2016 15:56

Instrument :
BNA_G
ClientSampleId :
JHGF7

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	43522		
138	32.5	20.8	31.2#	
277	28.0	17.6	26.4#	

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:06 PM

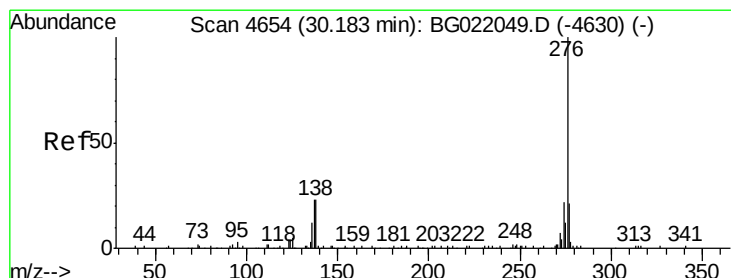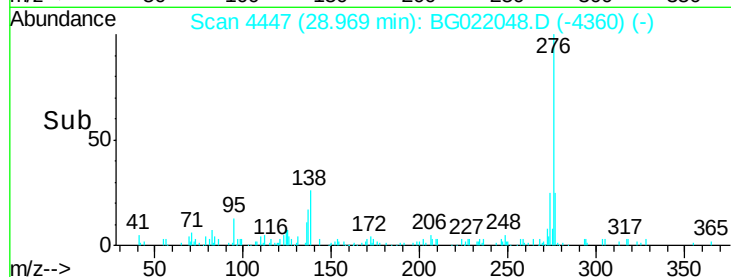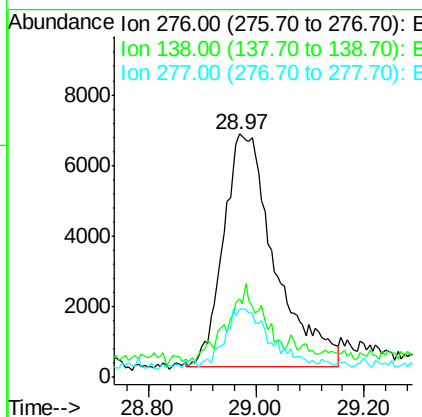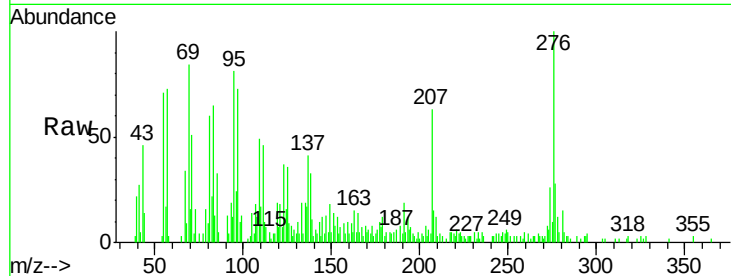

#91

Benzo(g,h,i)perylene
Concen: 4.11 ng/ul m
RT: 30.17 min Scan# 4652
Delta R.T. 0.01 min
Lab File: BG022048.D
Acq: 23 May 2016 15:56

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	36984		
138	37.1	22.1	33.1#	
277	25.0	17.0	25.4	

