

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052316\
 Data File : BG022052.D
 Acq On : 23 May 2016 18:37
 Operator : UM/SJ
 Sample : H3124-20
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHGJ3

Manual Integrations
 APPROVED

umangi
 5/24/2016 7:37:14 PM

Quant Time: May 24 08:07:40 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 07:40:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	42350	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	216940	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	114079	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.53	188	215396	20.00	ng/ul	0.00
75) Chrysene-d12	21.82	240	195962	20.00	ng/ul	0.00
83) Perylene-d12	25.16	264	183090	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	3646	4.49	ng/uL	0.00
5) Phenol-d5	7.31	99	84986	22.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	44717	22.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	75633	23.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	73487	22.64	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	37862	23.66	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	40918	23.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	71293	23.32	ng/ul	0.00
29) 4-Chloroaniline-d4	11.11	131	79584	23.90	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	213581	24.93	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	293584	24.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	24046	16.30	ng/ul	0.00
57) Fluorene-d10	15.78	176	189330	23.59	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	19139	17.00	ng/ul	0.00
70) Anthracene-d10	17.63	188	266571	25.78	ng/ul	0.00
76) Pyrene-d10	19.91	212	278600	25.21	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.93	264	237421	27.95	ng/ul	0.00

Target Compounds

					Qvalue
28) Naphthalene	11.03	128	26228	2.38 ng/ul	98
34) 2-Methylnaphthalene	12.63	142	21144	2.69 ng/ul	100
40) 1,1'-Biphenyl	13.62	154	9495	1.01 ng/ul#	94
44) Dimethylphthalate	14.22	163	83923	9.75 ng/ul	99
47) Acenaphthylene	14.51	152	34890	2.86 ng/ul	98
49) Acenaphthene	14.85	153	24063	2.86 ng/ul	95
53) Dibenzofuran	15.18	168	18770m	1.80 ng/ul	
58) Fluorene	15.83	166	83181	9.46 ng/ul	99
69) Phenanthrene	17.58	178	910304	75.98 ng/ul	97
71) Anthracene	17.67	178	184044	15.17 ng/ul	99
72) Carbazole	17.94	167	11019	1.05 ng/ul#	84
74) Fluoranthene	19.58	202	975436	79.67 ng/ul	98
77) Pyrene	19.94	202	1155545m	83.80 ng/ul	
80) Benzo(a)anthracene	21.80	228	382799	33.31 ng/ul	95
82) Chrysene	21.87	228	362457	32.88 ng/ul	95
85) Benzo(b)fluoranthene	24.10	252	354978	33.13 ng/ul#	95
86) Benzo(k)fluoranthene	24.15	252	94587m	9.07 ng/ul	
88) Benzo(a)pyrene	25.00	252	313672	30.34 ng/ul	99
89) Indeno(1,2,3-cd)pyrene	28.98	276	148720	12.55 ng/ul	97
90) Dibenzo(a,h)anthracene	29.04	278	38319m	3.86 ng/ul	
91) Benzo(g,h,i)perylene	30.18	276	119877	12.63 ng/ul	96

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052316\
Data File : BG022052.D
Acq On : 23 May 2016 18:37
Operator : UM/SJ
Sample : H3124-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHGJ3

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:14 PM

Quant Time: May 24 08:07:40 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 07:40:24 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#)=qualifier out of range (m)=manual integration (+)=signals summed						


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052316\
Data File : BG022052.D
Acq On : 23 May 2016 18:37
Operator : UM/SJ
Sample : H3124-20
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
JHGJ3

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:14 PM

Quant Time: May 24 08:07:40 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 07:40:24 2016
Response via : Initial Calibration

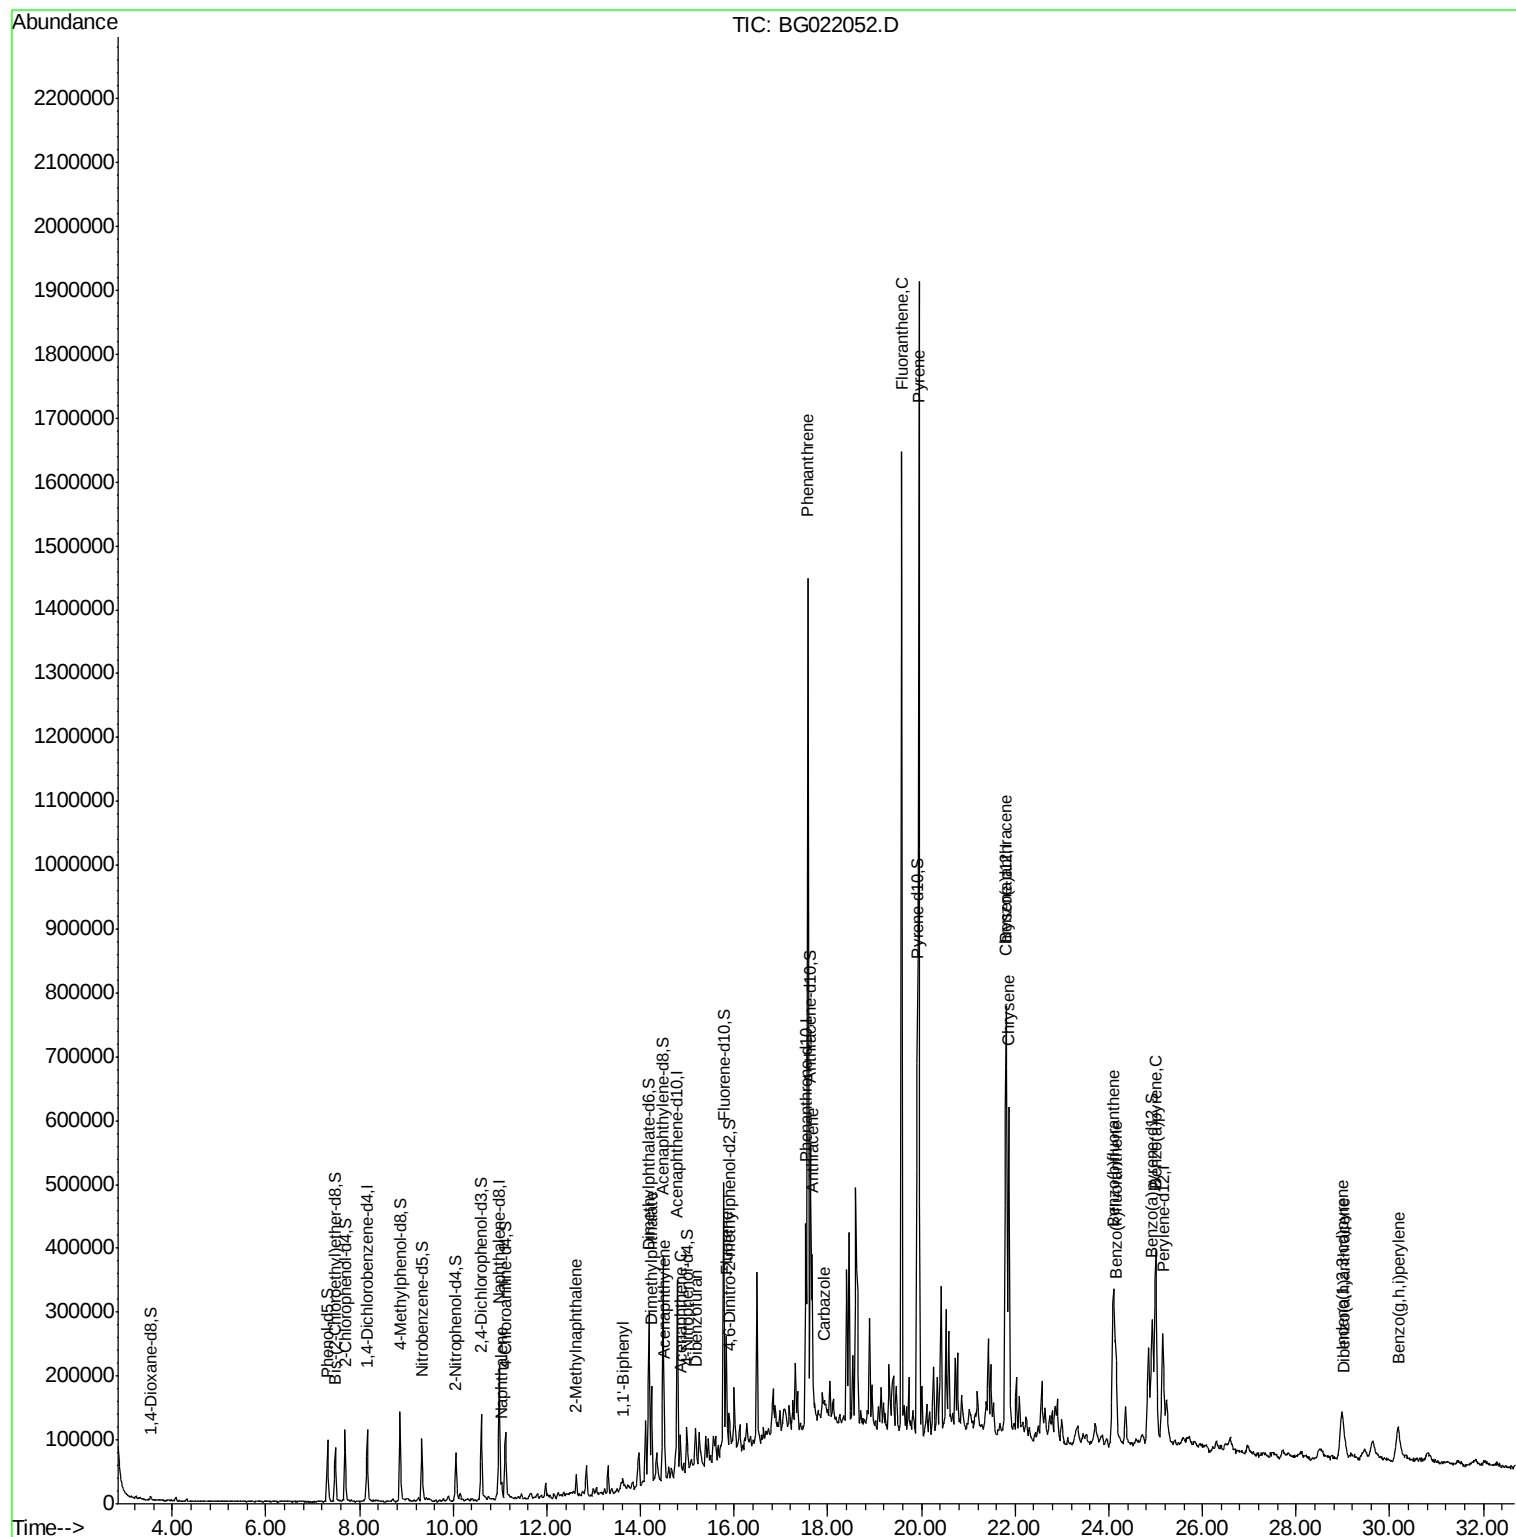

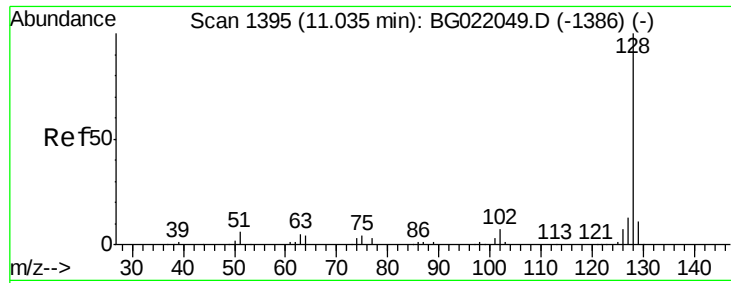





#28
Naphthalene
Concen: 2.38 ng/ul
RT: 11.03 min Scan# 1394
Delta R.T. -0.01 min
Lab File: BG022052.D
Acq: 23 May 2016 18:37

Instrument :
BNA_G
ClientSampleId :
JHGJ3

Tgt Ion	Ratio	Resp	Lower	Upper
128	100	26228		
129	11.3		9.4	14.2
127	15.0		11.2	16.8




Manual Integrations
APPROVED


umangi
5/24/2016 7:37:14 PM

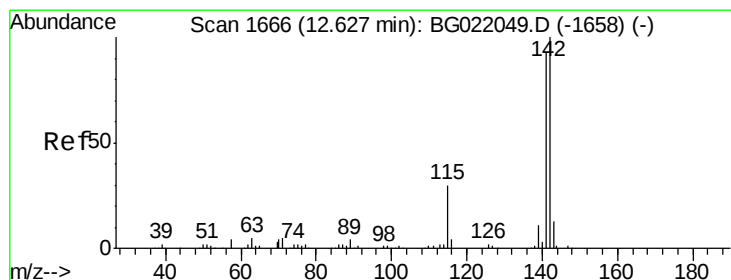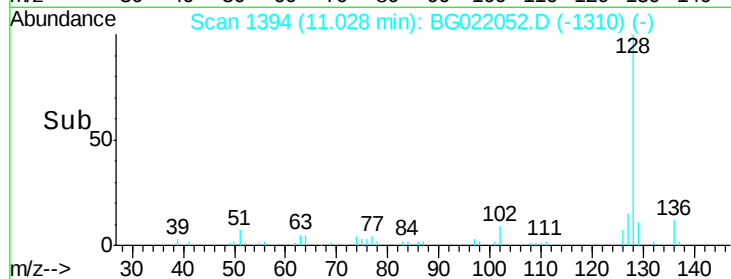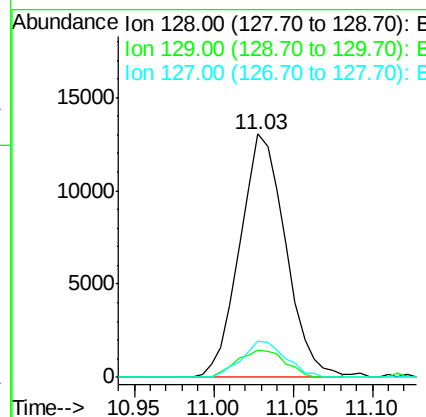

#34
2-Methylnaphthalene
Concen: 2.69 ng/ul
RT: 12.63 min Scan# 1666
Delta R.T. -0.00 min
Lab File: BG022052.D
Acq: 23 May 2016 18:37

Tgt Ion	Ratio	Resp	Lower	Upper
142	100	21144		
141	93.6		75.2	112.8

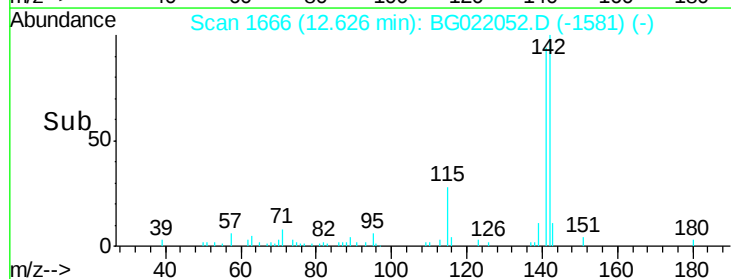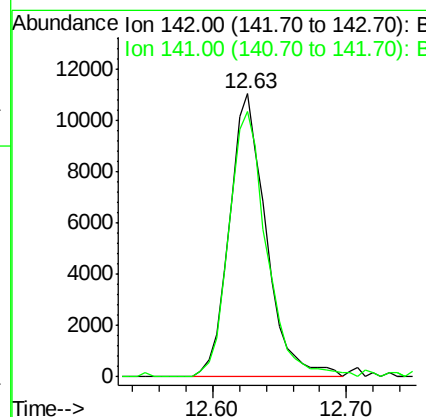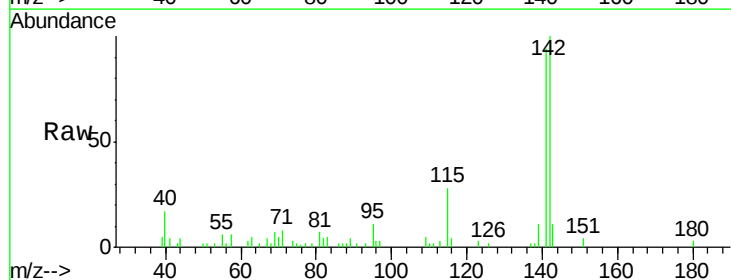

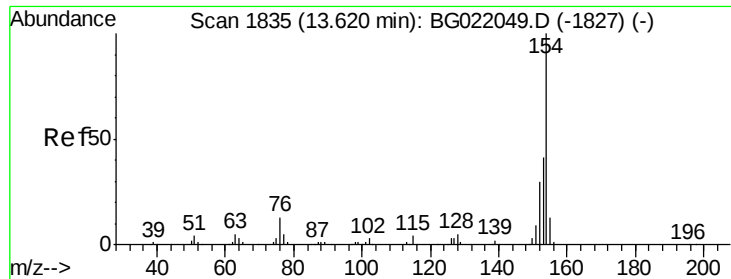





#40
 1,1'-Biphenyl
 Concen: 1.01 ng/ul
 RT: 13.62 min Scan# 1835
 Delta R.T. -0.00 min
 Lab File: BG022052.D
 Acq: 23 May 2016 18:37

Instrument :
 BNA_G
 ClientSampleId :
 JHGJ3

Tgt Ion:	154	Resp:	9495
Ion Ratio	Lower	Upper	
154	100		
153	40.4	34.6	52.0
76	11.0	11.9	17.9#




Manual Integrations
 APPROVED


umangi
 5/24/2016 7:37:14 PM

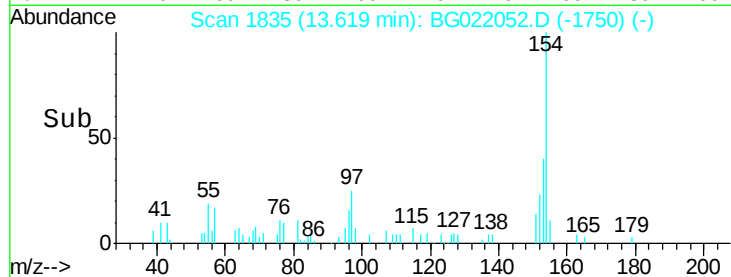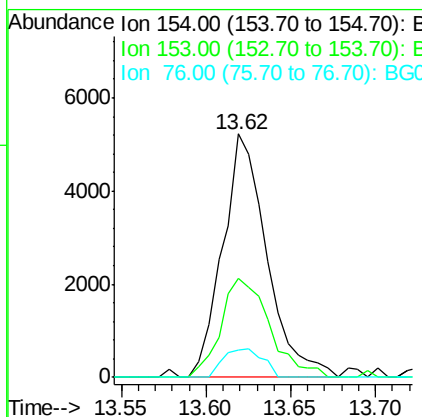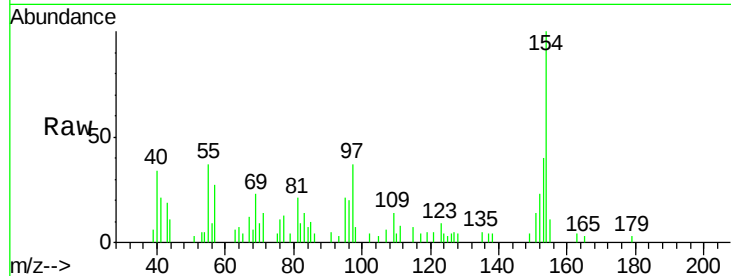

#44
 Dimethylphthalate
 Concen: 9.75 ng/ul
 RT: 14.22 min Scan# 1938
 Delta R.T. -0.01 min
 Lab File: BG022052.D
 Acq: 23 May 2016 18:37

Tgt Ion:	163	Resp:	83923
Ion Ratio	Lower	Upper	
163	100		
194	4.2	3.4	5.2
164	10.4	8.8	13.2

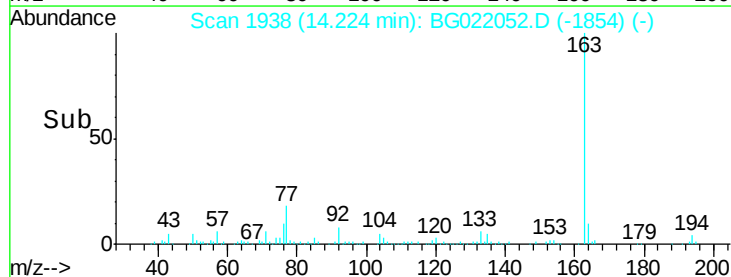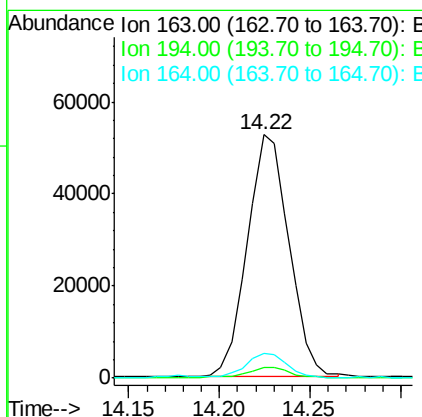

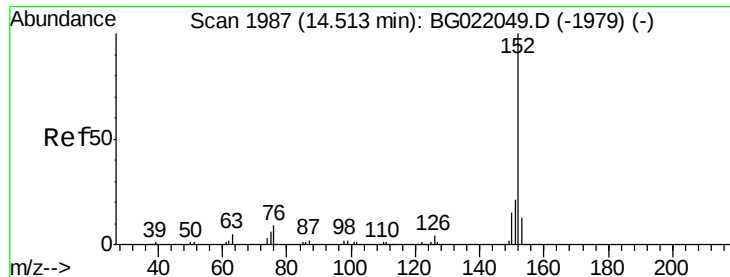

#47

Acenaphthylene

Concen: 2.86 ng/ul

RT: 14.51 min Scan# 1987

Delta R.T. -0.00 min

Lab File: BG022052.D


Acq: 23 May 2016 18:37

Instrument :

BNA_G

ClientSampleId :




JHGJ3

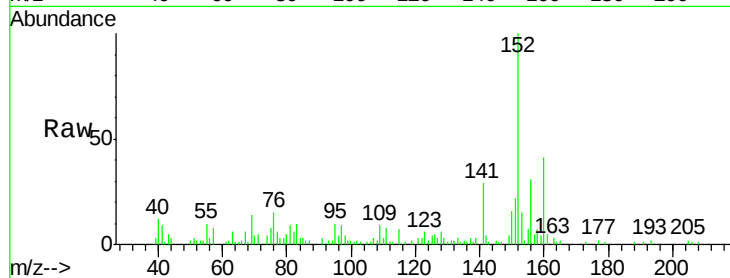

Tgt Ion:	152	Resp:	34890
Ion Ratio	Lower	Upper	
152	100		
151	21.5	17.5	26.3
153	15.2	11.1	16.7

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:14 PM

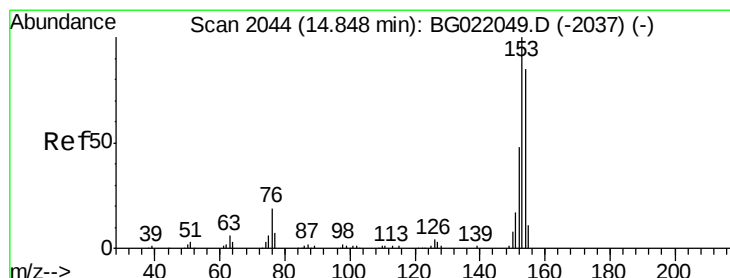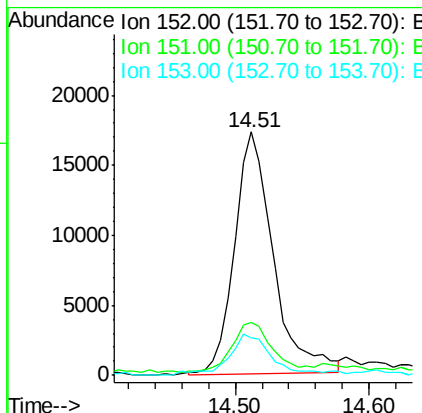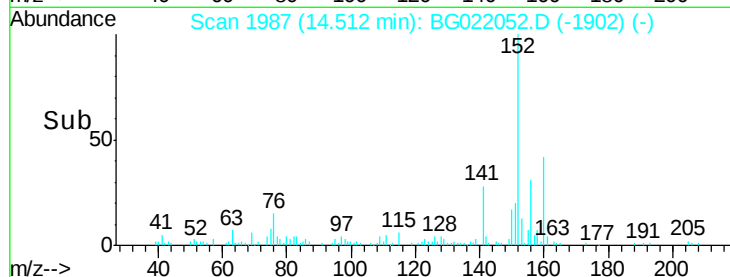

#49

Acenaphthene

Concen: 2.86 ng/ul




RT: 14.85 min Scan# 2044


Delta R.T. -0.00 min

Lab File: BG022052.D

Acq: 23 May 2016 18:37

Tgt Ion:	153	Resp:	24063
Ion Ratio	Lower	Upper	
153	100		
152	52.9	37.3	55.9
154	87.7	68.2	102.2

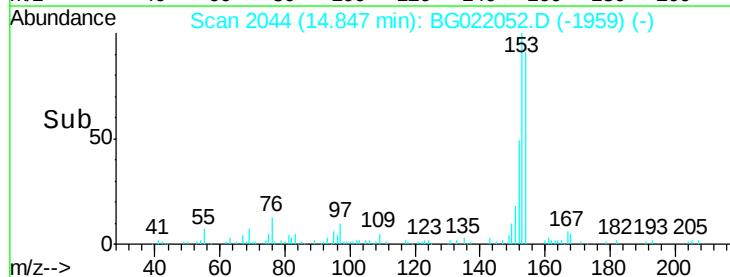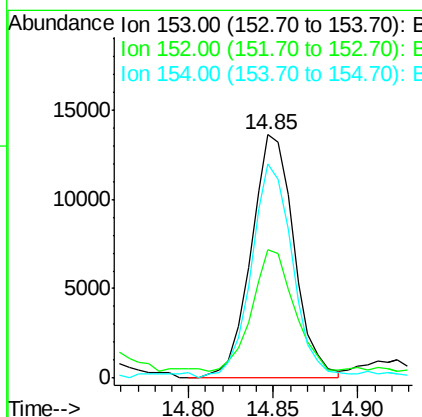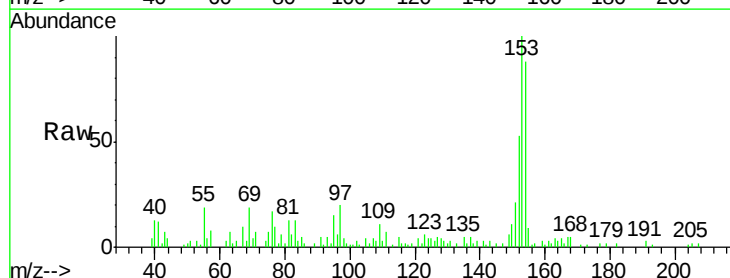

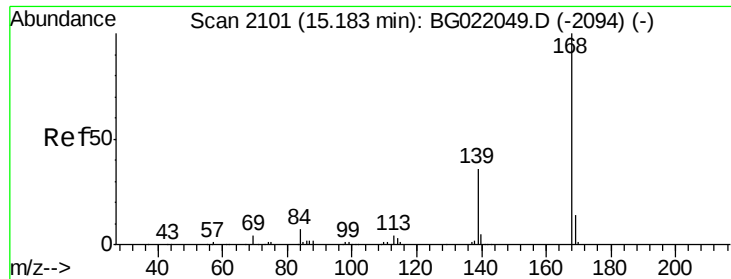

#53

Dibenzofuran

Concen: 1.80 ng/ul m

RT: 15.18 min Scan# 2101

Delta R.T. -0.00 min

Lab File: BG022052.D

Acq: 23 May 2016 18:37

Instrument :

BNA_G

ClientSampleId :

JHGJ3

Tgt Ion:168 Resp: 18770

Ion Ratio Lower Upper





168 100

139 42.3 27.4 41.0#

Manual Integrations
APPROVED

umangi

5/24/2016 7:37:14 PM

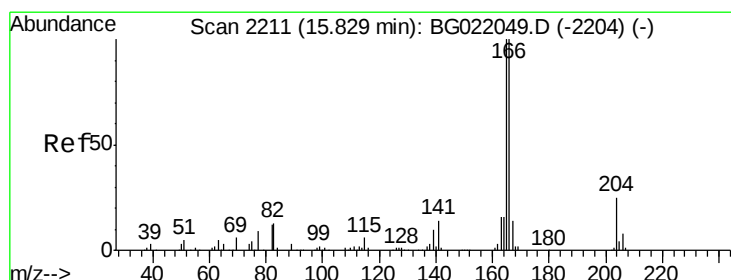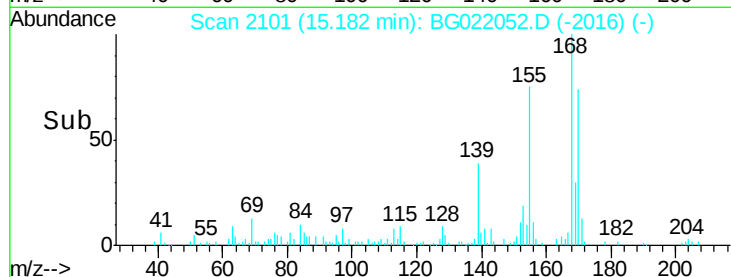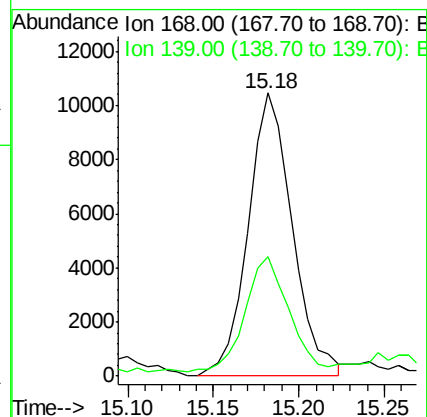

#58

Fluorene

Concen: 9.46 ng/ul

RT: 15.83 min Scan# 2211

Delta R.T. -0.00 min

Lab File: BG022052.D

Acq: 23 May 2016 18:37




Tgt Ion:166 Resp: 83181


Ion Ratio Lower Upper

166 100

165 99.1 80.3 120.5

167 12.2 10.3 15.5

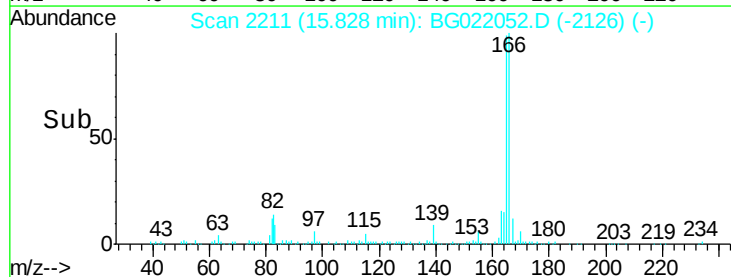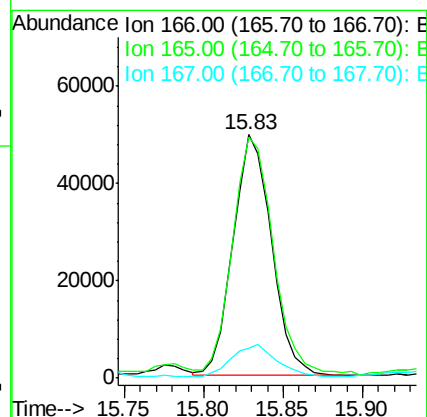

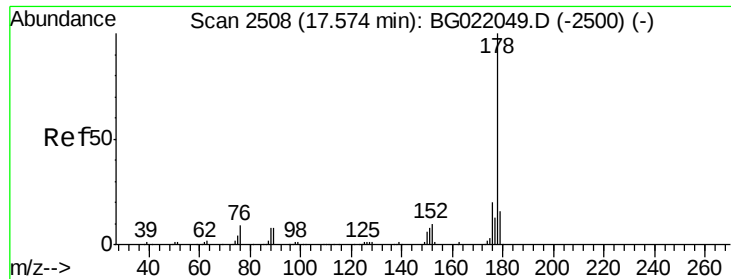

#69

Phenanthrene

Concen: 75.98 ng/ul

RT: 17.58 min Scan# 2509

Delta R.T. 0.00 min

Lab File: BG022052.D

Acq: 23 May 2016 18:37

Instrument :

BNA_G





ClientSampleId :

JHGJ3

Tgt Ion:	178	Resp:	910304
Ion Ratio	Lower	Upper	
178	100		
179	17.0	12.9	19.3
176	21.7	15.8	23.8

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:14 PM

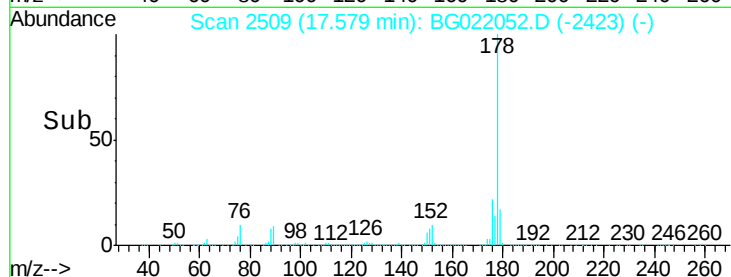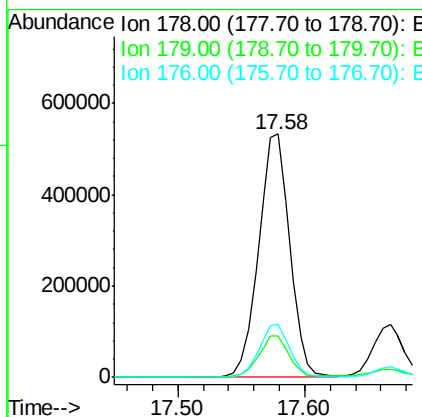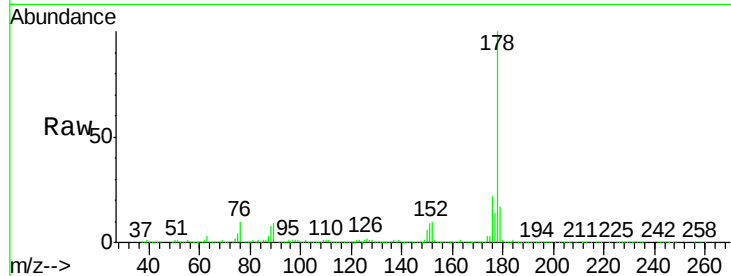

#71

Anthracene

Concen: 15.17 ng/ul




RT: 17.67 min Scan# 2524


Delta R.T. 0.00 min

Lab File: BG022052.D

Acq: 23 May 2016 18:37

Tgt Ion:	178	Resp:	184044
Ion Ratio	Lower	Upper	
178	100		
179	15.4	12.3	18.5
176	19.2	16.3	24.5

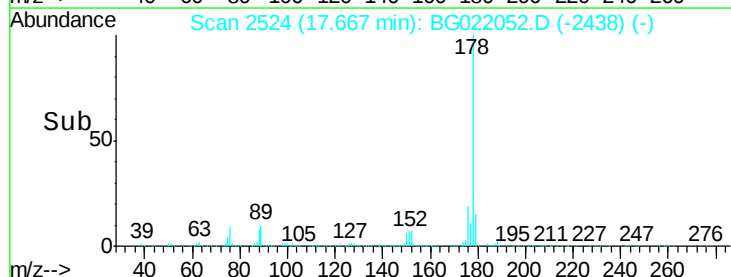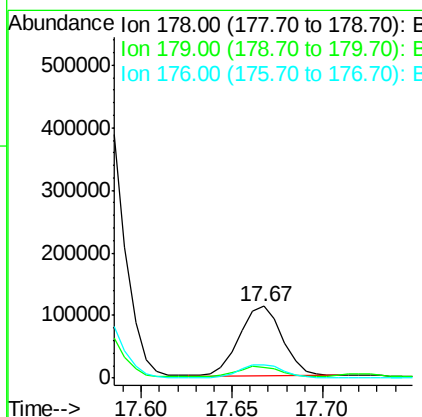

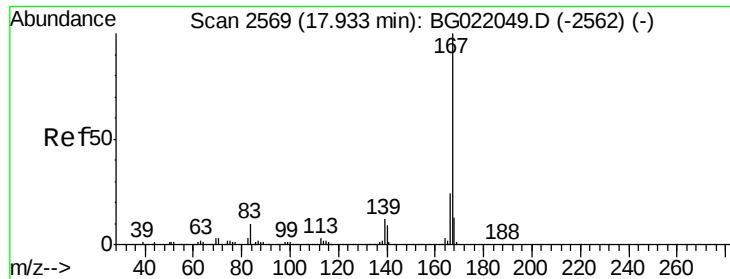





#72
 Carbazole
 Concen: 1.05 ng/ul
 RT: 17.94 min Scan# 2570
 Delta R.T. 0.01 min
 Lab File: BG022052.D
 Acq: 23 May 2016 18:37

Instrument :
 BNA_G
 ClientSampleId :
 JHGJ3

Tgt Ion	Ratio	Resp	Lower	Upper
167	100	11019		
166	30.8	19.2	28.8#	
139	20.5	10.2	15.4#	




Manual Integrations
 APPROVED


umangi
 5/24/2016 7:37:14 PM

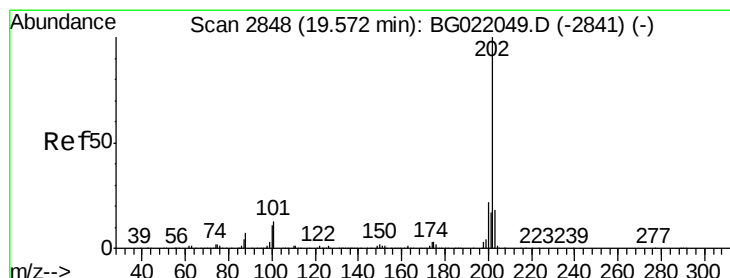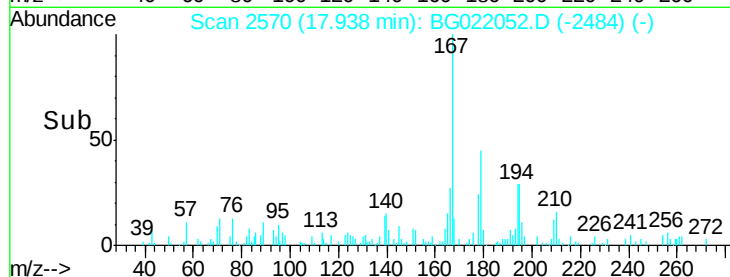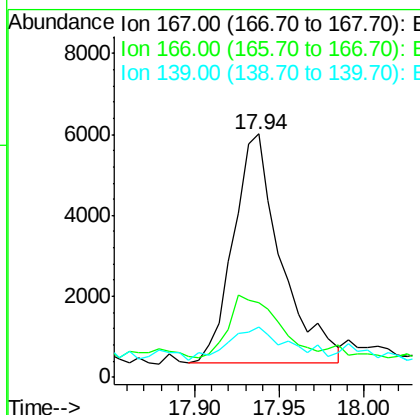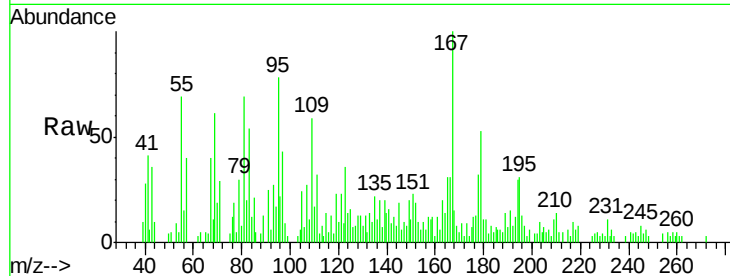

#74
 Fluoranthene
 Concen: 79.67 ng/ul
 RT: 19.58 min Scan# 2849
 Delta R.T. 0.01 min
 Lab File: BG022052.D
 Acq: 23 May 2016 18:37

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	975436		
101	14.1	10.6	16.0	
100	11.5	8.7	13.1	

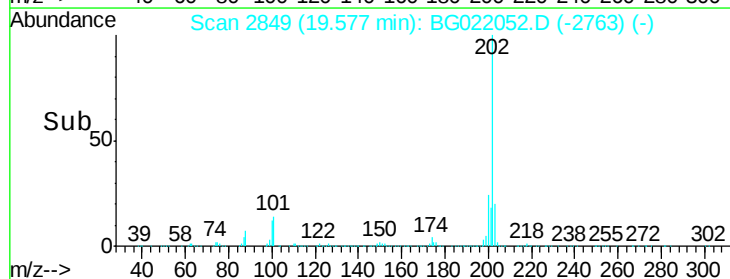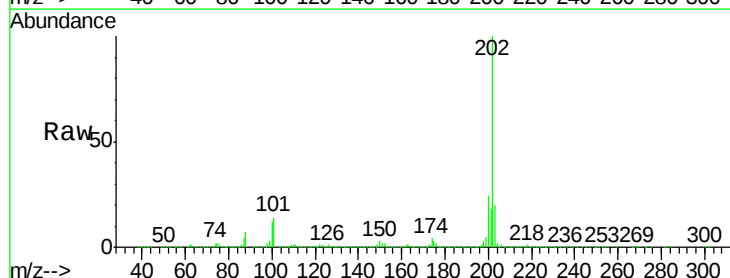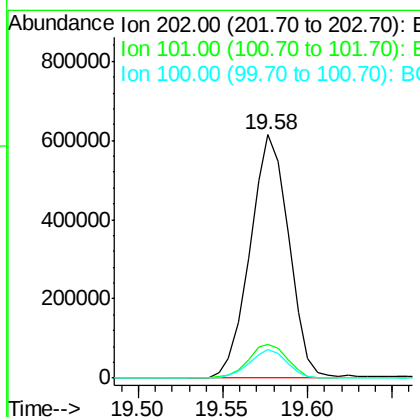

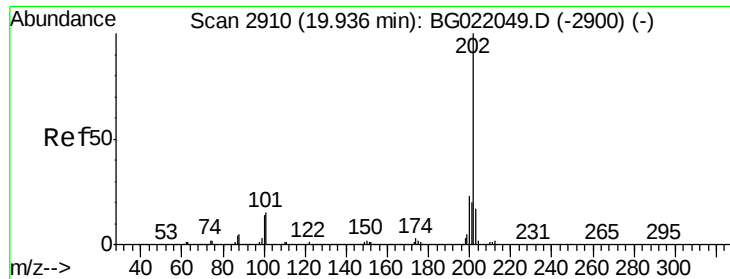

#77

Pyrene

Concen: 83.80 ng/ul m

RT: 19.94 min Scan# 2911

Delta R.T. 0.01 min

Lab File: BG022052.D

Acq: 23 May 2016 18:37

Instrument :

BNA_G





ClientSampleId :

JHGJ3

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:14 PM

Tgt	Ion	Ratio	Lower	Upper
202	100			
101	17.4	12.5	18.7	
100	15.4	10.2	15.4	

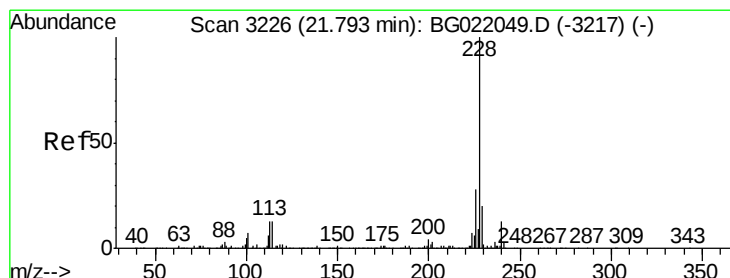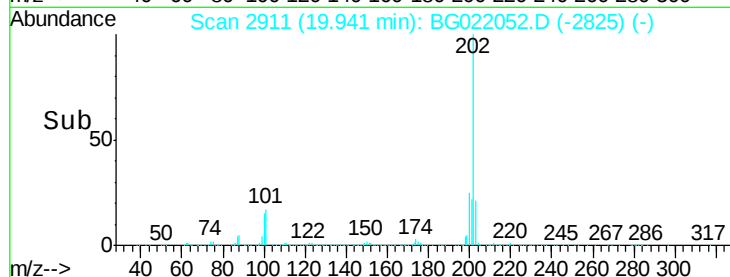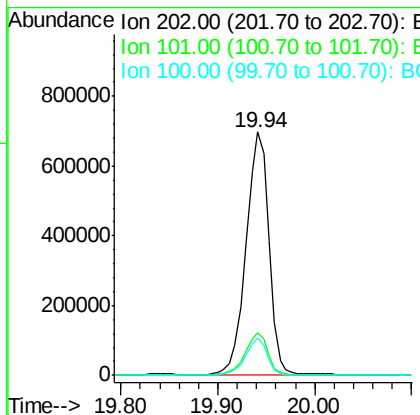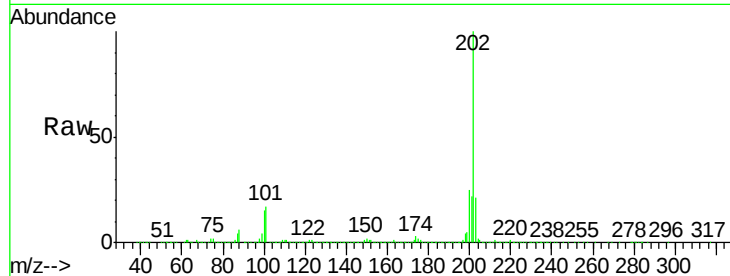

#80

Benzo(a)anthracene

Concen: 33.31 ng/ul




RT: 21.80 min Scan# 3227


Delta R.T. 0.01 min

Lab File: BG022052.D

Acq: 23 May 2016 18:37

Tgt	Ion	Ratio	Lower	Upper
228	100			
229	21.8	15.4	23.2	
226	31.2	22.8	34.2	

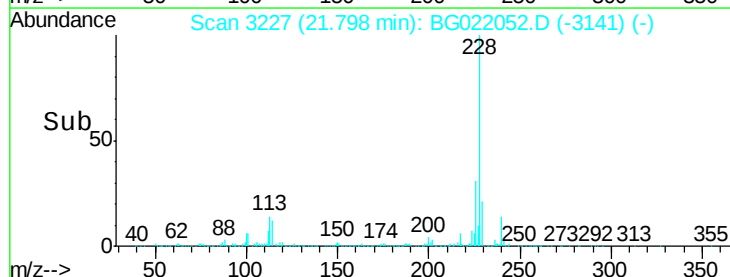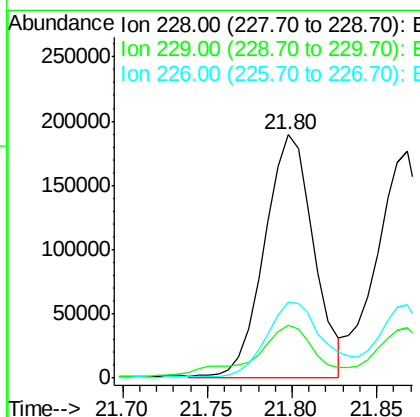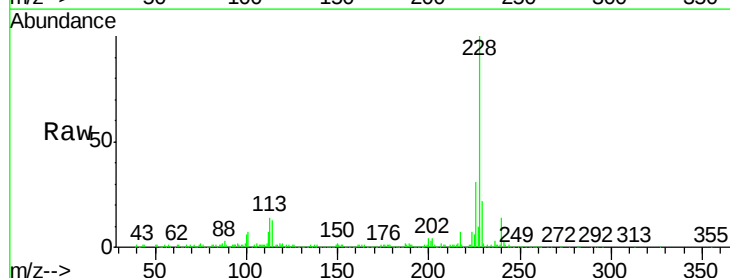

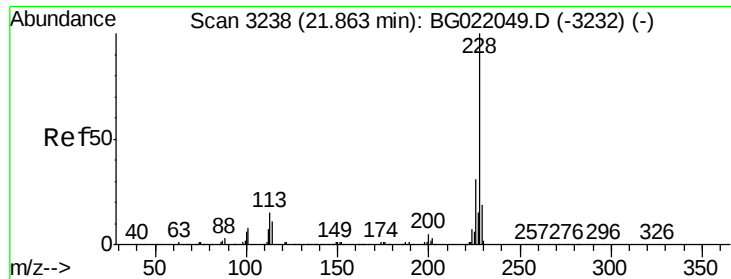





#82
Chrysene
Concen: 32.88 ng/u1
RT: 21.87 min Scan# 3239
Delta R.T. 0.00 min
Lab File: BG022052.D
Acq: 23 May 2016 18:37

Instrument :
BNA_G
ClientSampleId :
JHGJ3

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	362457		
226	32.2	24.2	36.4	
229	22.1	15.0	22.6	




Manual Integrations
APPROVED


umangi
5/24/2016 7:37:14 PM

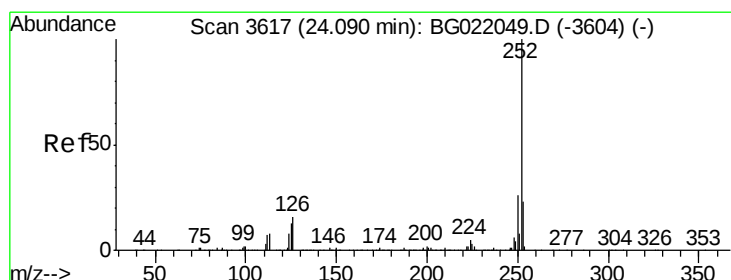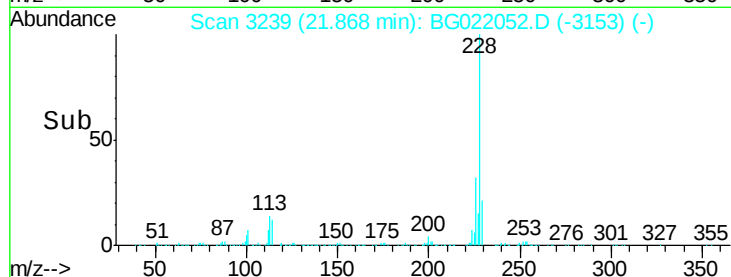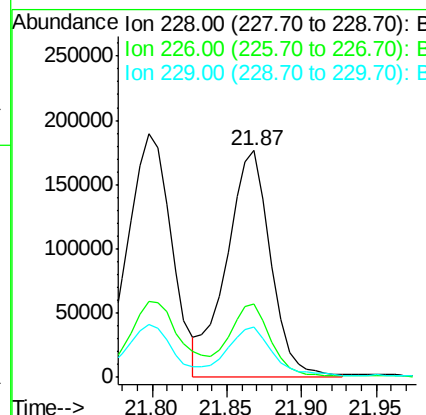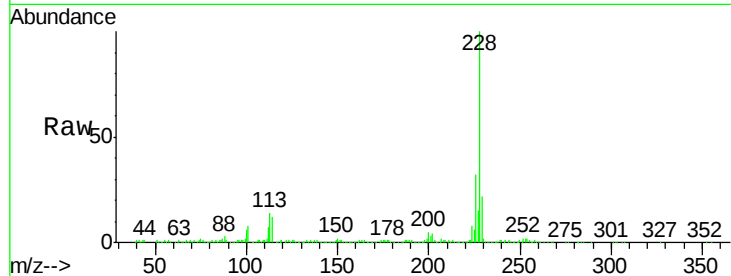

#85
Benzo(b)fluoranthene
Concen: 33.13 ng/u1
RT: 24.10 min Scan# 3619
Delta R.T. 0.01 min
Lab File: BG022052.D
Acq: 23 May 2016 18:37

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	354978		
253	23.9	18.2	27.2	
125	17.0	10.8	16.2	

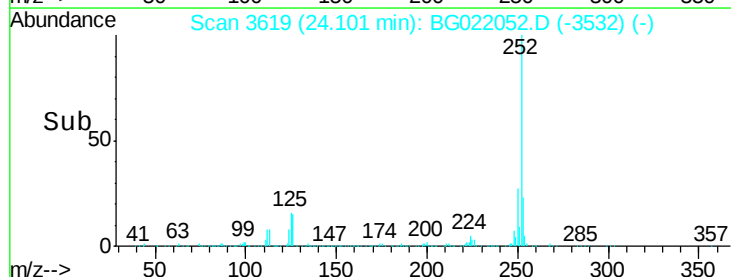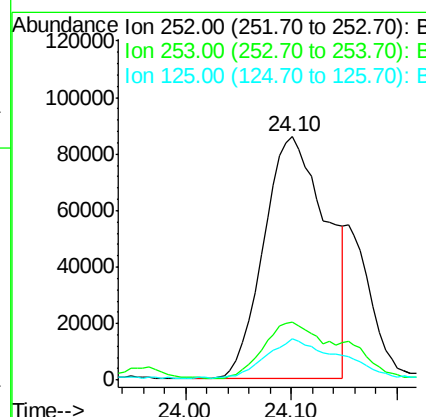

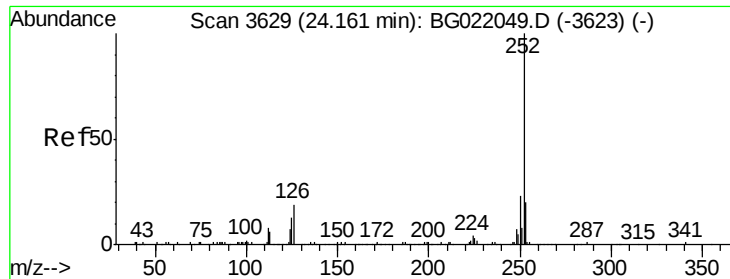

#86

Benzo(k)fluoranthene

Concen: 9.07 ng/ul m

RT: 24.15 min Scan# 3628

Delta R.T. -0.01 min

Lab File: BG022052.D

Acq: 23 May 2016 18:37

Instrument :

BNA_G





ClientSampleId :

JHGJ3

Tgt Ion:	252	Resp:	94587
Ion Ratio	Lower	Upper	
252	100		
253	25.4	15.8	23.6#
125	14.8	10.6	16.0

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:14 PM

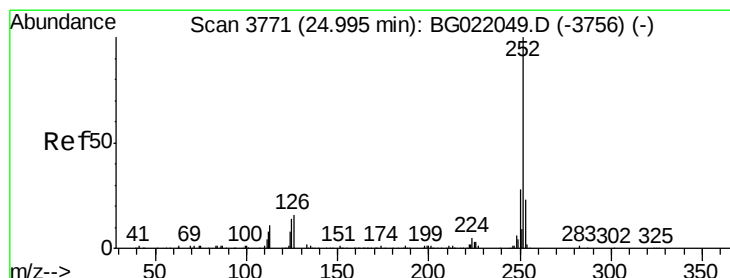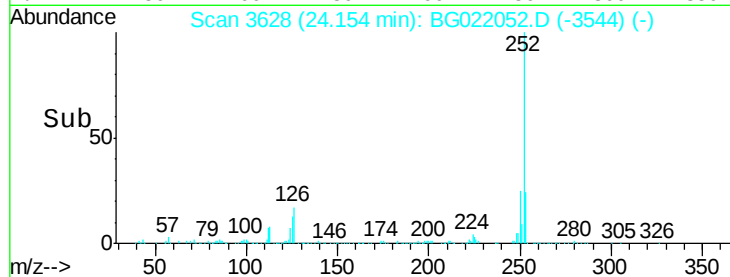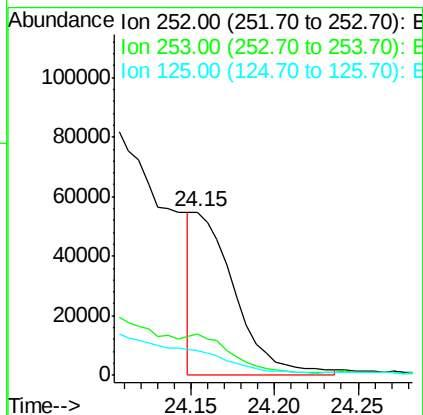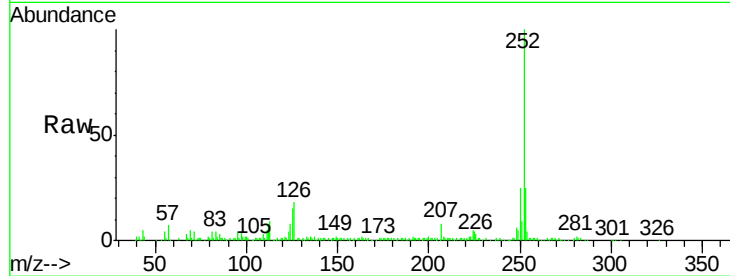

#88

Benzo(a)pyrene

Concen: 30.34 ng/ul




RT: 25.00 min Scan# 3772


Delta R.T. 0.00 min

Lab File: BG022052.D

Acq: 23 May 2016 18:37

Tgt Ion:	252	Resp:	313672
Ion Ratio	Lower	Upper	
252	100		
253	23.2	19.0	28.4
125	15.1	12.0	18.0

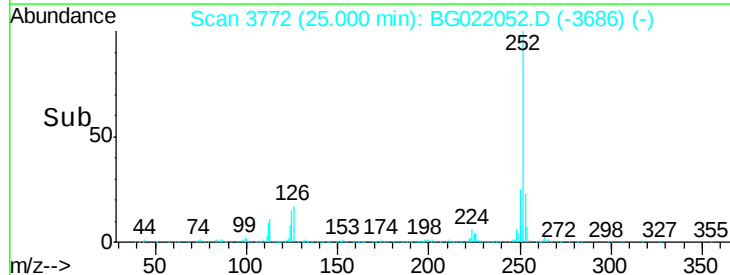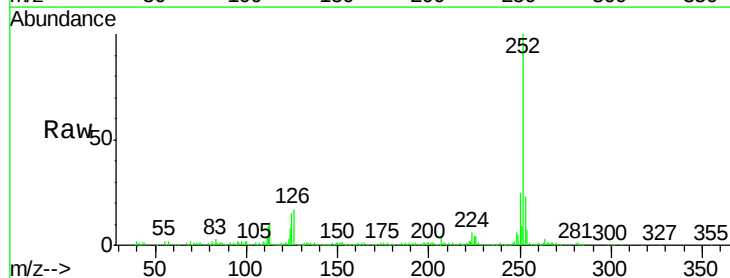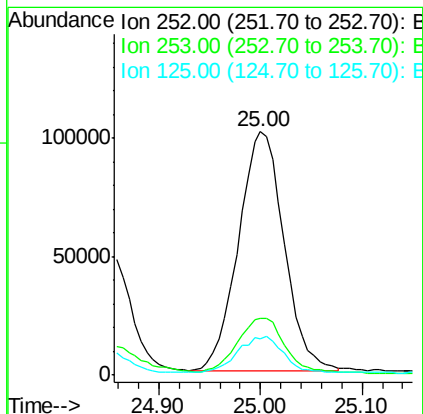

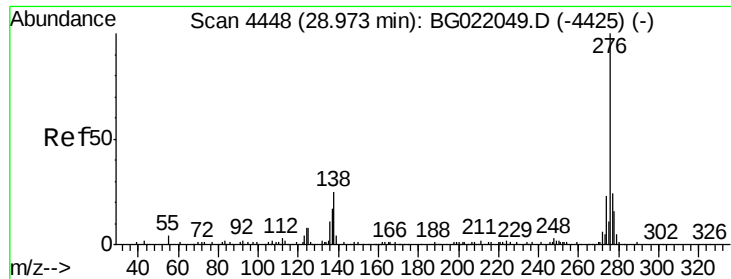

#89

Indeno(1,2,3-cd)pyrene

Concen: 12.55 ng/ul

RT: 28.98 min Scan# 4450

Delta R.T. 0.01 min

Lab File: BG022052.D

Acq: 23 May 2016 18:37

Instrument :

BNA_G





ClientSampleId :

JHGJ3

Tgt Ion:	276	Resp:	148720
Ion Ratio		Lower	Upper
276	100		
138	26.4	20.8	31.2
277	24.7	17.6	26.4

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:14 PM

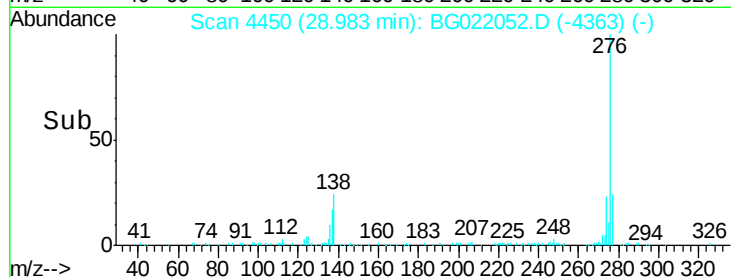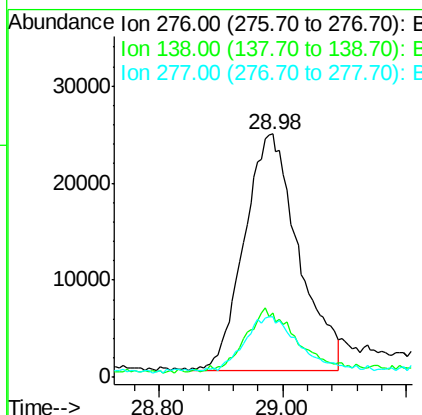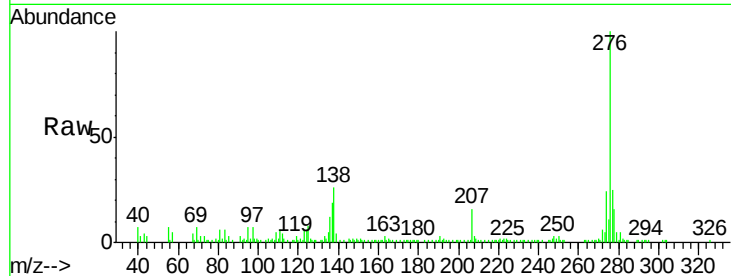

#90

Dibenzo(a,h)anthracene

Concen: 3.86 ng/ul m




RT: 29.04 min Scan# 4459


Delta R.T. -0.01 min

Lab File: BG022052.D

Acq: 23 May 2016 18:37

Tgt Ion:	278	Resp:	38319
Ion Ratio		Lower	Upper
278	100		
139	25.7	16.3	24.5#
279	29.8	19.1	28.7#

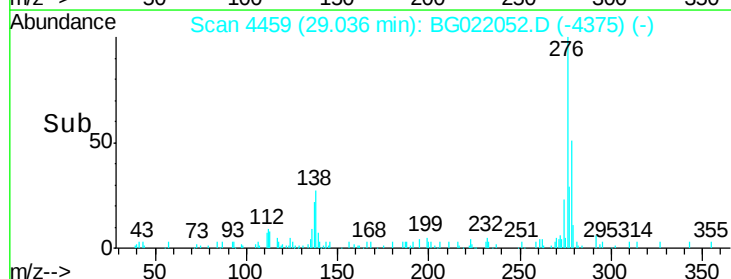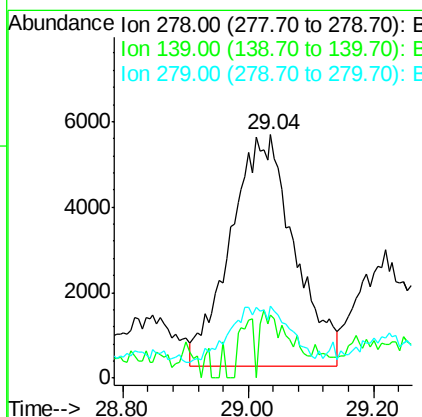

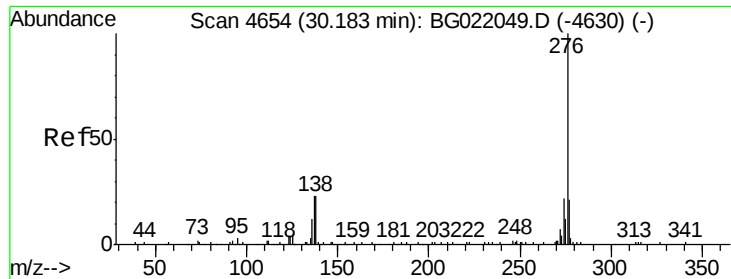

#91

Benzo(g,h,i)perylene

Concen: 12.63 ng/ul

RT: 30.18 min Scan# 4654

Delta R.T. -0.00 min

Lab File: BG022052.D


Acq: 23 May 2016 18:37

Instrument :

BNA_G

ClientSampleId :

JHGJ3

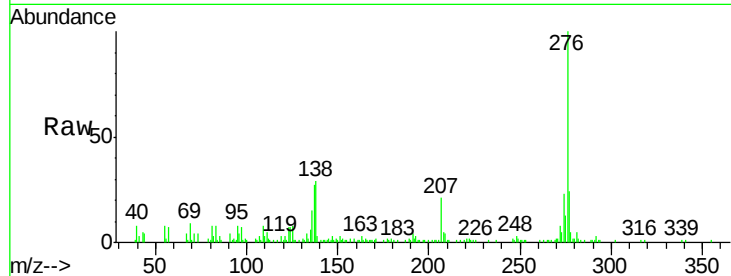

Tgt Ion	Ratio	Lower	Upper
276	100		
138	29.2	22.1	33.1
277	23.7	17.0	25.4

Manual Integrations
APPROVED

umangi
5/24/2016 7:37:14 PM

