

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\Data\BG052317\
 Data File : BG027062.D
 Acq On : 22 May 2017 17:38
 Operator : SJ/MA
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 23 02:36:04 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG051817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 23:42:44 2017
 Response via : Initial Calibration

Instrument :
 BNA_G
LabSampleId :
 SSTD02055

Manual Integrations
APPROVED

mohammad
 5/24/2017 11:21:51 AM

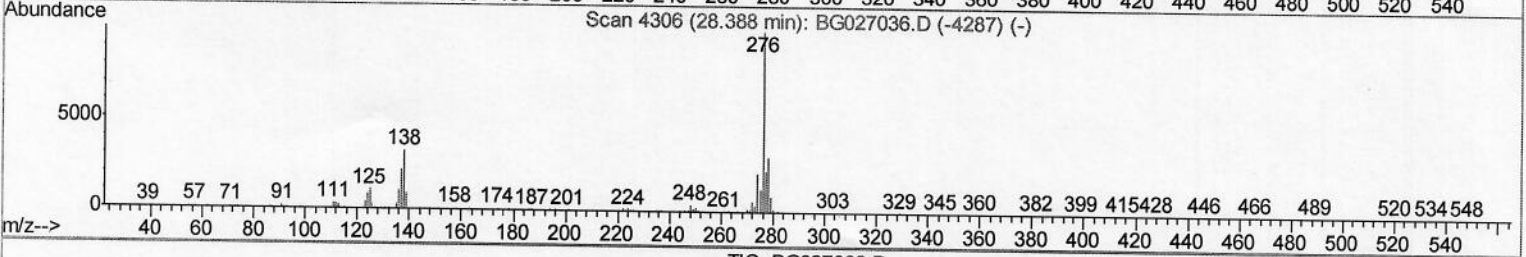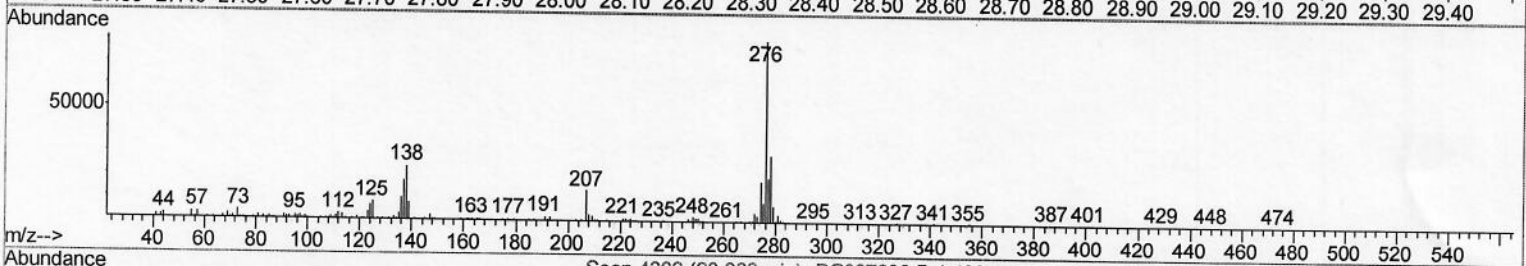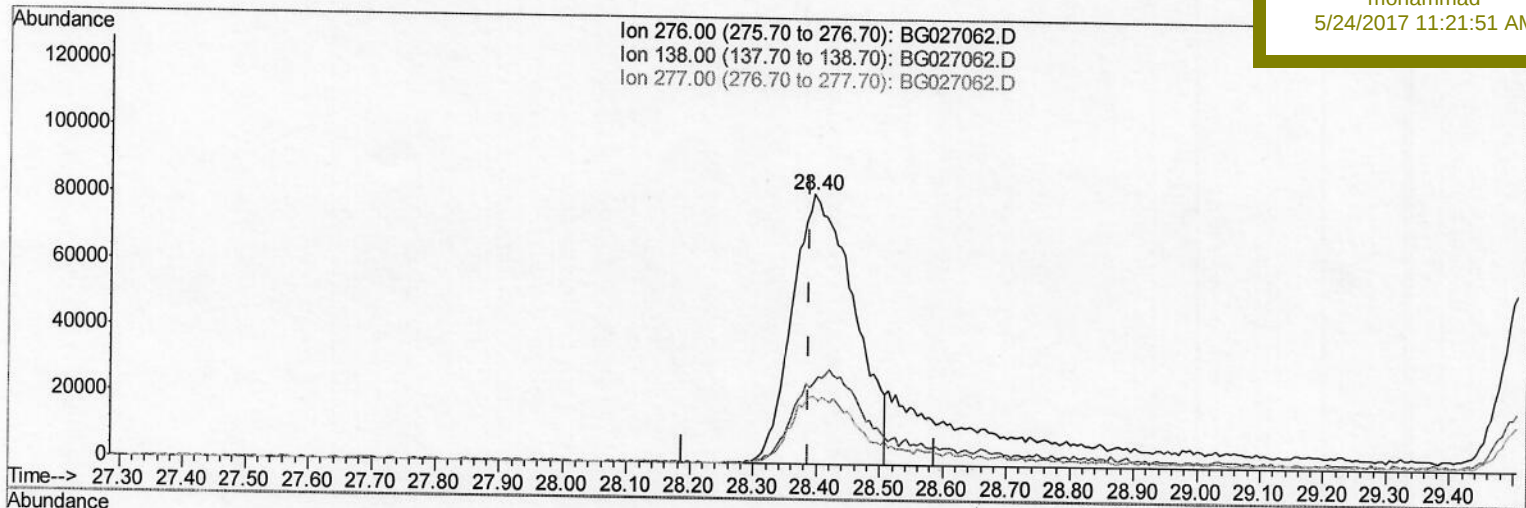

TIC: BG027062.D

(27) Indeno(1,2,3-cd)pyrene
 28.396min (+0.008) 16.04ng/ul
 response 549207

Ion	Exp%	Act%
276.00	100	100
138.00	18.00	29.59#
277.00	22.50	25.10
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\Data\BG052317\
 Data File : BG027062.D
 Acq On : 22 May 2017 17:38
 Operator : SJ/MA
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 23 02:36:04 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG051817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 23:42:44 2017
 Response via : Initial Calibration

Instrument :
 BNA_G
 LabSampleId :
 SSTD02055

Manual Integrations
 APPROVED

mohammad
 5/24/2017 11:21:51 AM

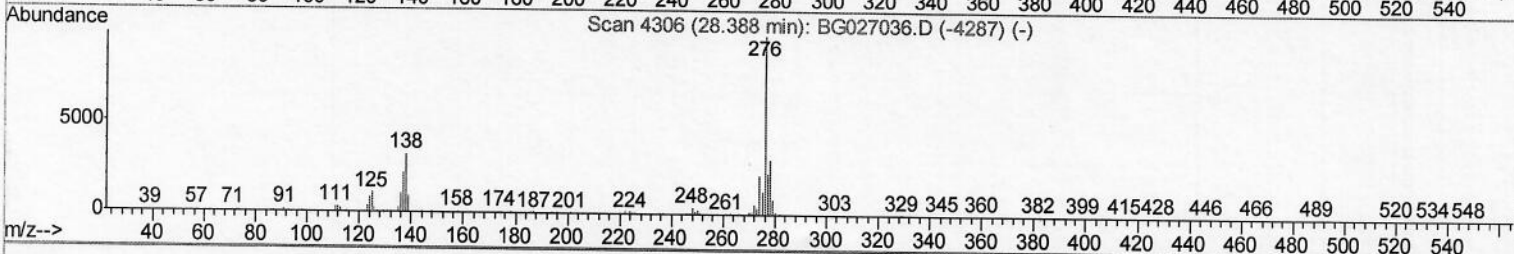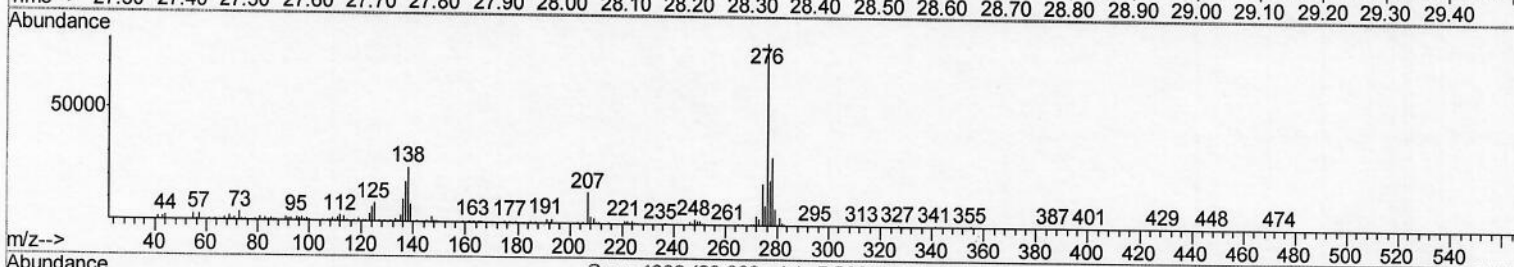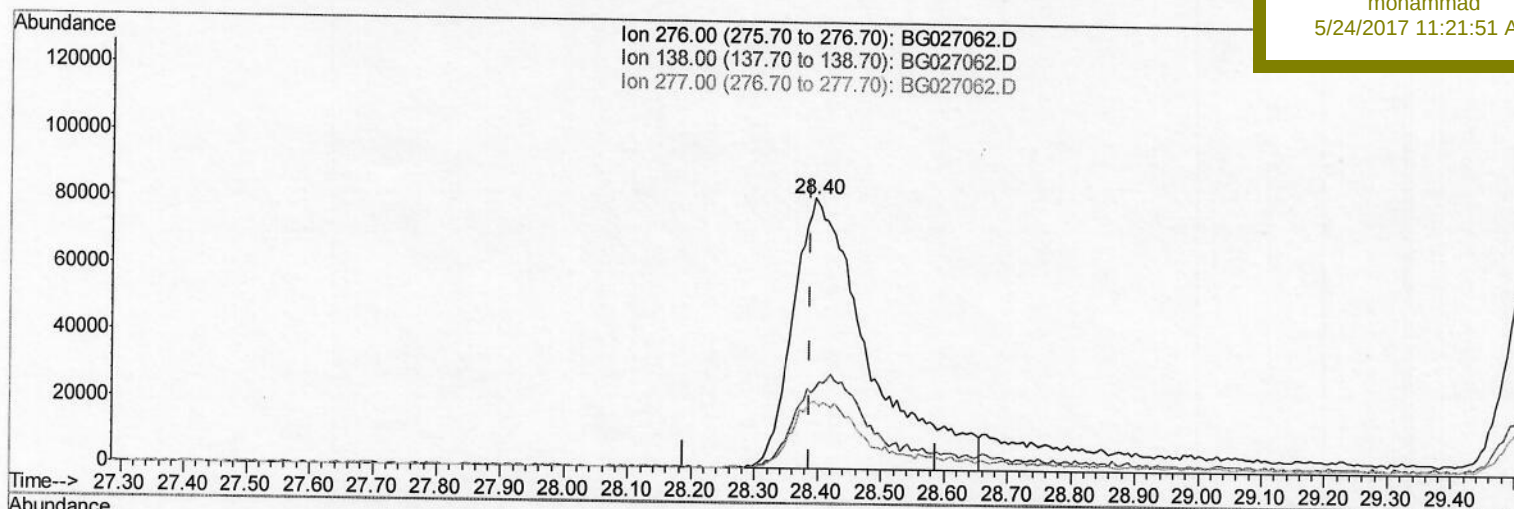

(27) Indeno(1,2,3-cd)pyrene

28.396min (+0.008) 19.75ng/ul m

response 676300

Ion Exp% Act%

276.00 100 100

138.00 18.00 29.59#

277.00 22.50 25.10

0.00 0.00 0.00

> 5.7
 05/30/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\Data\BG052317\
 Data File : BG027062.D
 Acq On : 22 May 2017 17:38
 Operator : SJ/MA
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 23 02:36:04 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG051817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 23:42:44 2017
 Response via : Initial Calibration

Instrument :
 BNA_G
 LabSampleId :
 SSTD02055

Manual Integrations
 APPROVED

mohammad
 5/24/2017 11:21:51 AM

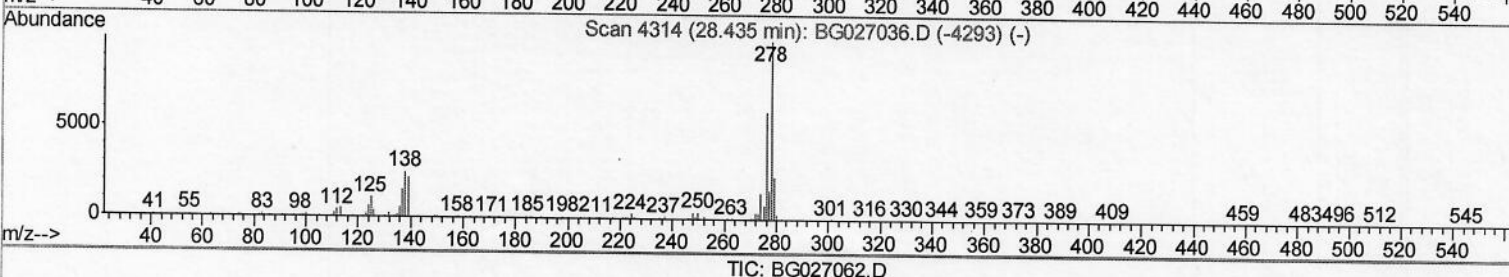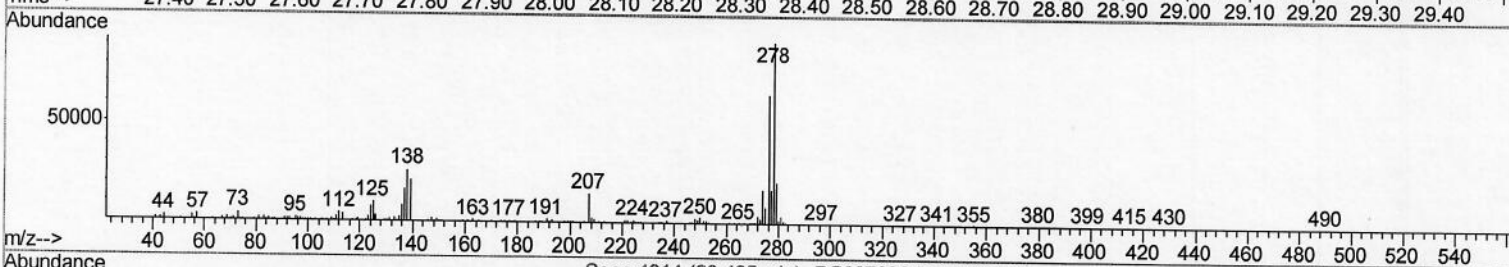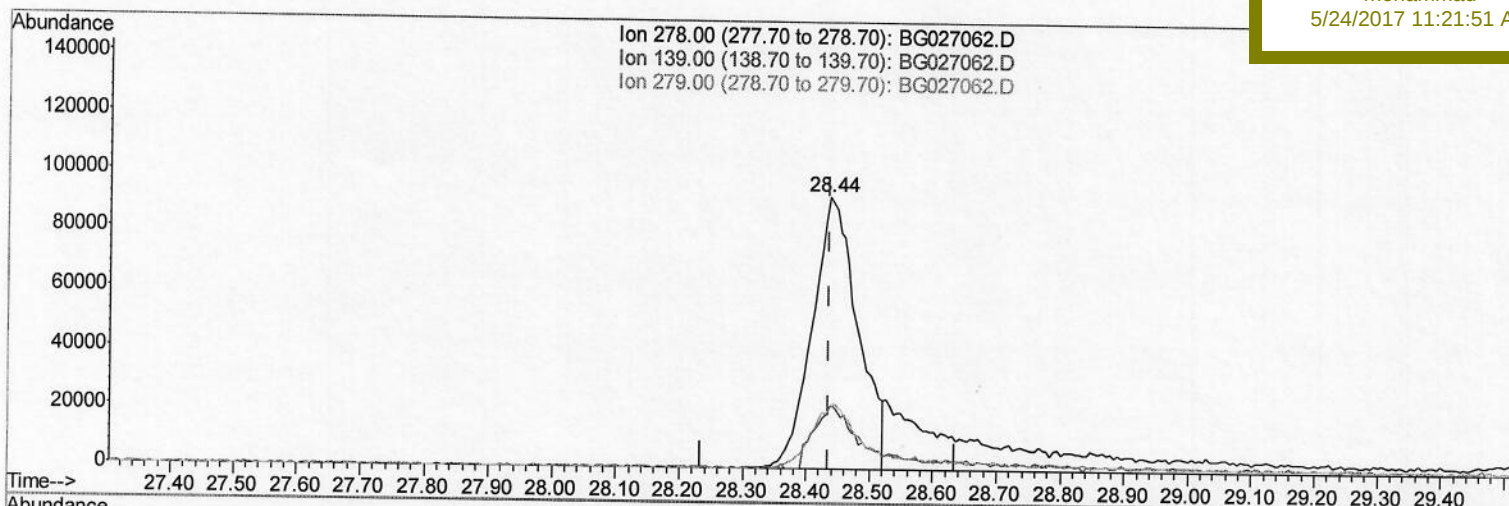

TIC: BG027062.D

(28) Dibenzo(a,h)anthracene

28.437min (+0.002) 15.64ng/ul

response 462209

Ion	Exp%	Act%
278.00	100	100
139.00	15.30	23.00#
279.00	24.00	22.99
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\Data\BG052317\
 Data File : BG027062.D
 Acq On : 22 May 2017 17:38
 Operator : SJ/MA
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 23 02:36:04 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG051817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 23:42:44 2017
 Response via : Initial Calibration

Instrument :
 BNA_G
 LabSampleId :
 SSTD02055

Manual Integrations
 APPROVED

mohammad
 5/24/2017 11:21:51 AM

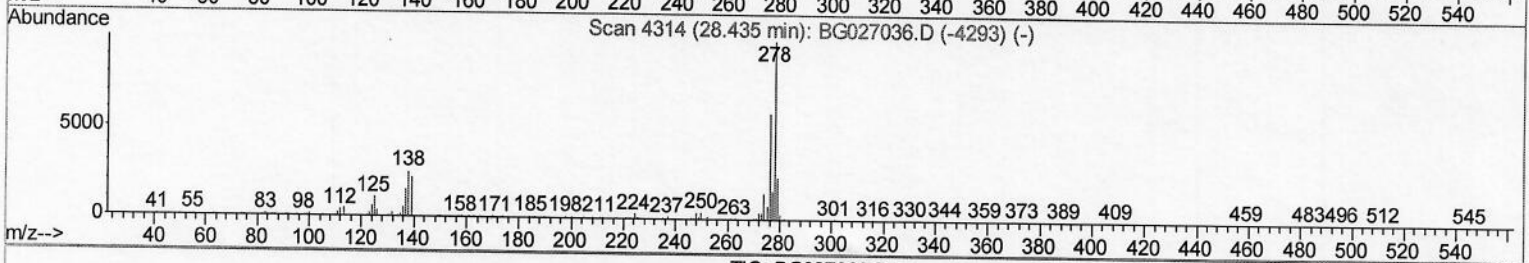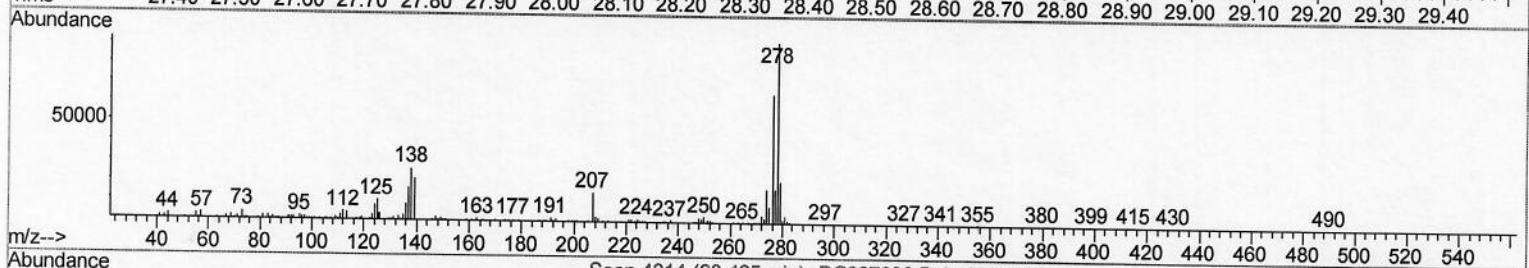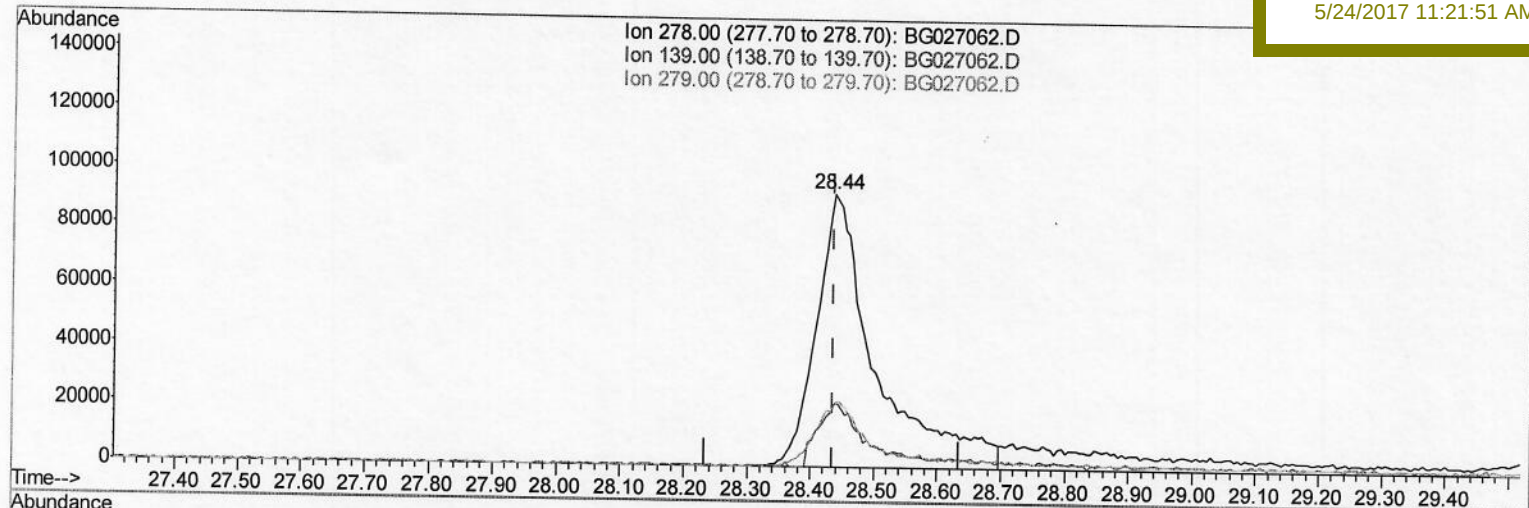

TIC: BG027062.D

(28) Dibenzo(a,h)anthracene

28.437min (+0.002) 20.48ng/ul m

response 605134

Ion	Exp%	Act%
278.00	100	100
139.00	15.30	23.00#
279.00	24.00	22.99
0.00	0.00	0.00

29.7
 05/30/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\Data\BG052317\
Data File : BG027062.D
Acq On : 22 May 2017 17:38
Operator : SJ/MA
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 23 02:36:04 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG051817MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 23:42:44 2017
Response via : Initial Calibration

Instrument :
BNA_G
LabSampleId :
SSTD02055

Manual Integrations
APPROVED

mohammad
5/24/2017 11:21:51 AM

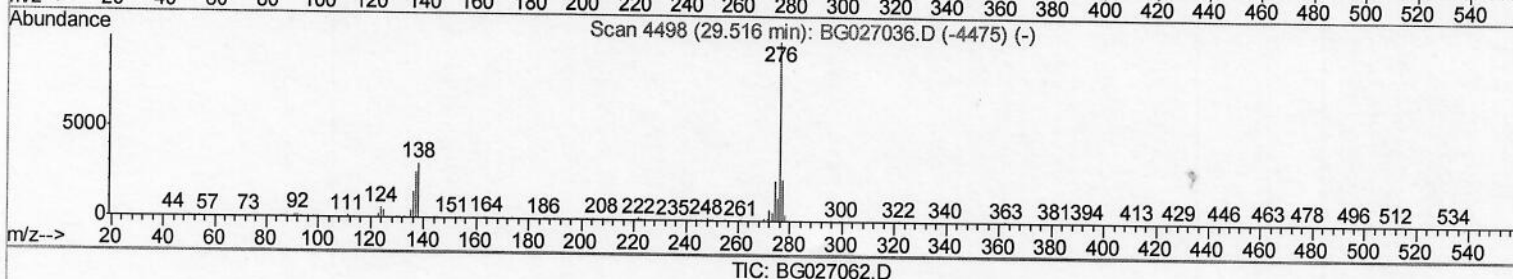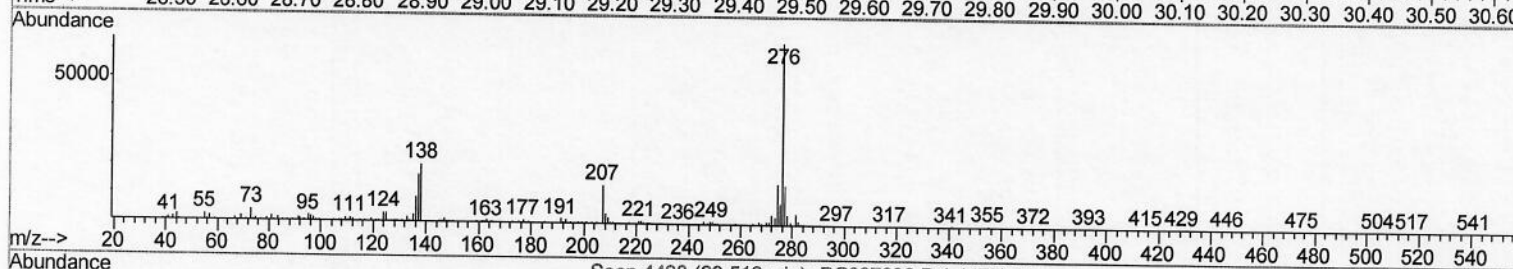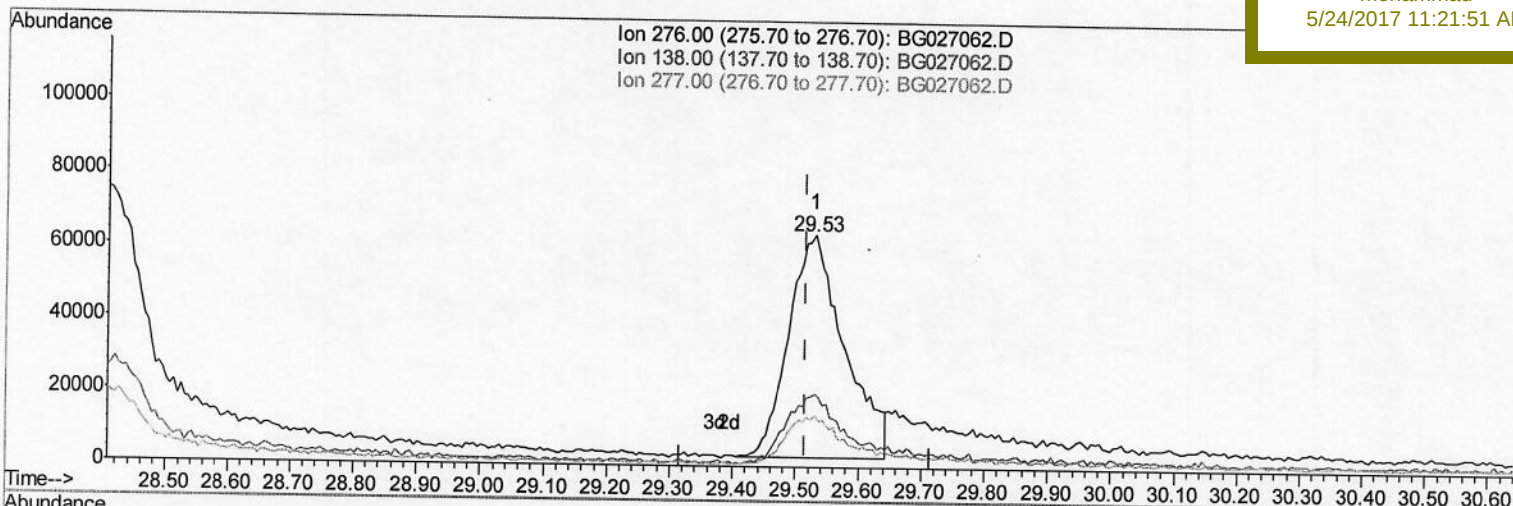

(29) Benzo(g,h,i)perylene

29.530min (+0.014) 13.78ng/ul

response 375293

Ion	Exp%	Act%
276.00	100	100
138.00	19.10	32.00#
277.00	23.70	22.43
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\Data\BG052317\
 Data File : BG027062.D
 Acq On : 22 May 2017 17:38
 Operator : SJ/MA
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 23 02:36:04 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG051817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 23:42:44 2017
 Response via : Initial Calibration

Instrument :
 BNA_G
 LabSampleId :
 SSTD02055

Manual Integrations
 APPROVED

mohammad
 5/24/2017 11:21:51 AM

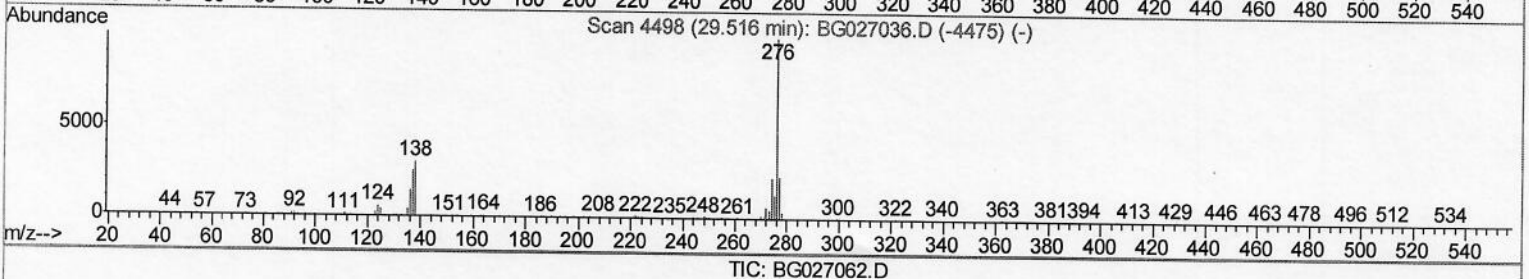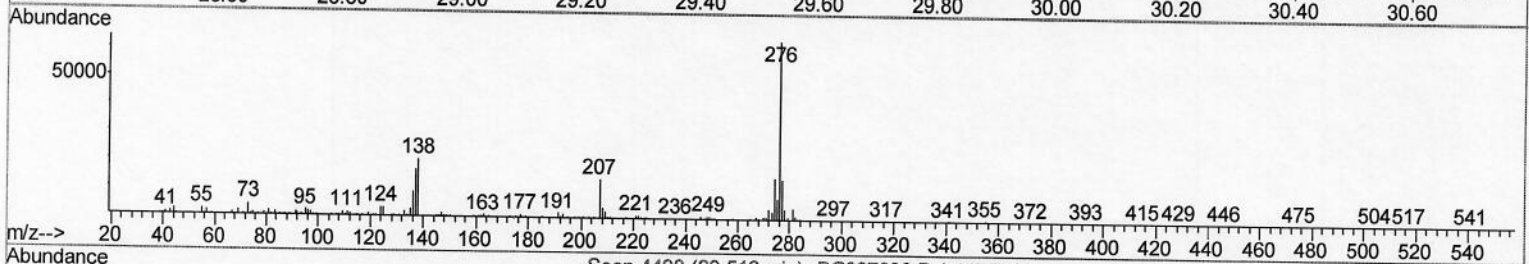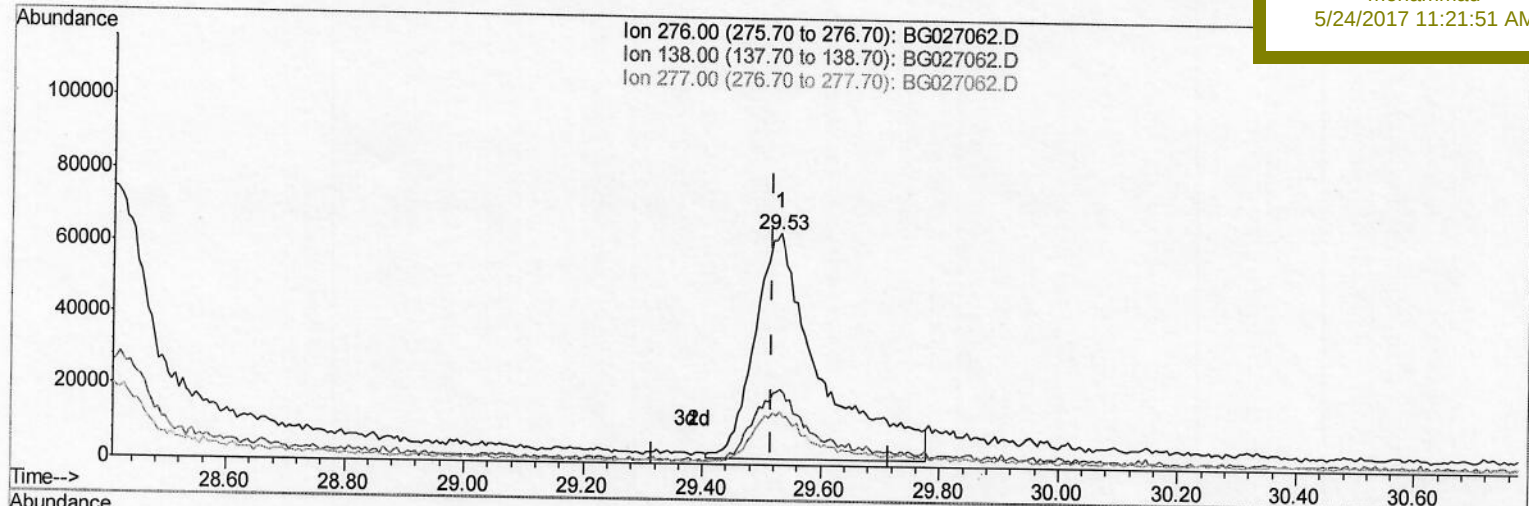

(29) Benzo(g,h,i)perylene

29.530min (+0.014) 17.48ng/ul m

response 476038

Ion	Exp%	Act%
276.00	100	100
138.00	19.10	32.00#
277.00	23.70	22.43
0.00	0.00	0.00

> 9.7
 05/30/17

Data Path : Z:\HPCHEM1\BNA G\Data\BG052317\
 Data File : BG027062.D
 Acq On : 22 May 2017 17:38
 Operator : SJ/MA
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTD02055

Quant Time: May 23 02:42:00 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG051817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 19 23:42:44 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 5/24/2017 11:21:51 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	175943	20.00	ng/ul	0.00
2) Naphthalene-d8	10.80	136	844943	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.62	164	439736	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.36	188	823069	20.00	ng/ul	0.00
17) Chrysene-d12	21.60	240	729656	20.00	ng/ul	0.00
22) Perylene-d12	24.77	264	640155	20.00	ng/ul	0.00

System Monitoring Compounds

7) Acenaphthylene-d8	14.31	160	937780	20.79	ng/ul	0.00
10) Fluorene-d10	15.60	176	617080	20.51	ng/ul	0.00
14) Anthracene-d10	17.46	188	822430	20.49	ng/ul	0.00
18) Perylene-d10	19.74	212	777814	20.42	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.56	264	668679	21.02	ng/ul	0.00

Target Compounds

						Ovalue
3) Naphthalene	10.86	128	896497	20.45	ng/ul	99
4) 2-Methylnaphthalene	12.46	142	656111	20.20	ng/ul	100
5) 1-Methylnaphthalene	12.67	142	701045	20.05	ng/ul#	96
8) Acenaphthylene	14.34	152	943245	20.81	ng/ul	98
9) Acenaphthene	14.68	153	649873	20.94	ng/ul	98
11) Fluorene	15.66	166	667264	20.18	ng/ul	97
13) Phenanthrene	17.40	178	949077	20.63	ng/ul	97
15) Anthracene	17.49	178	972217	20.57	ng/ul	98
16) Fluoranthene	19.41	202	973800	20.70	ng/ul#	93
19) Pyrene	19.76	202	993922	20.84	ng/ul#	86
20) Benzo(a)anthracene	21.59	228	892450	20.30	ng/ul	95
21) Chrysene	21.65	228	819990	20.32	ng/ul	99
23) Benzo(b)fluoranthene	23.77	252	807832	21.23	ng/ul#	95
24) Benzo(k)fluoranthene	23.83	252	860039	21.98	ng/ul#	95
26) Benzo(a)pyrene	24.63	252	792038	21.28	ng/ul#	92
27) Indeno(1,2,3-cd)pyrene	28.40	276	676300m	19.75	ng/ul	
28) Dibenzo(a,h)anthracene	28.44	278	605134m	20.48	ng/ul	
29) Benzo(a,h,i)perylene	29.53	276	476038m	17.48	ng/ul	

2 9.9
 05/30/17

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\Data\BG052317\
Data File : BG027062.D
Acq On : 22 May 2017 17:38
Operator : SJ/MA
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 23 02:42:00 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG051817MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 19 23:42:44 2017
Response via : Initial Calibration

Instrument :
BNA_G
LabSampleId :
SSTD02055

Manual Integrations
APPROVED

mohammad
5/24/2017 11:21:51 AM

