
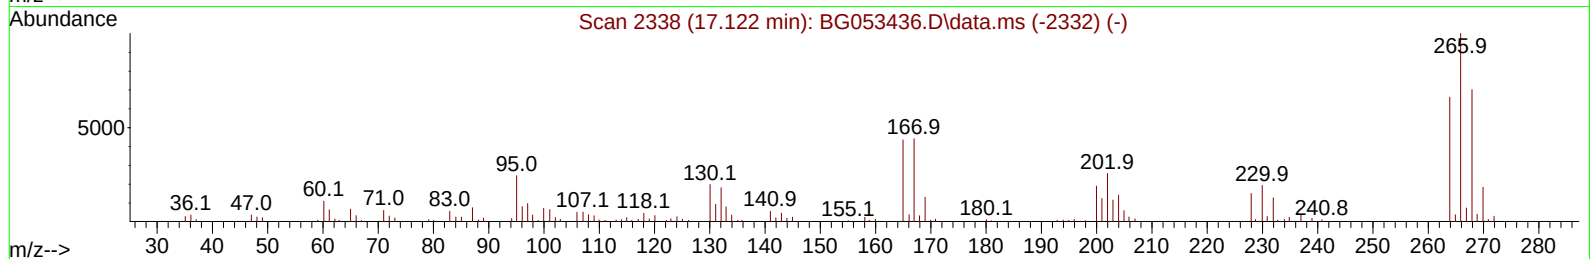
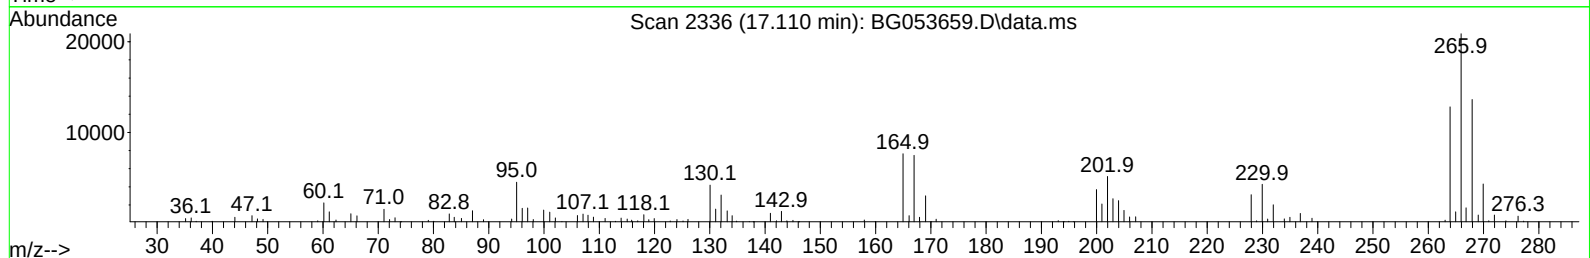


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052322\
Data File : BG053659.D
Acq On : 23 May 2022 9:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 06:25:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 24 05:05:32 2022
Response via : Initial Calibration

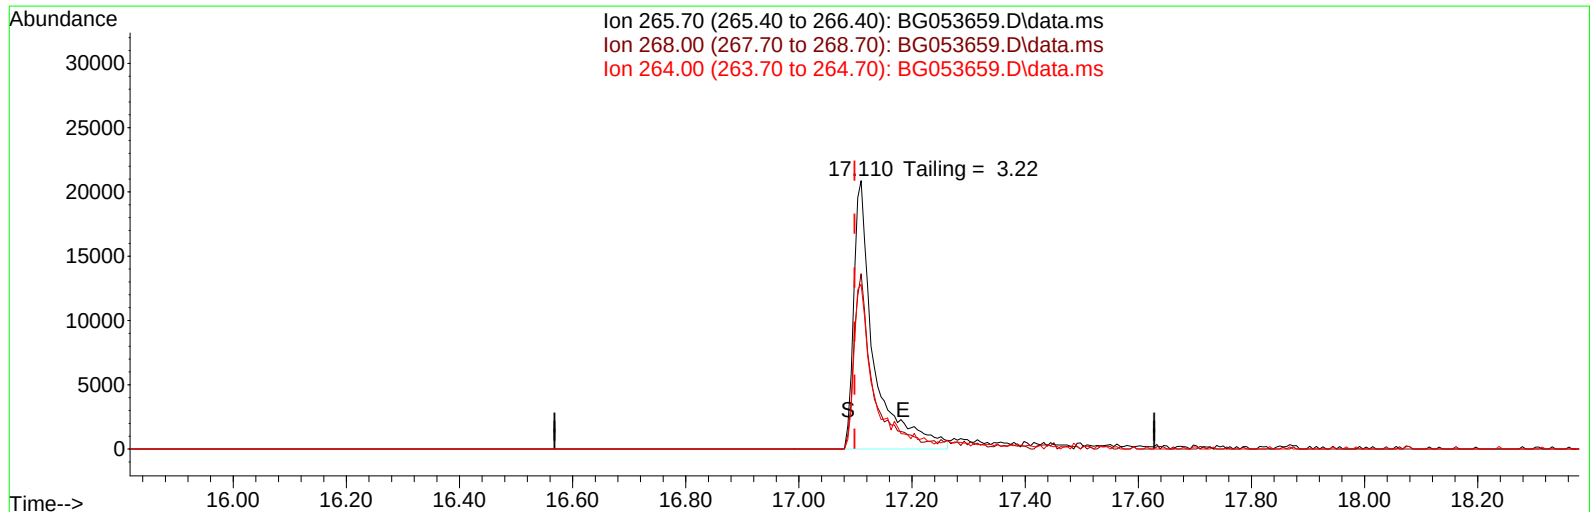

TIC: BG053659.D\data.ms

(70) Pentachlorophenol (C)




17.110min (+ 0.012) 23822.46 ng

response 51907

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.29
264.00	66.20	61.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052322\
 Data File : BG053659.D
 Acq On : 23 May 2022 9:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 06:25:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 24 05:05:32 2022
 Response via : Initial Calibration

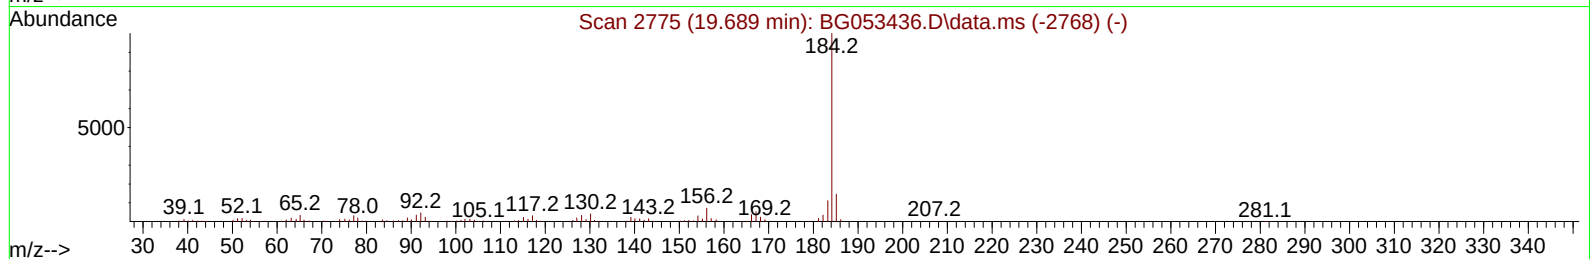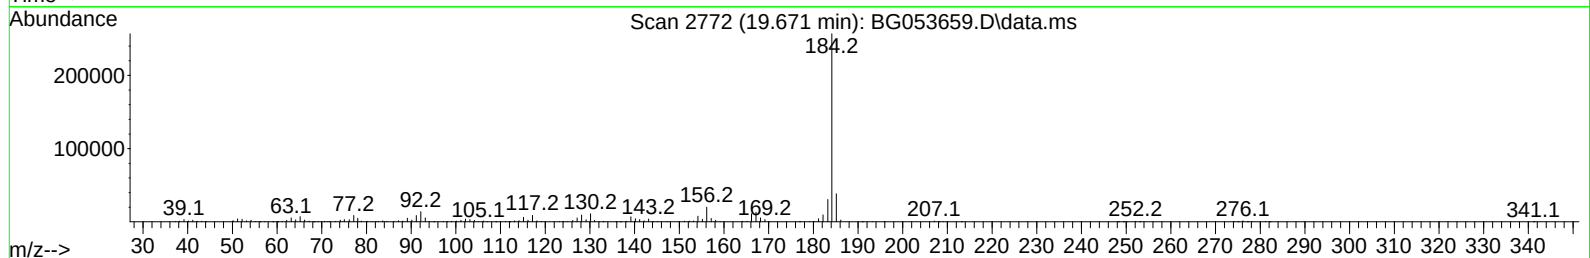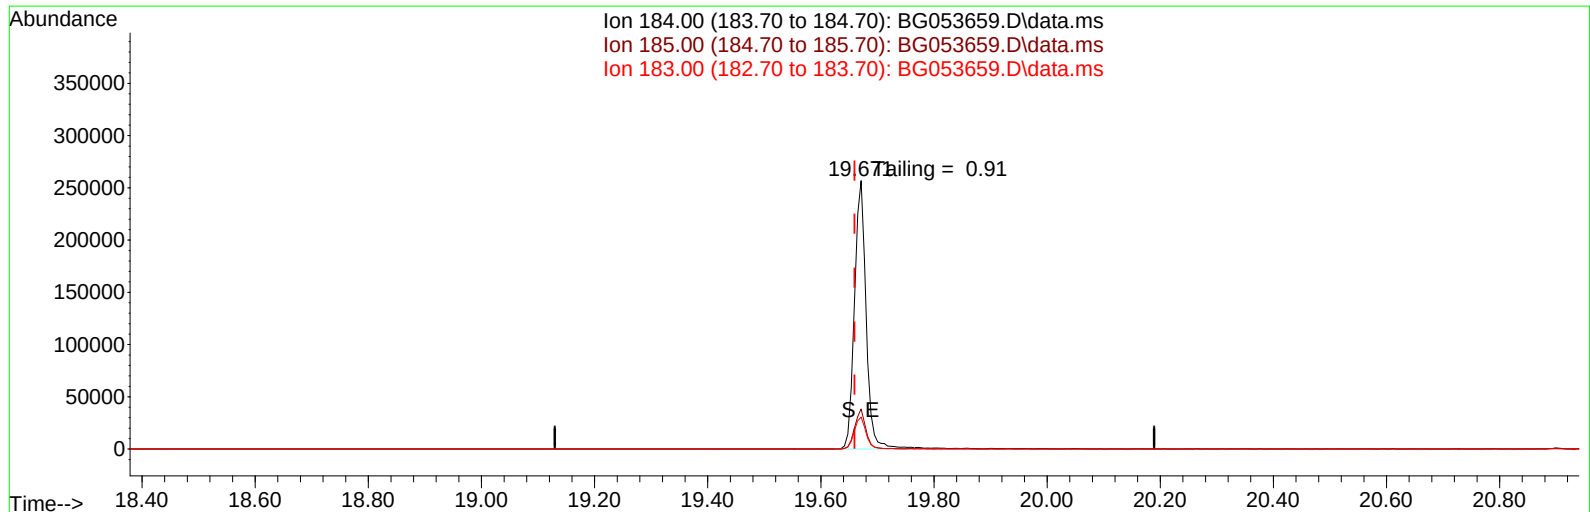

TIC: BG053659.D\data.ms

(77) Benzidine**19.671min (+ 0.012) 272312.89 ng****response 369769**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.93
183.00	11.10	11.87
0.00	0.00	0.00