

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052322\
 Data File : BG053671.D
 Acq On : 23 May 2022 19:29
 Operator : CG/JU
 Sample : N2968-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-39

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.746	55	61	69	rVB	98199	161435	1.20%	0.208%
2	4.222	135	142	158	rBV	1522089	2613021	19.47%	3.359%
3	4.534	189	195	208	rVB2	71160	147082	1.10%	0.189%
4	5.562	362	370	378	rBV	3005750	5209441	38.82%	6.697%
5	5.638	378	383	386	rVV	246968	388027	2.89%	0.499%
6	5.703	386	394	410	rVB	4995064	13417900	100.00%	17.249%
7	6.067	445	456	466	rBV	3455350	5986760	44.62%	7.696%
8	6.543	530	537	546	rBV	188162	318716	2.38%	0.410%
9	7.036	613	621	631	rBV	473773	801610	5.97%	1.031%
10	7.148	631	640	645	rVV	1627329	2776797	20.69%	3.570%
11	7.206	645	650	657	rVV	1000292	1881308	14.02%	2.418%
12	7.277	657	662	674	rVB	944275	1636480	12.20%	2.104%
13	7.447	679	691	701	rBV	1181716	1961664	14.62%	2.522%
14	7.712	723	736	744	rBV	3600829	6388341	47.61%	8.212%
15	8.058	788	795	799	rBV	104004	197301	1.47%	0.254%
16	8.176	807	815	823	rVB	1366416	2407392	17.94%	3.095%
17	8.434	853	859	868	rVB	1021210	1821308	13.57%	2.341%
18	8.552	873	879	883	rVV	119956	201719	1.50%	0.259%
19	8.605	883	888	896	rVB2	256818	445855	3.32%	0.573%
20	8.699	896	904	910	rBV2	333256	586186	4.37%	0.754%
21	8.863	922	932	942	rBV3	128270	321216	2.39%	0.413%
22	9.016	950	958	962	rBV	205640	349331	2.60%	0.449%
23	9.069	962	967	972	rBV	174426	326682	2.43%	0.420%
24	9.168	978	984	989	rBV	427320	810264	6.04%	1.042%
25	9.227	989	994	1009	rVB2	502763	1332764	9.93%	1.713%
26	9.503	1034	1041	1047	rBV2	125507	230782	1.72%	0.297%
27	9.691	1067	1073	1078	rBV	215525	351429	2.62%	0.452%
28	9.750	1078	1083	1090	rVB	305734	506270	3.77%	0.651%
29	9.838	1090	1098	1107	rBV4	82036	206603	1.54%	0.266%
30	10.050	1128	1134	1140	rBV4	165494	366695	2.73%	0.471%
31	10.114	1140	1145	1156	rVB	235570	450918	3.36%	0.580%
32	10.267	1164	1171	1178	rBV2	600278	1190244	8.87%	1.530%
33	10.502	1205	1211	1217	rVV2	223913	395947	2.95%	0.509%
34	10.749	1241	1253	1258	rBV	468473	876122	6.53%	1.126%
35	10.866	1263	1273	1277	rVV2	145517	410294	3.06%	0.527%
36	10.925	1277	1283	1290	rVV	1672732	3224628	24.03%	4.145%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052322\
 Data File : BG053671.D
 Acq On : 23 May 2022 19:29
 Operator : CG/JU
 Sample : N2968-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-39

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.971	1455	1461	1470	rVV3	78912	172335	1.28%	0.222%
38	12.247	1502	1508	1516	rVB	207131	369151	2.75%	0.475%
39	12.523	1544	1555	1561	rVV	1116208	1964417	14.64%	2.525%
40	12.576	1561	1564	1570	rVB2	85149	140382	1.05%	0.180%
41	12.740	1582	1592	1600	rBV2	1050752	1945909	14.50%	2.502%
42	12.899	1614	1619	1631	rVB10	60234	181266	1.35%	0.233%
43	13.151	1657	1662	1670	rVB2	112147	188449	1.40%	0.242%
44	13.310	1679	1689	1696	rVB	1125718	1766408	13.16%	2.271%
45	13.521	1713	1725	1731	rBV2	132643	370218	2.76%	0.476%
46	13.651	1739	1747	1753	rBV2	88695	179689	1.34%	0.231%
47	13.727	1754	1760	1771	rVB3	126731	314883	2.35%	0.405%
48	13.821	1771	1776	1777	rBV	110372	146827	1.09%	0.189%
49	13.862	1777	1783	1790	rVB3	347009	796845	5.94%	1.024%
50	14.009	1802	1808	1813	rBV	397218	755342	5.63%	0.971%
51	14.062	1813	1817	1827	rVB	298292	548493	4.09%	0.705%
52	14.244	1843	1848	1852	rBV	154081	244219	1.82%	0.314%
53	14.414	1872	1877	1882	rVB	90958	137769	1.03%	0.177%
54	14.532	1893	1897	1908	rVB	80701	155895	1.16%	0.200%
55	14.690	1919	1924	1930	rVB	245918	403434	3.01%	0.519%
56	14.896	1949	1959	1968	rVB8	66350	234391	1.75%	0.301%
57	15.084	1986	1991	1997	rVB2	99526	156387	1.17%	0.201%
58	15.307	2022	2029	2033	rBV3	81914	161656	1.20%	0.208%
59	15.730	2095	2101	2106	rBV2	76693	141091	1.05%	0.181%
60	16.177	2171	2177	2185	rVB	931392	1458821	10.87%	1.875%
61	17.434	2385	2391	2395	rBV	311401	474744	3.54%	0.610%
62	20.042	2829	2835	2840	rVB	1930452	2613821	19.48%	3.360%
63	21.710	3113	3119	3127	rVB2	310138	533747	3.98%	0.686%
64	24.977	3665	3675	3685	rVB2	186158	533291	3.97%	0.686%




Sum of corrected areas: 77788412

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052322\
Data File : BG053671.D
Acq On : 23 May 2022 19:29
Operator : CG/JU
Sample : N2968-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-39

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

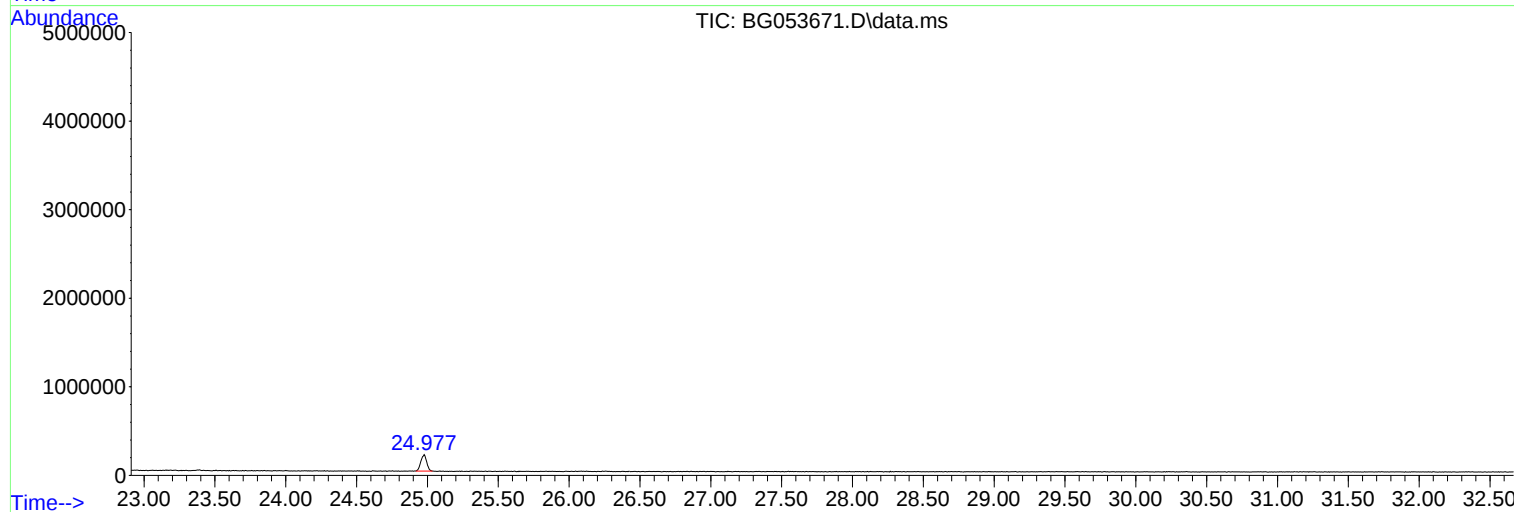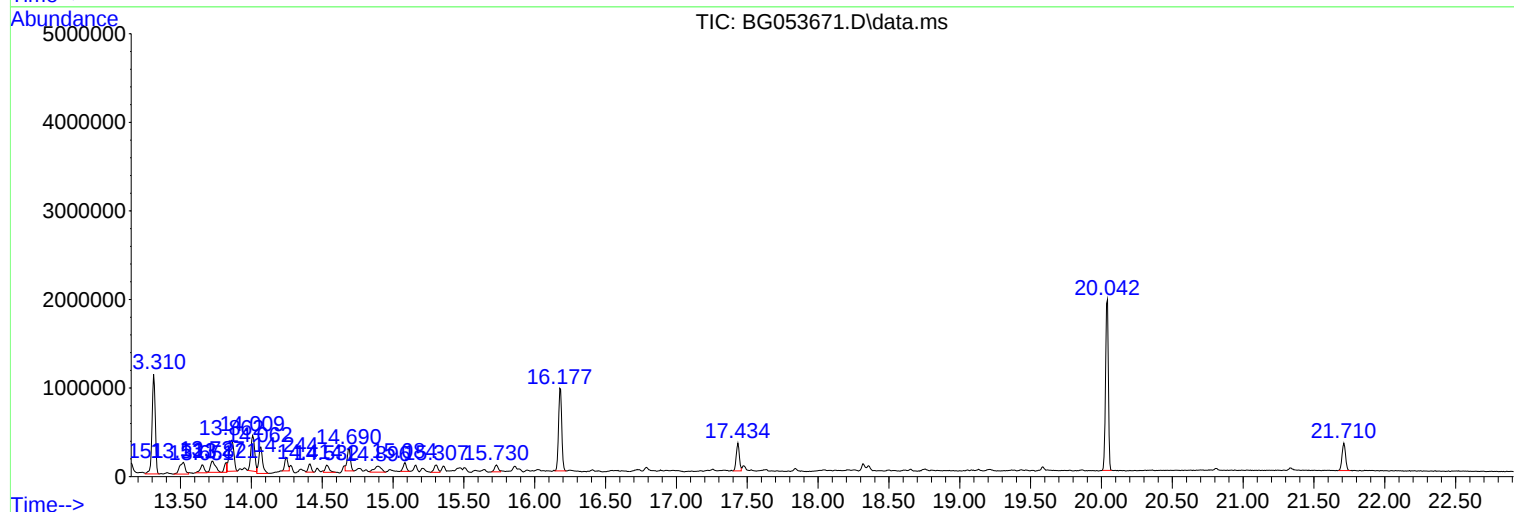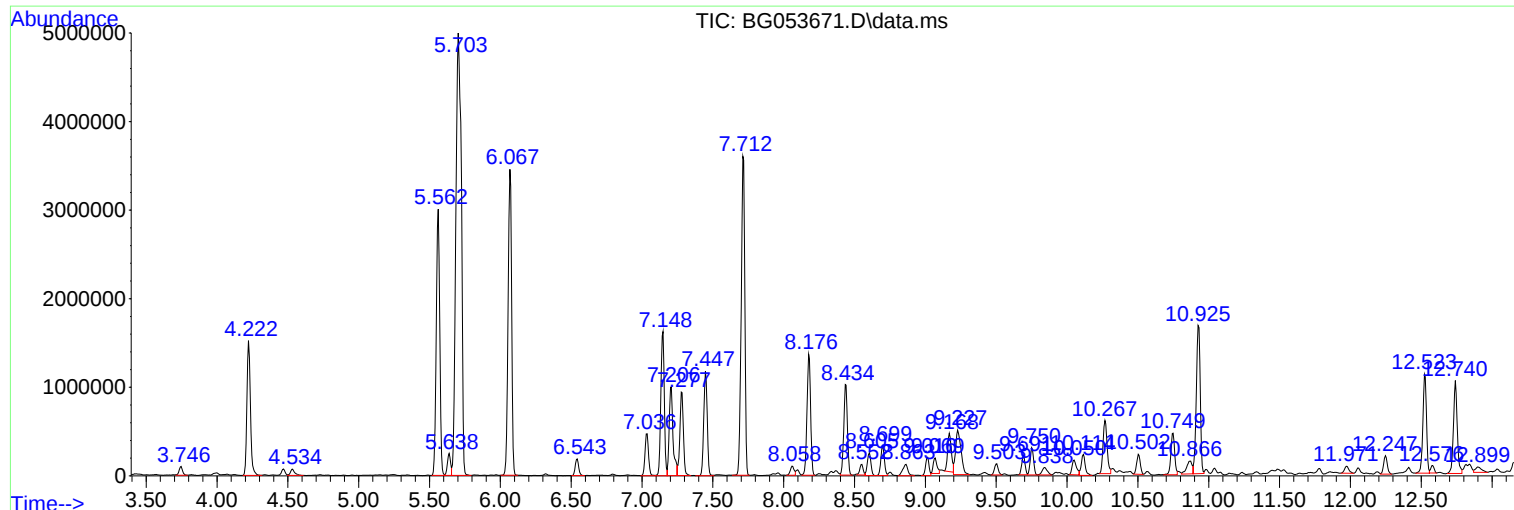

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052322\
Data File : BG053671.D
Acq On : 23 May 2022 19:29
Operator : CG/JU
Sample : N2968-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-39

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052322\
Data File : BG053671.D
Acq On : 23 May 2022 19:29
Operator : CG/JU
Sample : N2968-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-39

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------