


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052322\
 Data File : BG053659.D
 Acq On : 23 May 2022 9:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 24 05:05:32 2022

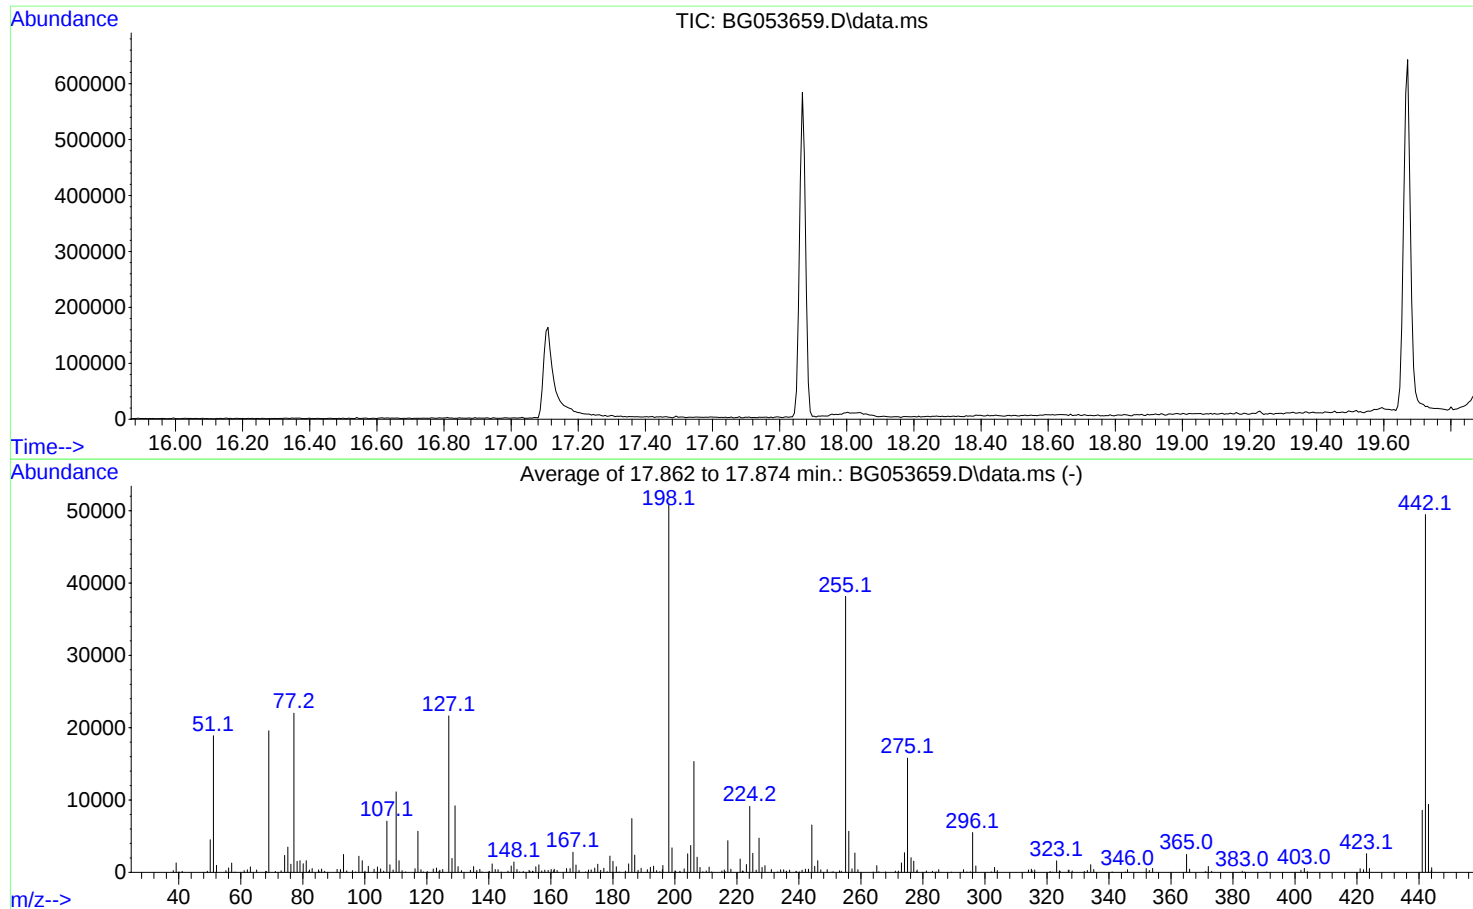




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	18895	PASS
68	69	0.00	2	0.8	152	PASS
69	198	0.00	100	38.5	19571	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	21640	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50856	PASS
199	198	5	9	6.7	3392	PASS
275	198	10	60	31.1	15791	PASS
365	198	1	100	4.9	2485	PASS
441	198	0.01	100	16.9	8575	PASS
442	442	50	100	100.0	49472	PASS
443	442	15	24	19.0	9405	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052322\
 Data File : BG053659.D
 Acq On : 23 May 2022 9:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: May 24 06:25:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 24 05:05:32 2022
 Response via : Initial Calibration

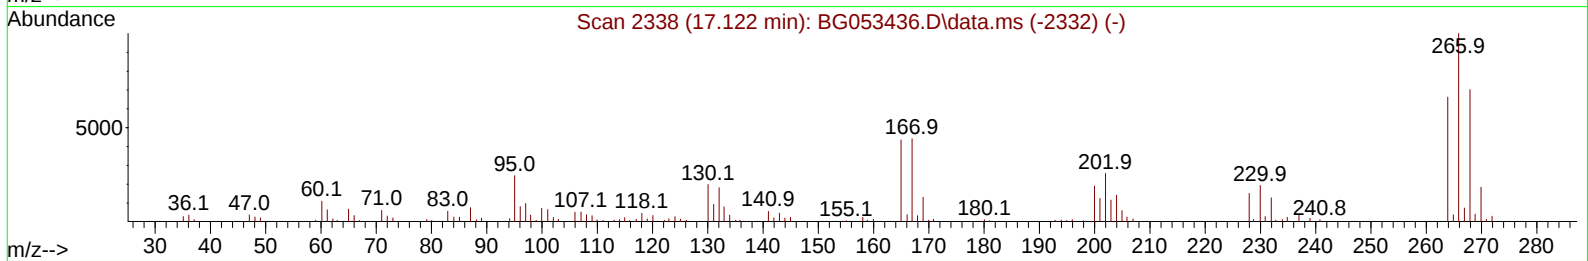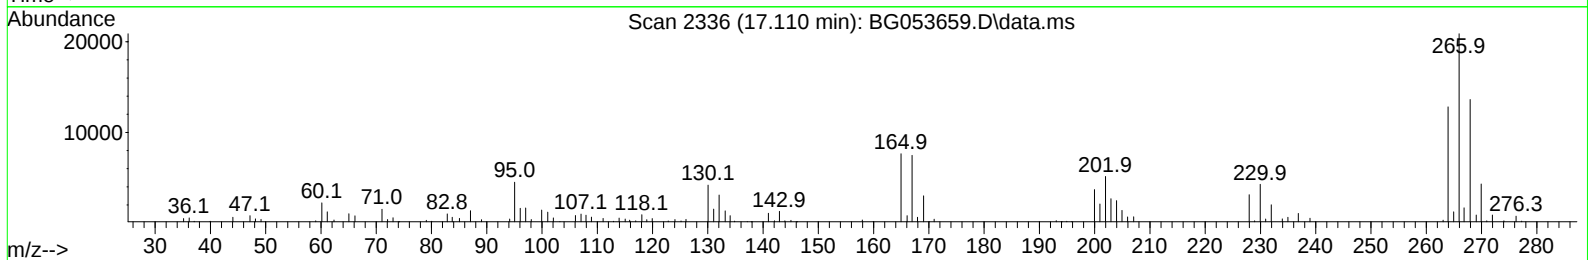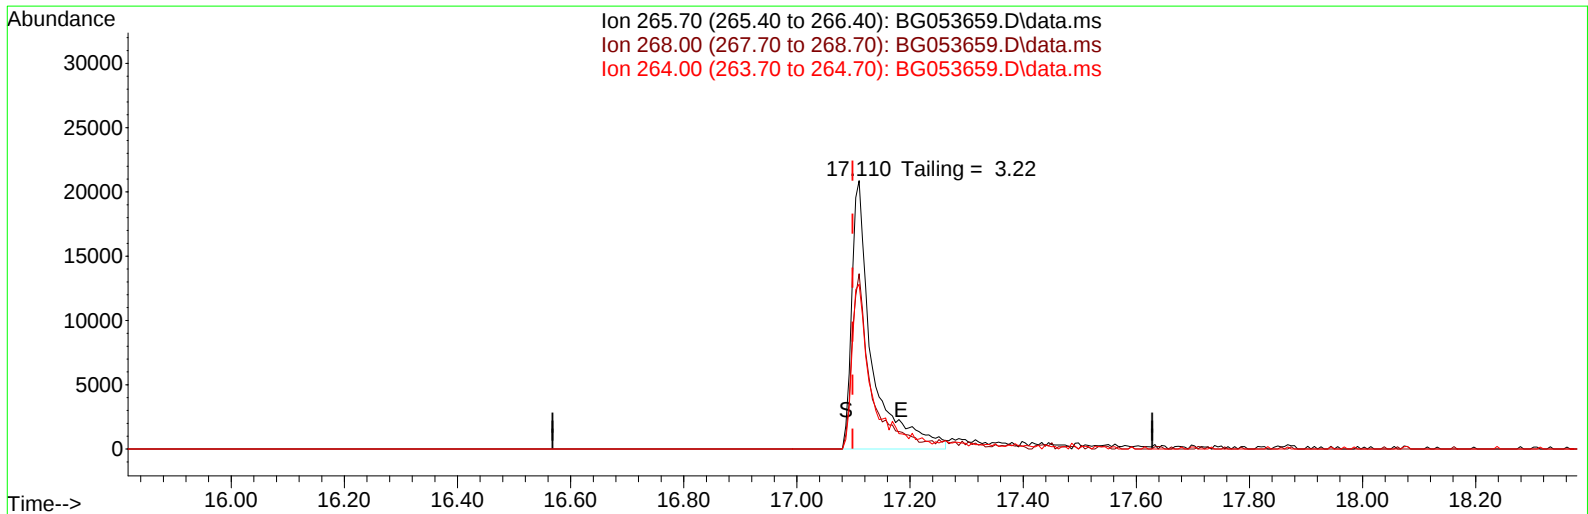

TIC: BG053659.D\data.ms

(70) Pentachlorophenol (C)

17.110min (+ 0.012) 23822.46 ng




response 51907

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.29
264.00	66.20	61.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052322\
Data File : BG053659.D
Acq On : 23 May 2022 9:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 24 06:25:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 24 05:05:32 2022
Response via : Initial Calibration

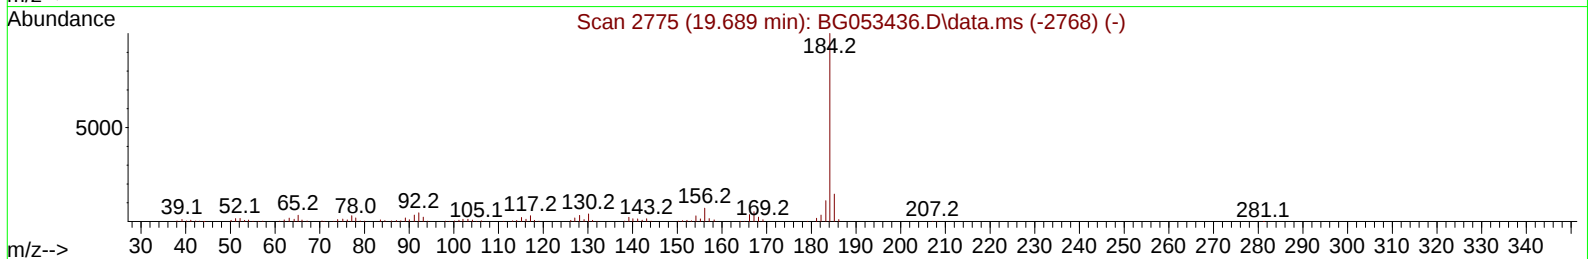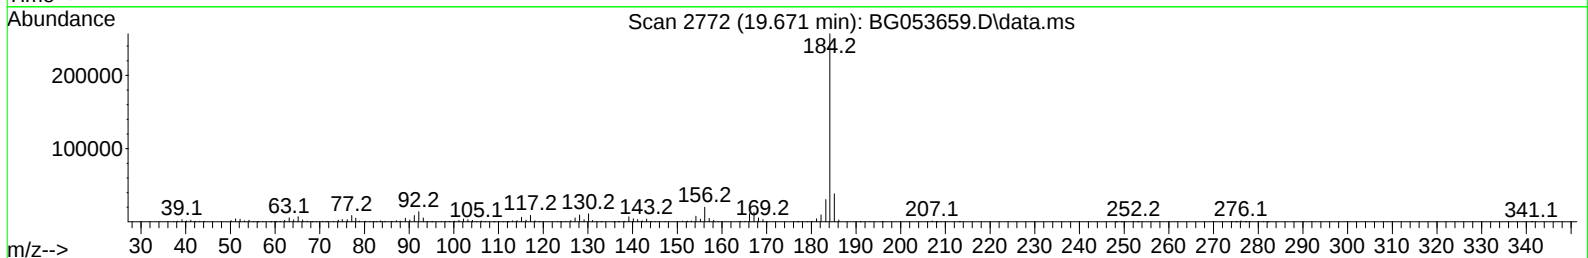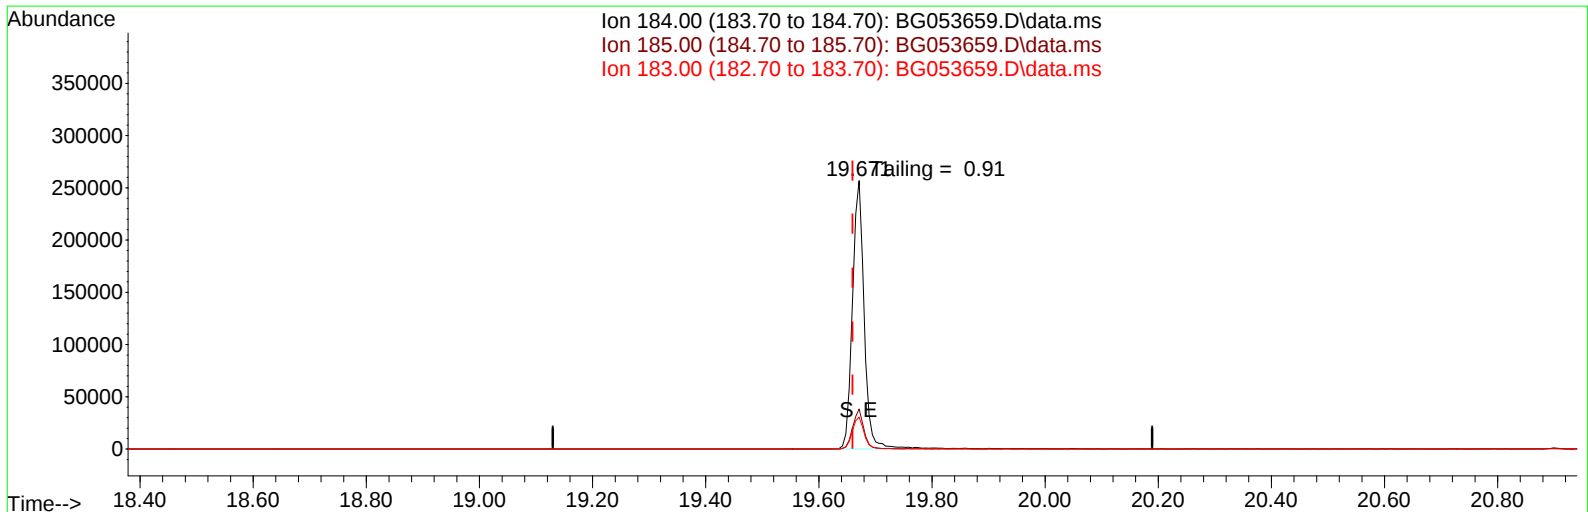

TIC: BG053659.D\data.ms

(77) Benzidine

19.671min (+ 0.012) 272312.89 ng

response 369769

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.93
183.00	11.10	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/23/2022	BNA_G	<u>BG053659.D</u>
Compound Name	Response	Retention Time
DDT	163885	20.899
DDD	3746	20.464
DDE	62	20.024
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3808	167693	2.27

Instrument :
BNA_G
ClientSampleId :
DFTPP