
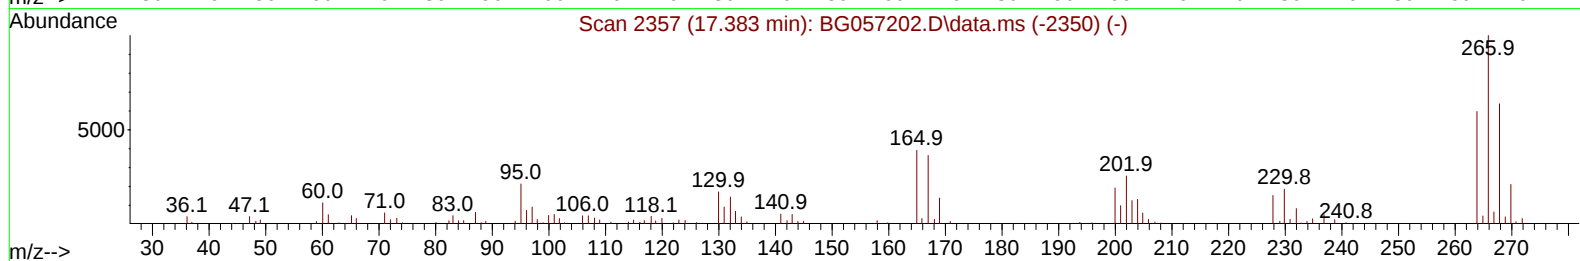
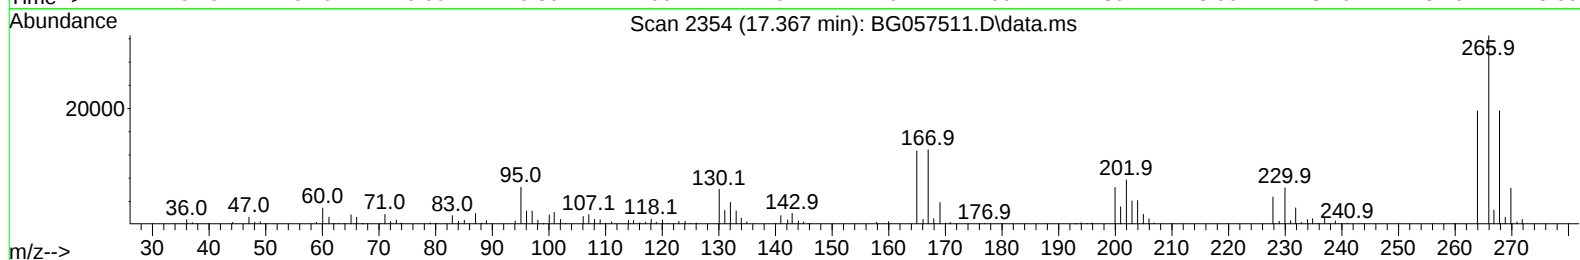


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052323\
Data File : BG057511.D
Acq On : 23 May 2023 9:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 11:23:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

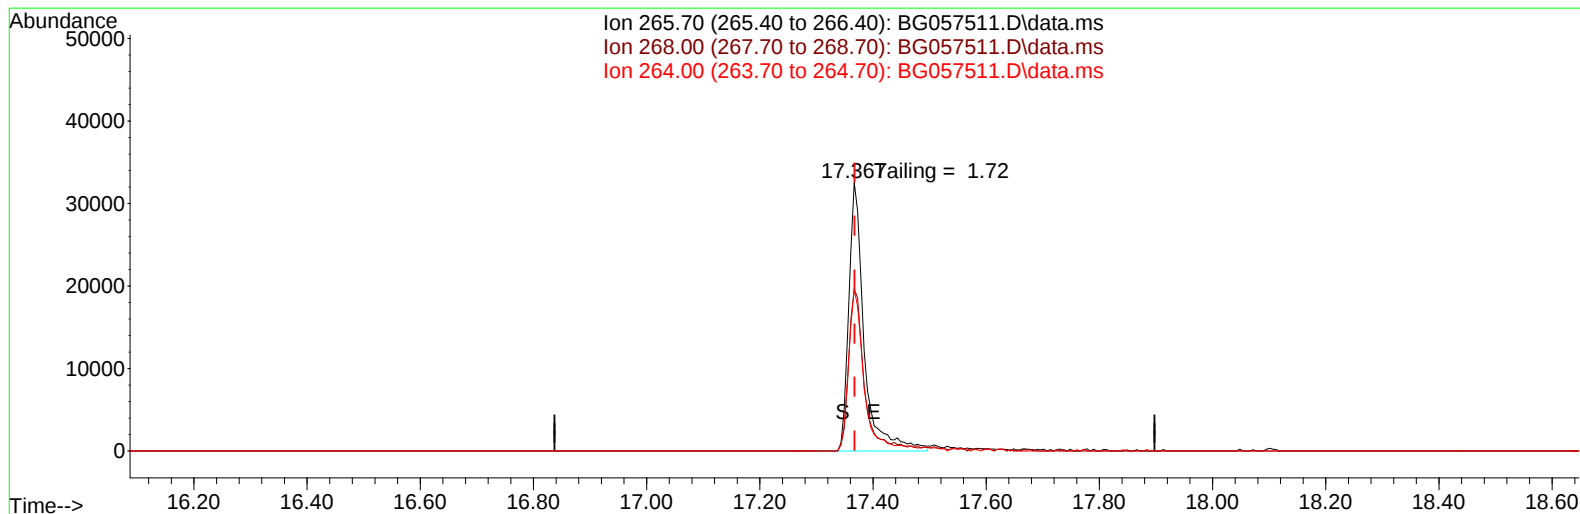

TIC: BG057511.D\data.ms

(70) Pentachlorophenol (C)




17.367min (-0.000) 62692.89 ng

response 61721

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	60.31
264.00	59.70	60.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052323\
Data File : BG057511.D
Acq On : 23 May 2023 9:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 11:23:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

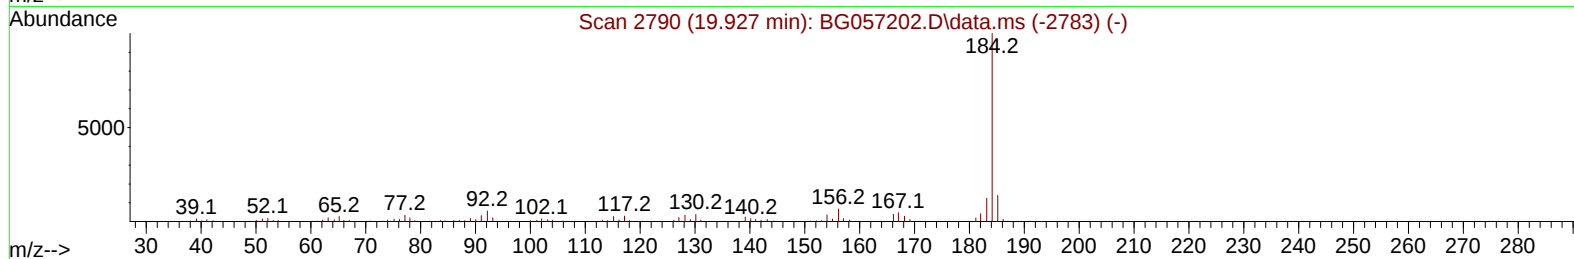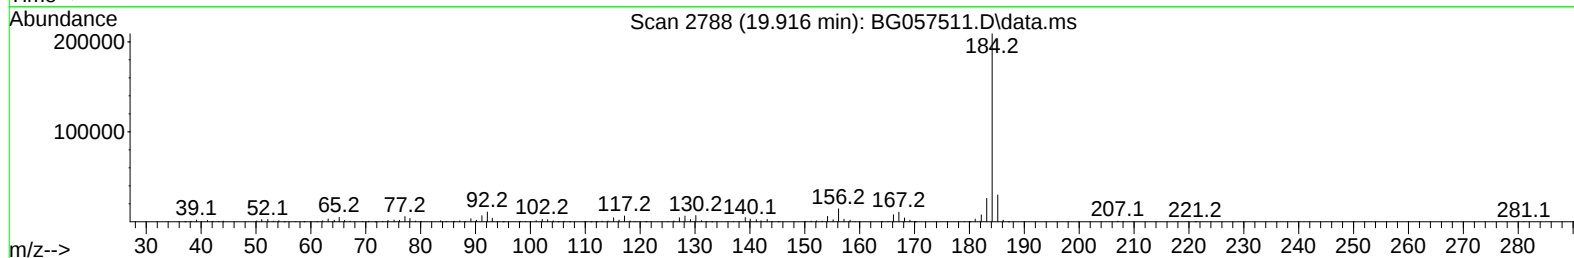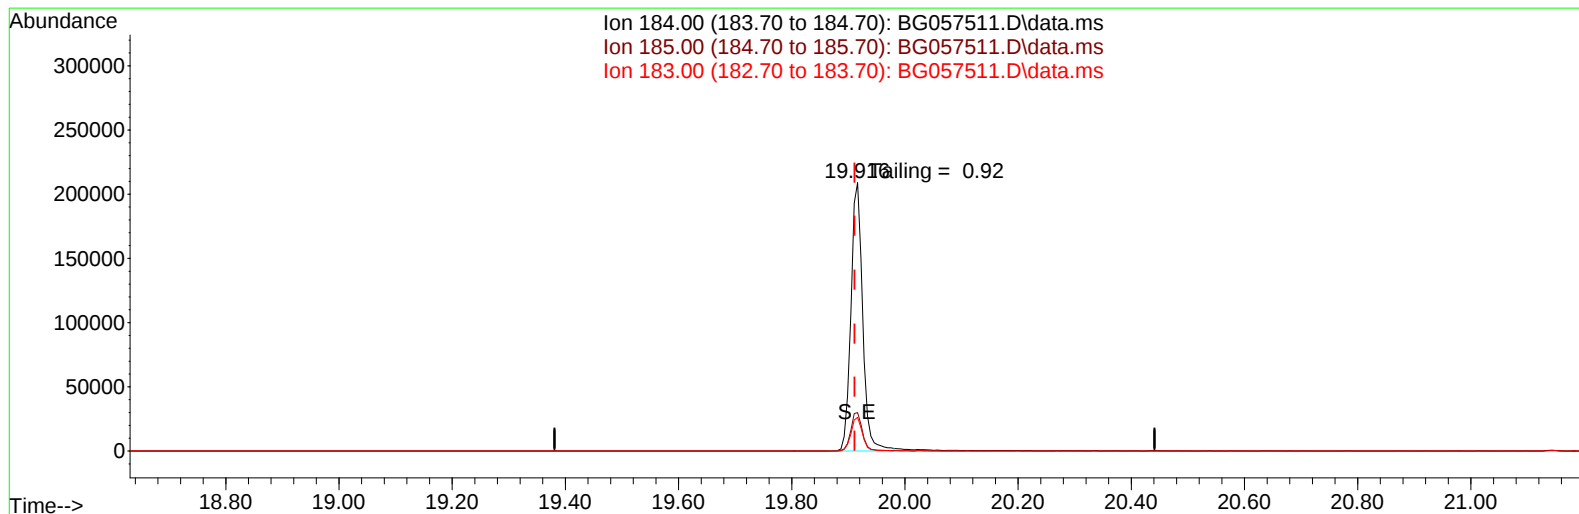

TIC: BG057511.D\data.ms

(77) Benzidine**19.916min (+ 0.005) 0.00 ng****response 302549**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.30
183.00	12.40	12.52
0.00	0.00	0.00