

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052323\
 Data File : BG057527.D
 Acq On : 23 May 2023 20:03
 Operator : CG/JU
 Sample : 02886-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-1

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 05/24/2023
 Supervised By : mohammad ahmed 05/24/2023

Quant Time: May 24 04:35:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 20 04:19:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.355	152	27745	20.000	ng	0.00
21) Naphthalene-d8	11.192	136	103327	20.000	ng	0.00
39) Acenaphthene-d10	14.969	164	69563	20.000	ng	0.00
64) Phenanthrene-d10	17.712	188	150014	20.000	ng	0.00
76) Chrysene-d12	22.018	240	126987	20.000	ng	0.00
86) Perylene-d12	25.531	264	141234	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.876	112	123684	76.257	ng	0.00
7) Phenol-d6	7.503	99	177883	72.223	ng	0.00
23) Nitrobenzene-d5	9.535	82	116280	47.232	ng	0.00
42) 2,4,6-Tribromophenol	16.455	330	74229	75.205	ng	0.00
45) 2-Fluorobiphenyl	13.595	172	257881	49.928	ng	0.00
79) Terphenyl-d14	20.280	244	344917	44.326	ng	0.00
Target Compounds						Qvalue
71) Phenanthrene	17.754	178	180181	23.440	ng	100
72) Anthracene	17.848	178	32272	4.092	ng	97
73) Carbazole	18.112	167	18023	2.714	ng	96
75) Fluoranthene	19.745	202	343246	35.902	ng	99
78) Pyrene	20.109	202	300243	32.537	ng	98
81) Benzo(a)anthracene	22.001	228	168428	18.616	ng	99
83) Chrysene	22.071	228	160342	18.836	ng	98
87) Indeno(1,2,3-cd)pyrene	29.579	276	73752m	7.165	ng	
88) Benzo(b)fluoranthene	24.403	252	199096	21.565	ng	# 97
89) Benzo(k)fluoranthene	24.468	252	74205m	7.910	ng	
90) Benzo(a)pyrene	25.361	252	139645	15.482	ng	95
91) Dibenzo(a,h)anthracene	29.596	278	20954m	2.444	ng	
92) Benzo(g,h,i)perylene	30.854	276	73774	8.814	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052323\
Data File : BG057527.D
Acq On : 23 May 2023 20:03
Operator : CG/JU
Sample : 02886-01
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
WC-1

Quant Time: May 24 04:35:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

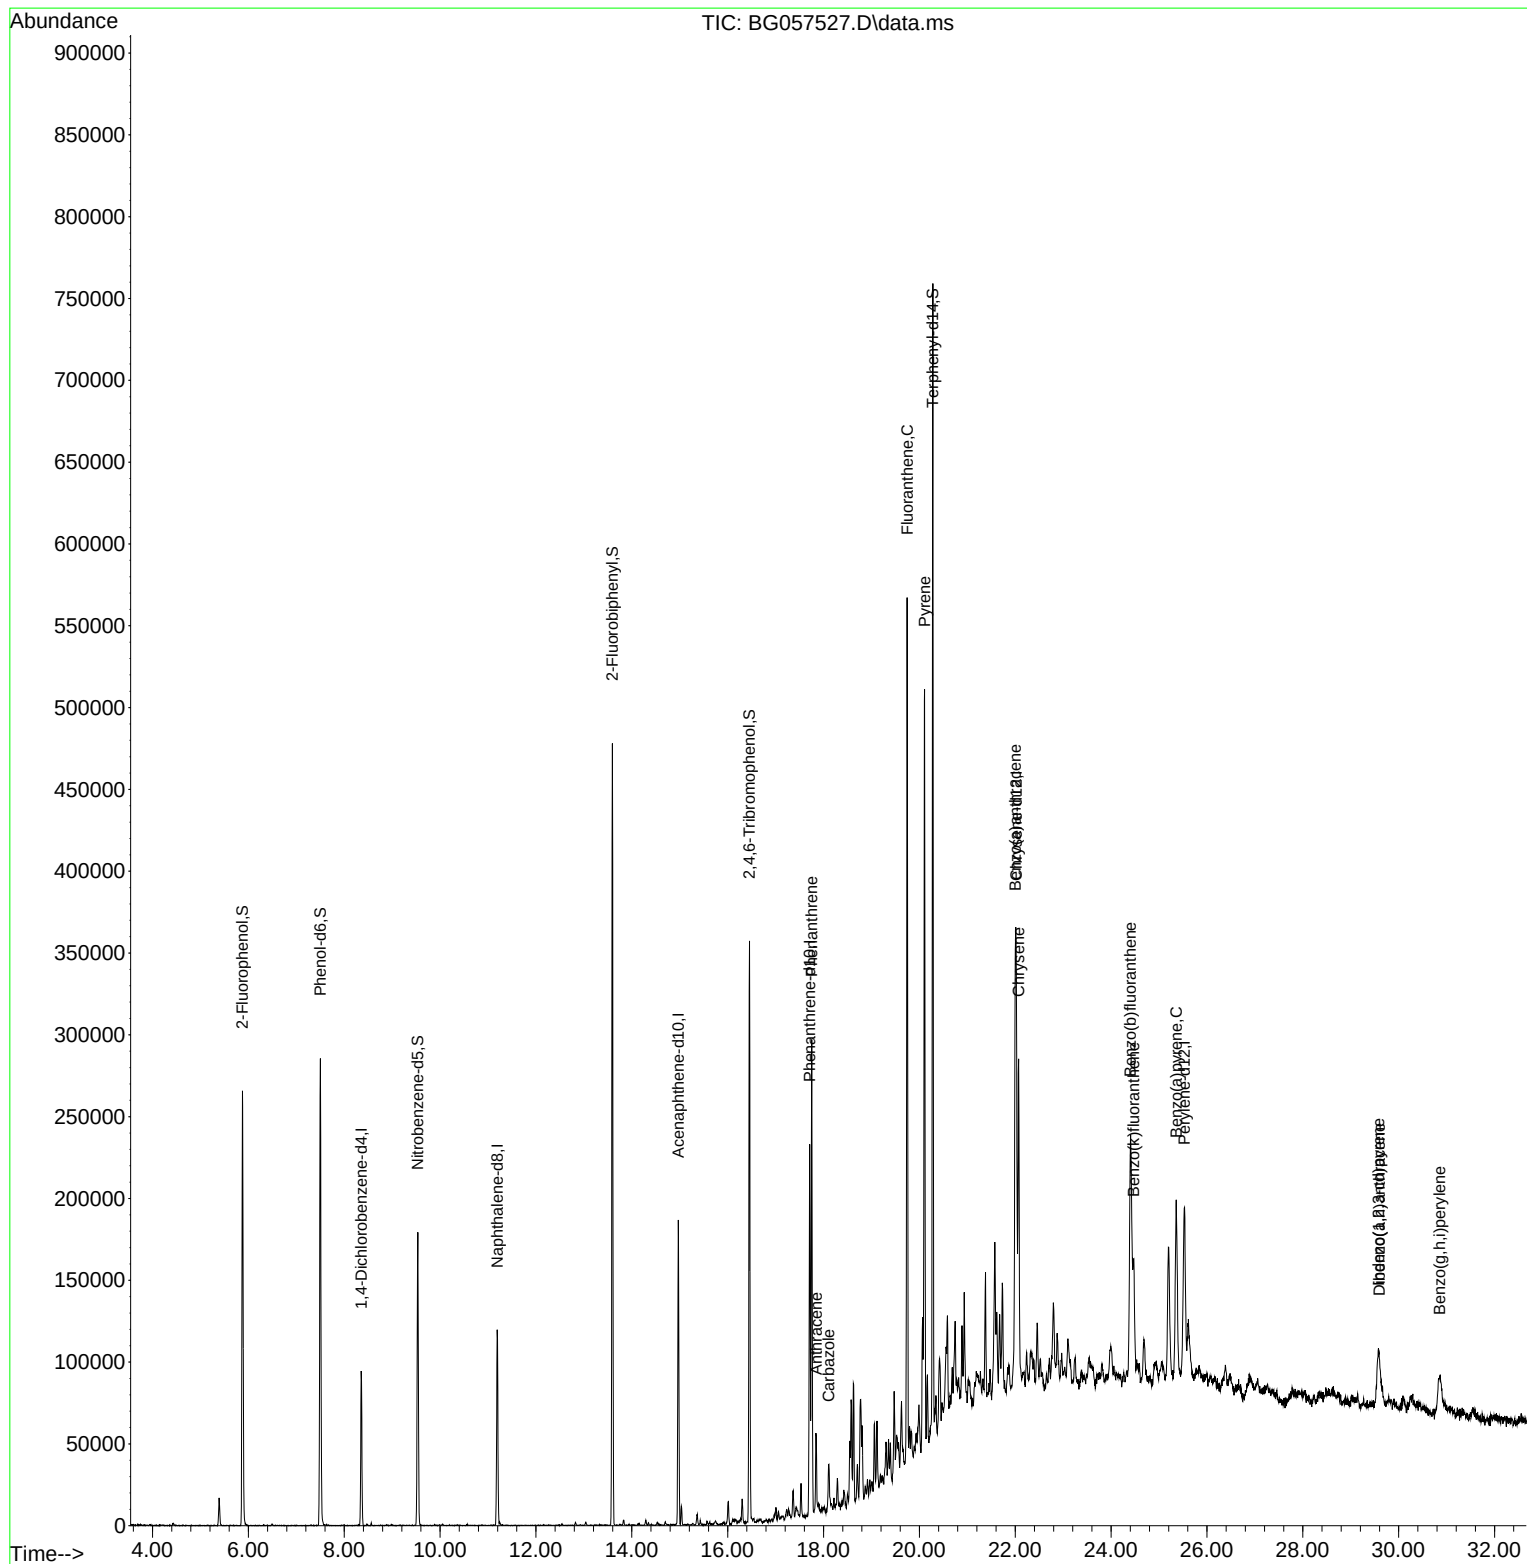



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.355 min Scan# 81
Delta R.T. -0.007 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03




Instrument :
BNA_G
ClientSampleId :
WC-1




Tgt Ion:152 Resp: 2774
Ion Ratio Lower Upper
152 100
150 154.2 126.2 189.4
115 59.3 45.0 67.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

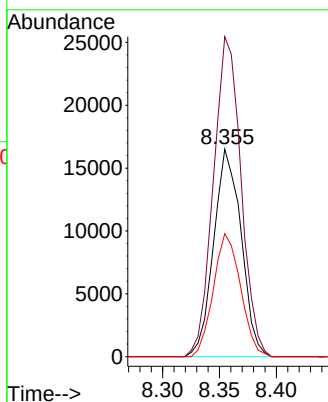


#5
2-Fluorophenol
Concen: 76.257 ng
RT: 5.876 min Scan# 398
Delta R.T. 0.005 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03




Tgt Ion:112 Resp: 123684
Ion Ratio Lower Upper
112 100
64 64.0 49.4 74.2
63 34.7 31.6 47.4

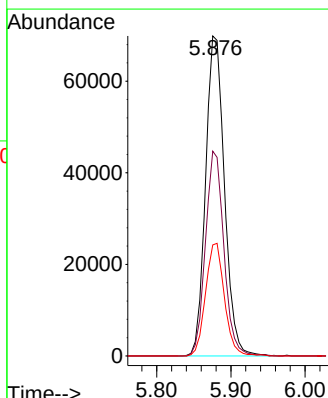



#7
Phenol-d6
Concen: 72.223 ng
RT: 7.503 min Scan# 61
Delta R.T. 0.005 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03




Instrument :
BNA_G
ClientSampleId :
WC-1




Tgt Ion: 99 Resp: 17788
Ion Ratio Lower Upper
99 100
42 17.5 15.1 22.7
71 38.9 35.2 52.8

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

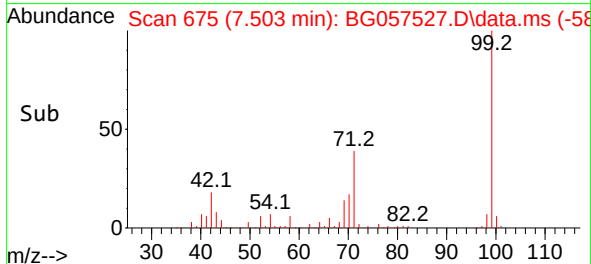


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.192 min Scan# 1303
Delta R.T. -0.007 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03



Tgt Ion:136 Resp: 103327
Ion Ratio Lower Upper
136 100
137 11.5 8.3 12.5
54 7.0 6.7 10.1
68 5.4 4.6 6.8

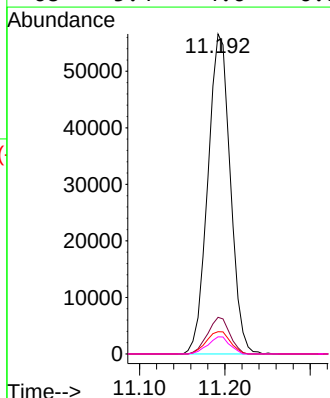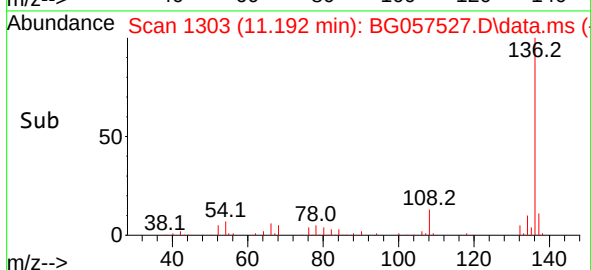

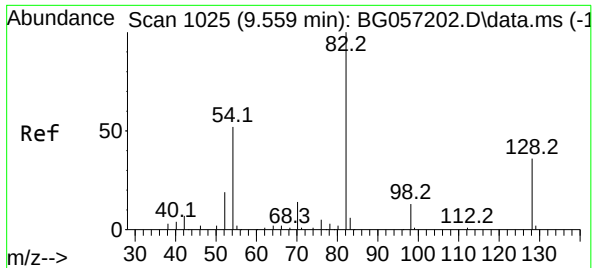

#23

Nitrobenzene-d5

Concen: 47.232 ng

RT: 9.535 min Scan# 1021

Delta R.T. -0.001 min

Lab File: BG057527.D

Acq: 23 May 2023 20:03

Instrument :

BNA_G

ClientSampleId :

WC-1

Tgt Ion: 82 Resp: 116280

Ion Ratio Lower Upper

82 100





128 39.3 29.0 43.4

54 46.8 41.4 62.0

Manual Integrations

APPROVED

Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

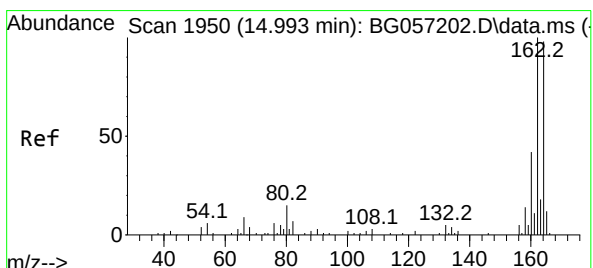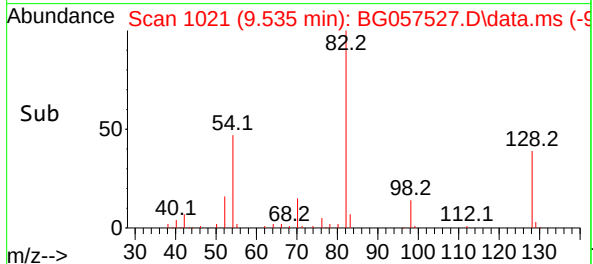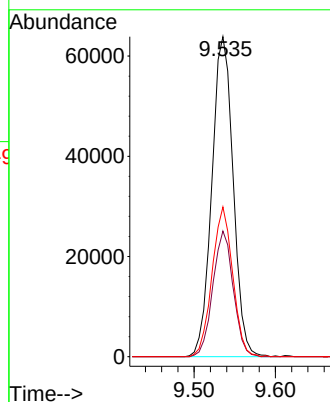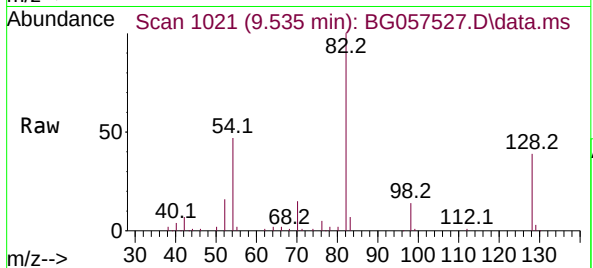

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.969 min Scan# 1946

Delta R.T. -0.007 min

Lab File: BG057527.D

Acq: 23 May 2023 20:03




Tgt Ion:164 Resp: 69563


Ion Ratio Lower Upper

164 100

162 96.3 81.8 122.6

160 44.9 34.6 52.0

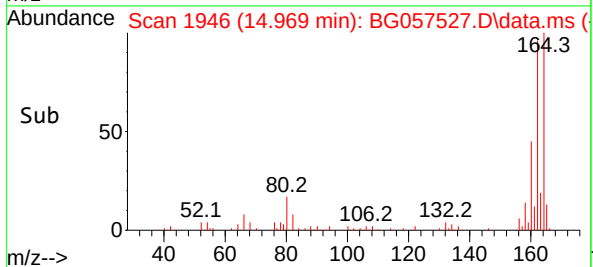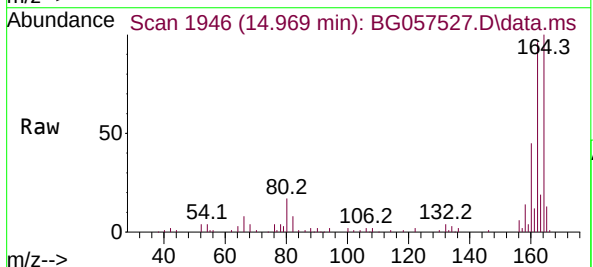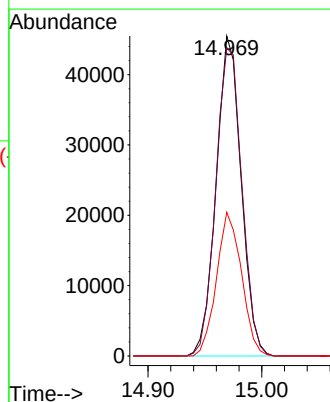







#42
2,4,6-Tribromophenol
Concen: 75.205 ng
RT: 16.455 min Scan# 2199
Delta R.T. -0.001 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03

Instrument :
BNA_G
ClientSampleId :
WC-1

Tgt Ion:330 Resp: 74229
Ion Ratio Lower Upper
330 100
332 96.4 78.2 117.2
141 30.6 27.8 41.8




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

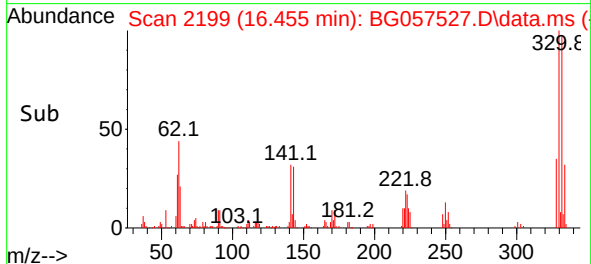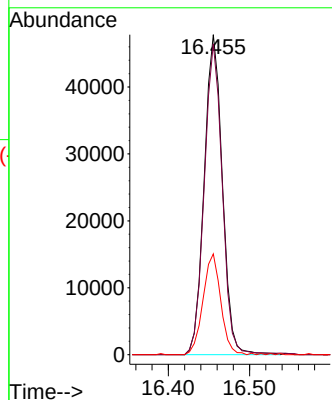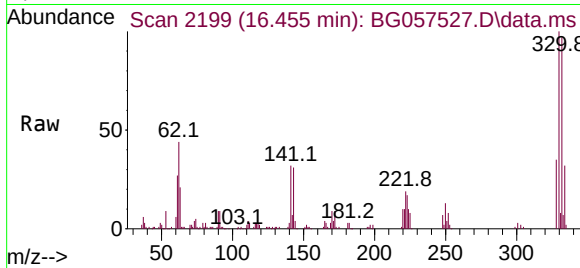

#45
2-Fluorobiphenyl
Concen: 49.928 ng
RT: 13.595 min Scan# 1712
Delta R.T. -0.007 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03


Tgt Ion:172 Resp: 257881
Ion Ratio Lower Upper
172 100
171 36.3 29.4 44.0
170 22.9 19.0 28.6

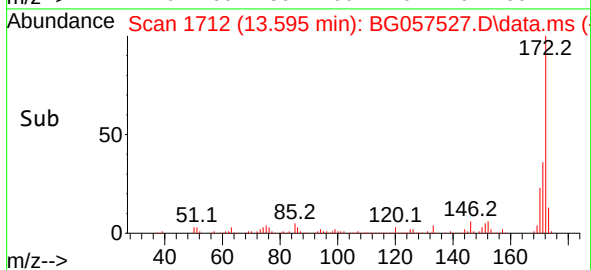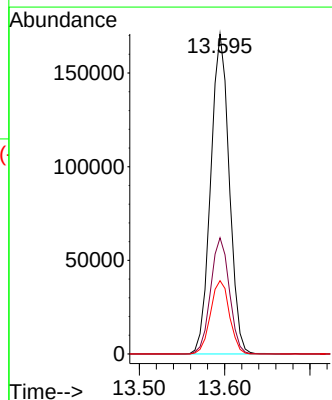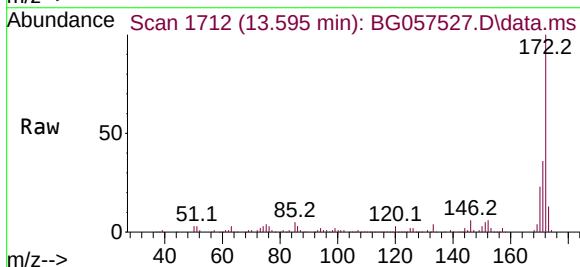



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.712 min Scan# 2416
Delta R.T. -0.001 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03




Instrument :
BNA_G
ClientSampleId :
WC-1




Tgt Ion:188 Resp: 150014
Ion Ratio Lower Upper
188 100
94 6.8 5.1 7.7
80 6.8 5.7 8.5

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

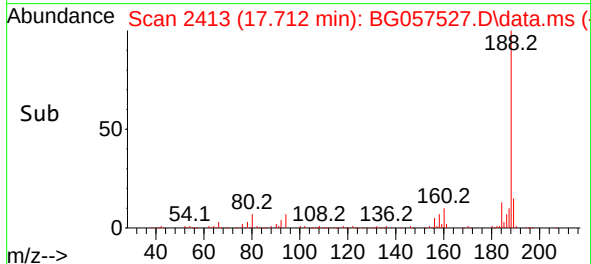


#71
Phenanthrene
Concen: 23.440 ng
RT: 17.754 min Scan# 2420
Delta R.T. -0.001 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03

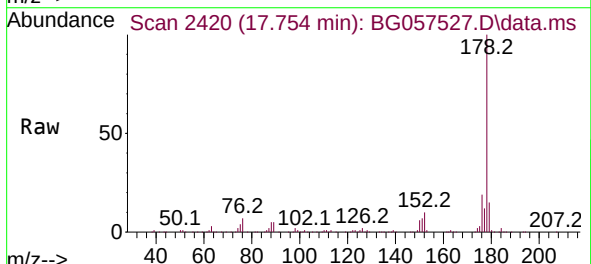


Tgt Ion:178 Resp: 180181
Ion Ratio Lower Upper
178 100
176 19.2 15.4 23.2
179 15.4 12.3 18.5

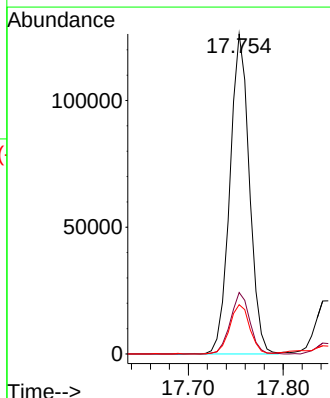



#72
 Anthracene
 Concen: 4.092 ng
 RT: 17.848 min Scan# 2436
 Delta R.T. -0.001 min
 Lab File: BG057527.D
 Acq: 23 May 2023 20:03




Instrument :
 BNA_G
 ClientSampleId :
 WC-1




Tgt Ion:178 Resp: 3227
 Ion Ratio Lower Upper
 178 100
 176 19.7 14.7 22.1
 179 14.8 13.2 19.8

Manual Integrations
 APPROVED



Reviewed By :Christian Giraldo 05/24/2023
 Supervised By :mohammad ahmed 05/24/2023

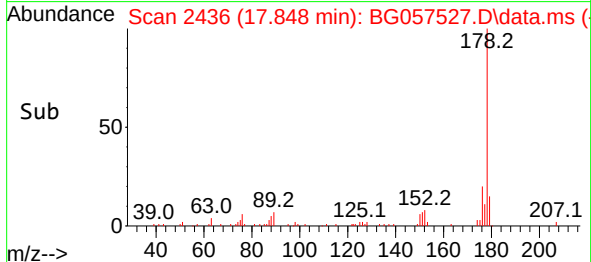


#73
 Carbazole
 Concen: 2.714 ng
 RT: 18.112 min Scan# 2481
 Delta R.T. -0.001 min
 Lab File: BG057527.D
 Acq: 23 May 2023 20:03

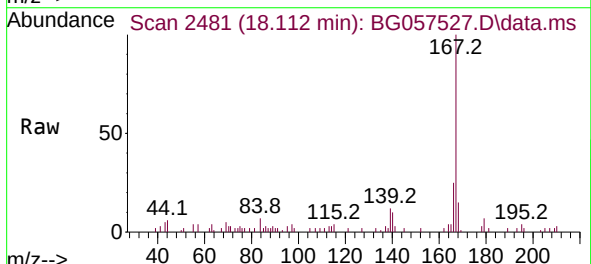


Tgt Ion:167 Resp: 18023
 Ion Ratio Lower Upper
 167 100
 166 24.7 17.4 26.0
 139 12.0 9.6 14.4

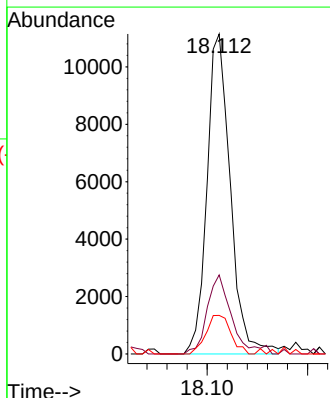



#75
Fluoranthene
Concen: 35.902 ng
RT: 19.745 min Scan# 21
Delta R.T. -0.001 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03




Instrument :
BNA_G
ClientSampleId :
WC-1



Tgt Ion:202 Resp: 343240
Ion Ratio Lower Upper
202 100
101 6.3 0.0 26.2
203 18.6 0.0 37.9




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

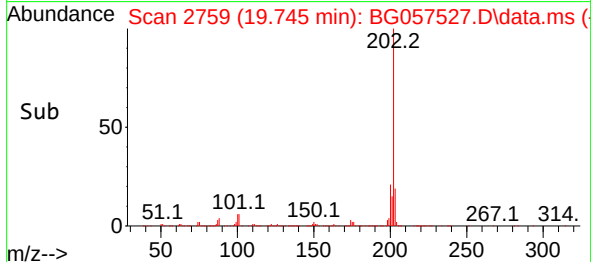

#76
Chrysene-d12
Concen: 20.000 ng
RT: 22.018 min Scan# 3146
Delta R.T. -0.001 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03


Tgt Ion:240 Resp: 126987
Ion Ratio Lower Upper
240 100
120 5.6 4.9 7.3
236 25.6 21.4 32.2

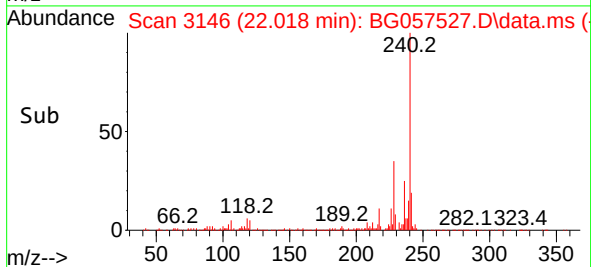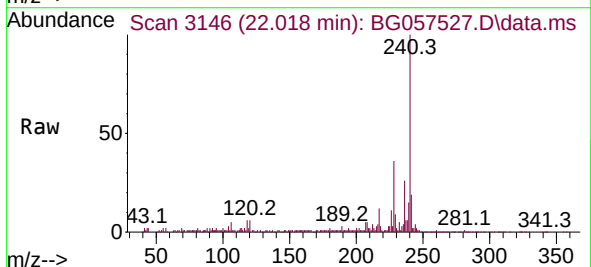



#78
 Pyrene
 Concen: 32.537 ng
 RT: 20.109 min Scan# 2821
 Delta R.T. 0.005 min
 Lab File: BG057527.D
 Acq: 23 May 2023 20:03




Instrument :
 BNA_G
 ClientSampleId :
 WC-1




Tgt Ion:202 Resp: 30024
 Ion Ratio Lower Upper
 202 100
 200 21.8 17.0 25.4
 203 19.5 14.2 21.4

Manual Integrations
 APPROVED



Reviewed By :Christian Giraldo 05/24/2023
 Supervised By :mohammad ahmed 05/24/2023

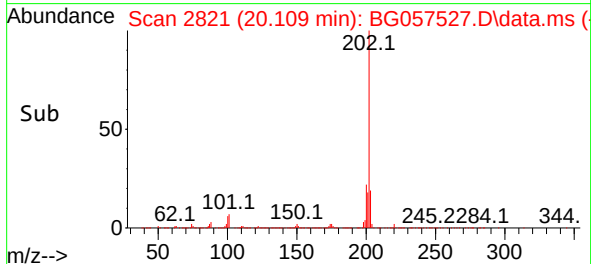


#79
 Terphenyl-d14
 Concen: 44.326 ng
 RT: 20.280 min Scan# 2850
 Delta R.T. -0.001 min
 Lab File: BG057527.D
 Acq: 23 May 2023 20:03

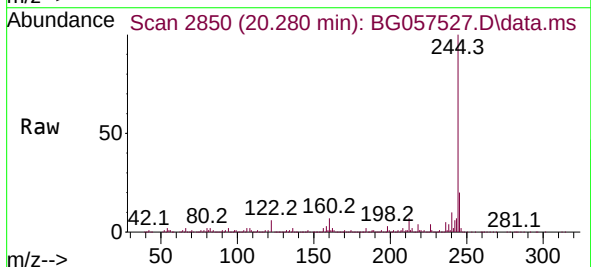


Tgt Ion:244 Resp: 344917
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.1 9.1
 122 5.5 5.1 7.7

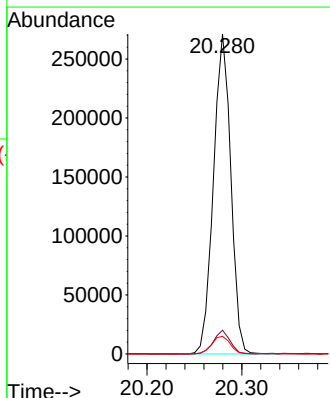



#81
Benzo(a)anthracene
Concen: 18.616 ng
RT: 22.001 min Scan# 3143
Delta R.T. 0.005 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03




Instrument :
BNA_G
ClientSampleId :
WC-1



Tgt Ion:228 Resp: 168428
Ion Ratio Lower Upper
228 100
226 27.2 22.0 33.0
229 20.0 15.8 23.8




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

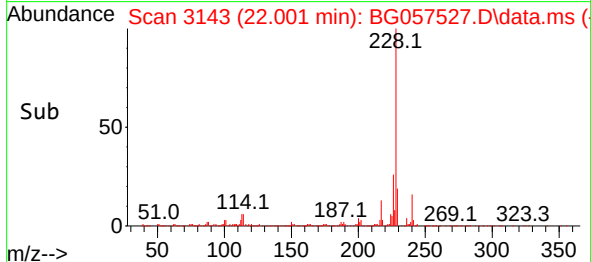

#83
Chrysene
Concen: 18.836 ng
RT: 22.071 min Scan# 3155
Delta R.T. -0.001 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03


Tgt Ion:228 Resp: 160342
Ion Ratio Lower Upper
228 100
226 30.0 24.3 36.5
229 22.0 15.9 23.9

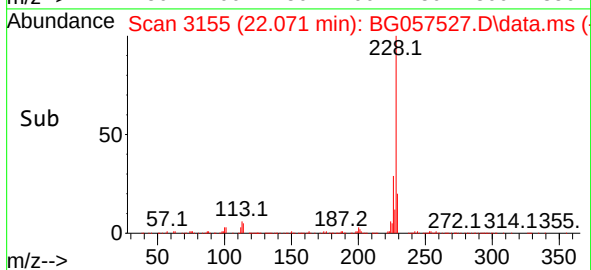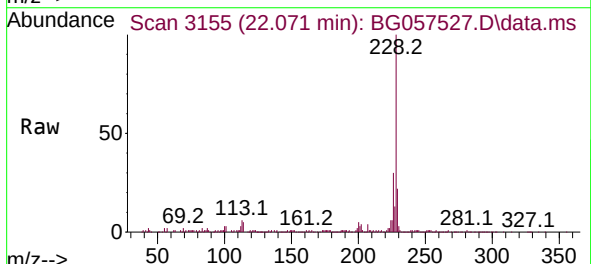



#86
Perylene-d12
Concen: 20.000 ng
RT: 25.531 min Scan# 31
Delta R.T. 0.016 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03




Instrument :
BNA_G
ClientSampleId :
WC-1



Tgt Ion:264 Resp: 141234
Ion Ratio Lower Upper
264 100
260 22.8 18.8 28.2
265 22.8 17.9 26.9




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

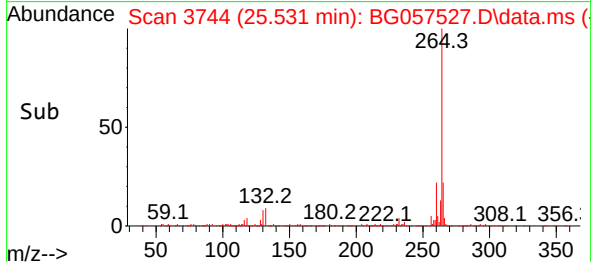

#87
Indeno(1,2,3-cd)pyrene
Concen: 7.165 ng m
RT: 29.579 min Scan# 4433
Delta R.T. 0.016 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03


Tgt Ion:276 Resp: 73752
Ion Ratio Lower Upper
276 100
138 0.7 5.4 8.0#
277 2.9 20.6 30.8#

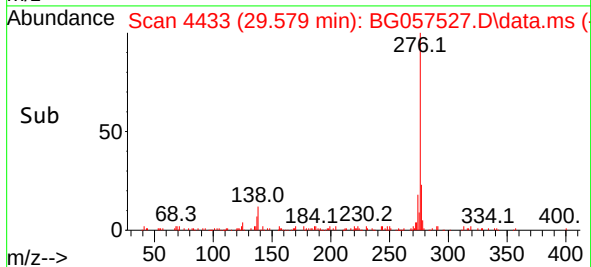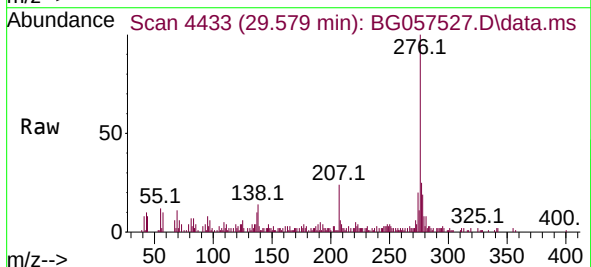



#88
Benzo(b)fluoranthene
Concen: 21.565 ng
RT: 24.403 min Scan# 3552
Delta R.T. 0.011 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03




Instrument :
BNA_G
ClientSampleId :
WC-1




Tgt Ion:252 Resp: 199090
Ion Ratio Lower Upper
252 100
253 22.7 17.0 25.6
125 6.5 4.2 6.2

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

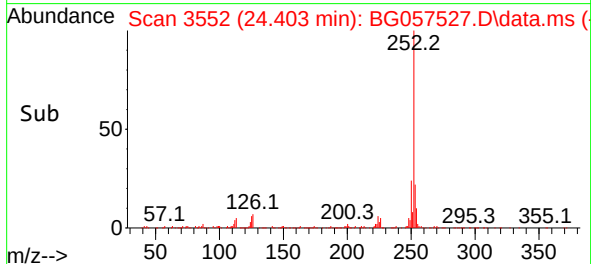


#89
Benzo(k)fluoranthene
Concen: 7.910 ng m
RT: 24.468 min Scan# 3563
Delta R.T. -0.001 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03

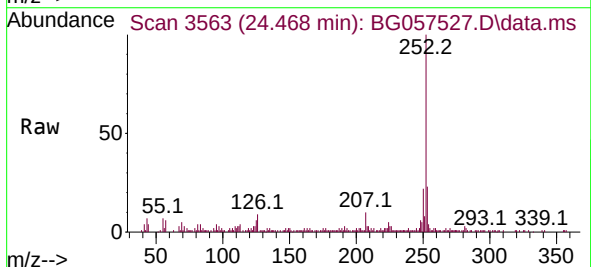


Tgt Ion:252 Resp: 74205
Ion Ratio Lower Upper
252 100
253 22.9 17.4 26.0
125 5.7 4.1 6.1

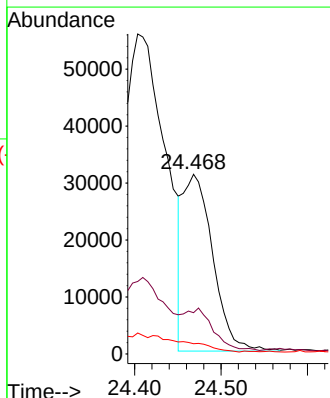

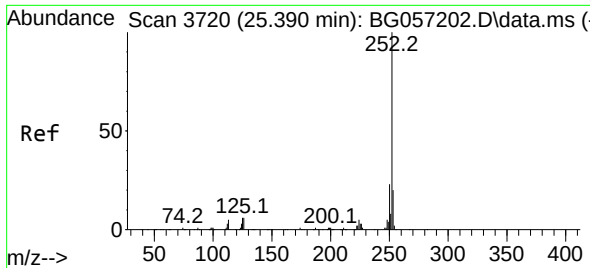

#90
Benzo(a)pyrene
Concen: 15.482 ng
RT: 25.361 min Scan# 31
Delta R.T. 0.005 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03




Instrument :
BNA_G
ClientSampleId :
WC-1

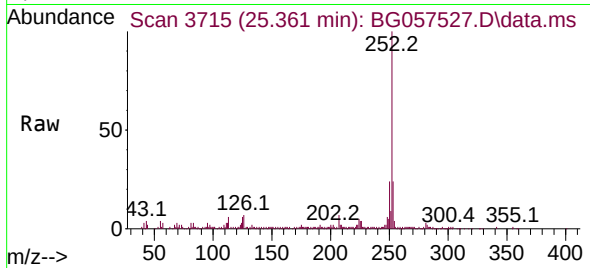


Tgt Ion:252 Resp: 13964
Ion Ratio Lower Upper
252 100
253 23.6 16.3 24.5
125 6.2 5.0 7.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

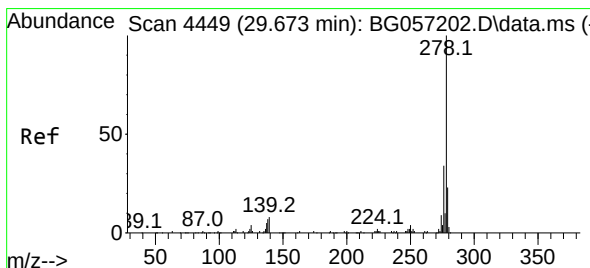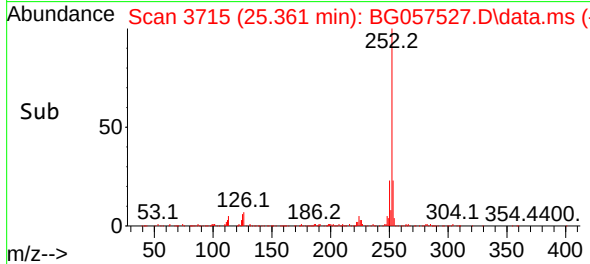


#91
Dibenzo(a,h)anthracene
Concen: 2.444 ng m
RT: 29.596 min Scan# 4436
Delta R.T. -0.013 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03

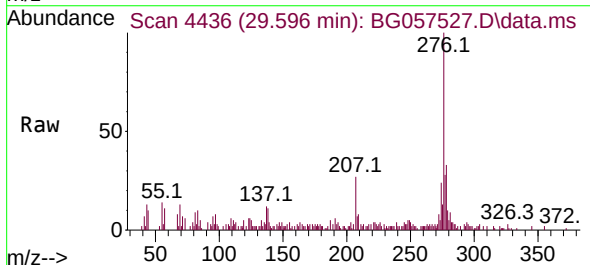


Tgt Ion:278 Resp: 20954
Ion Ratio Lower Upper
278 100
139 12.7 6.2 9.2#
279 30.4 18.6 27.8#

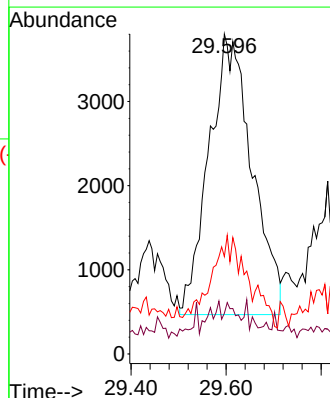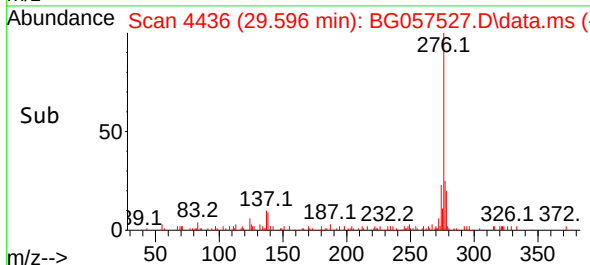

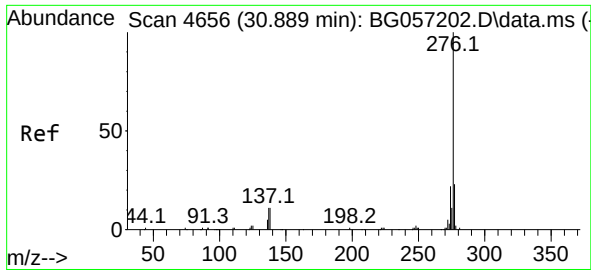

#92
Benzo(g,h,i)perylene
Concen: 8.814 ng
RT: 30.854 min Scan# 4650
Delta R.T. 0.016 min
Lab File: BG057527.D
Acq: 23 May 2023 20:03

Instrument :
BNA_G
ClientSampleId :
WC-1

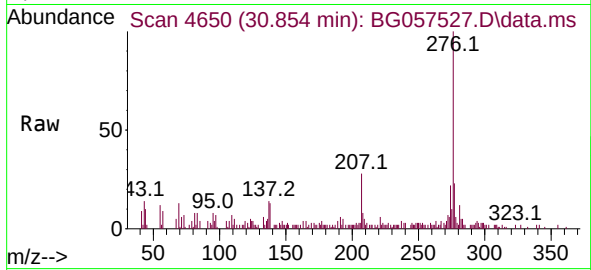

Tgt Ion:276 Resp: 73774
Ion Ratio Lower Upper
276 100
277 23.0 18.4 27.6
138 13.4 9.0 13.4

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

