
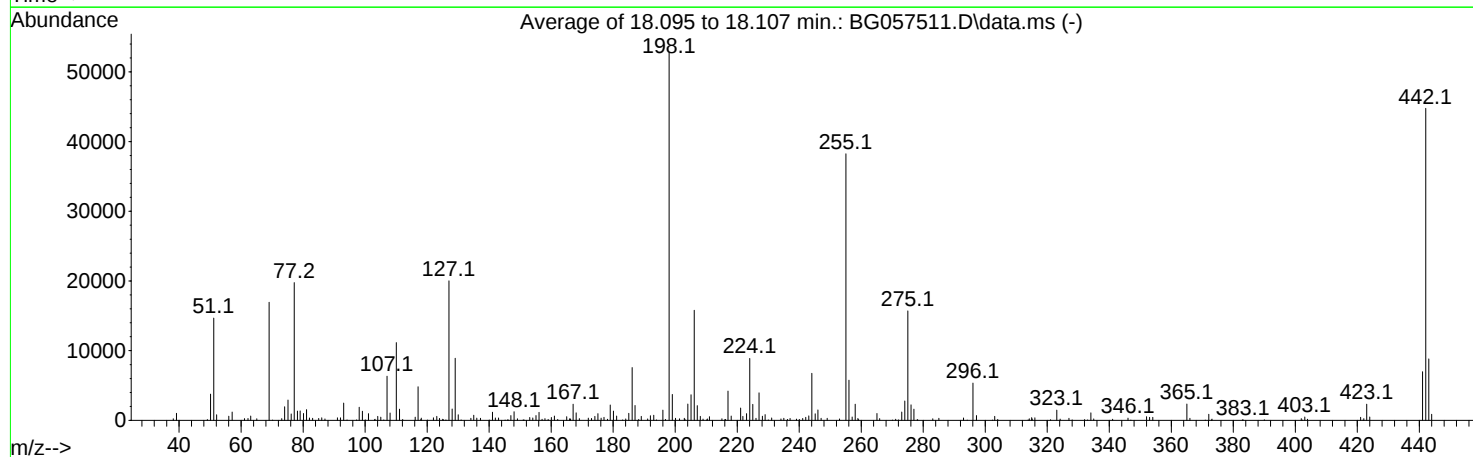


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052323\
 Data File : BG057511.D
 Acq On : 23 May 2023 9:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 20 04:19:55 2023

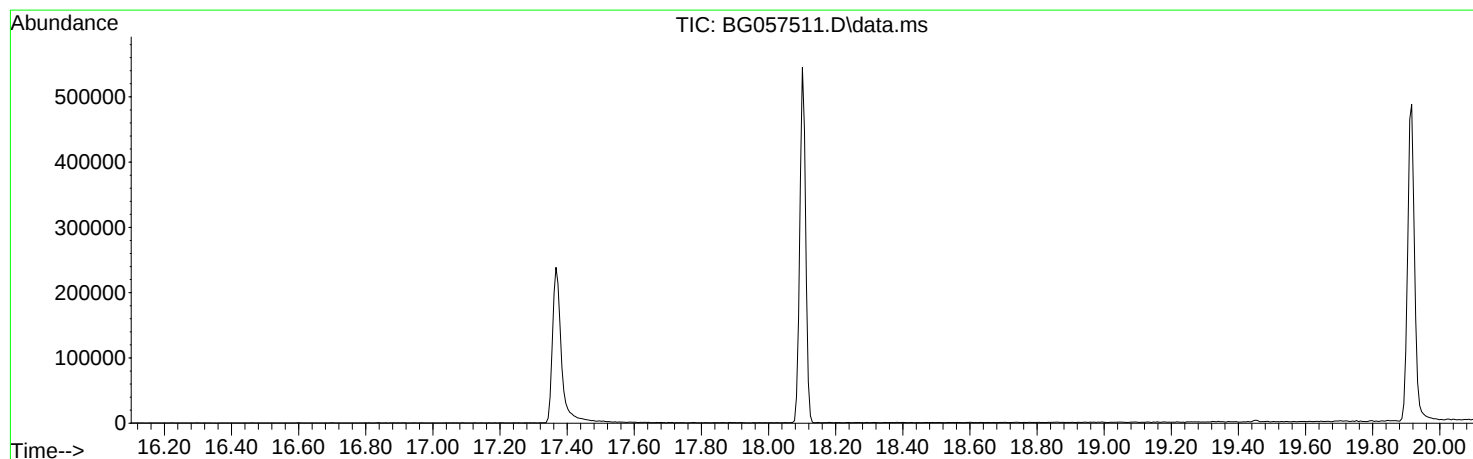

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	14663	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.1	16940	PASS
70	69	0.00	2	0.3	57	PASS
127	198	10	80	37.9	20016	PASS
197	198	0.00	2	0.3	139	PASS
198	198	100	100	100.0	52781	PASS
199	198	5	9	7.0	3715	PASS
275	198	10	60	29.8	15708	PASS
365	198	1	100	4.4	2343	PASS
441	198	0.01	100	13.2	6982	PASS
442	442	50	100	100.0	44765	PASS
443	442	15	24	19.7	8816	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/23/2023	BNA_G	<u>BG057511.D</u>
Compound Name	Response	Retention Time
DDT	160179	21.144
DDD	4502	20.692
DDE	337	20.186
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4839	165018	2.93

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052323\
Data File : BG057511.D
Acq On : 23 May 2023 9:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 23 11:23:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

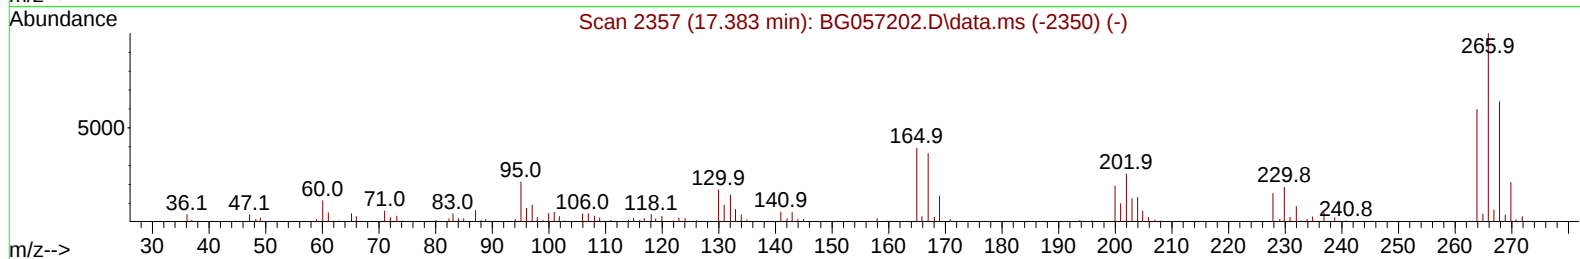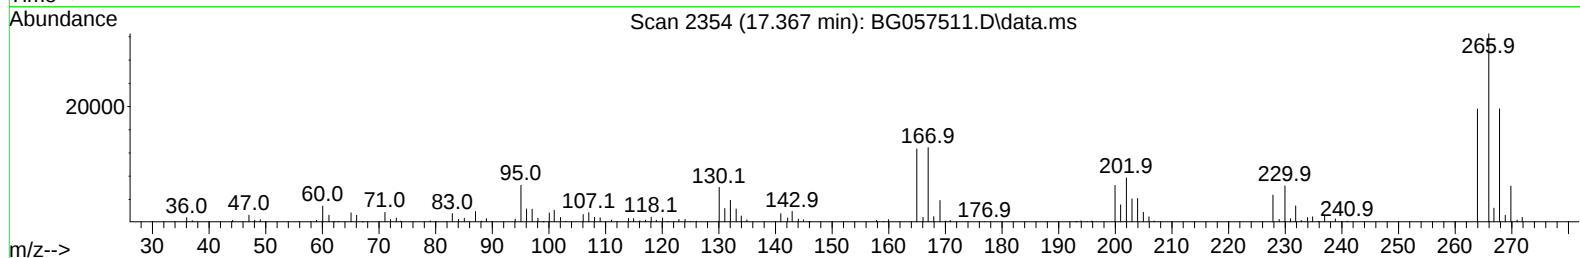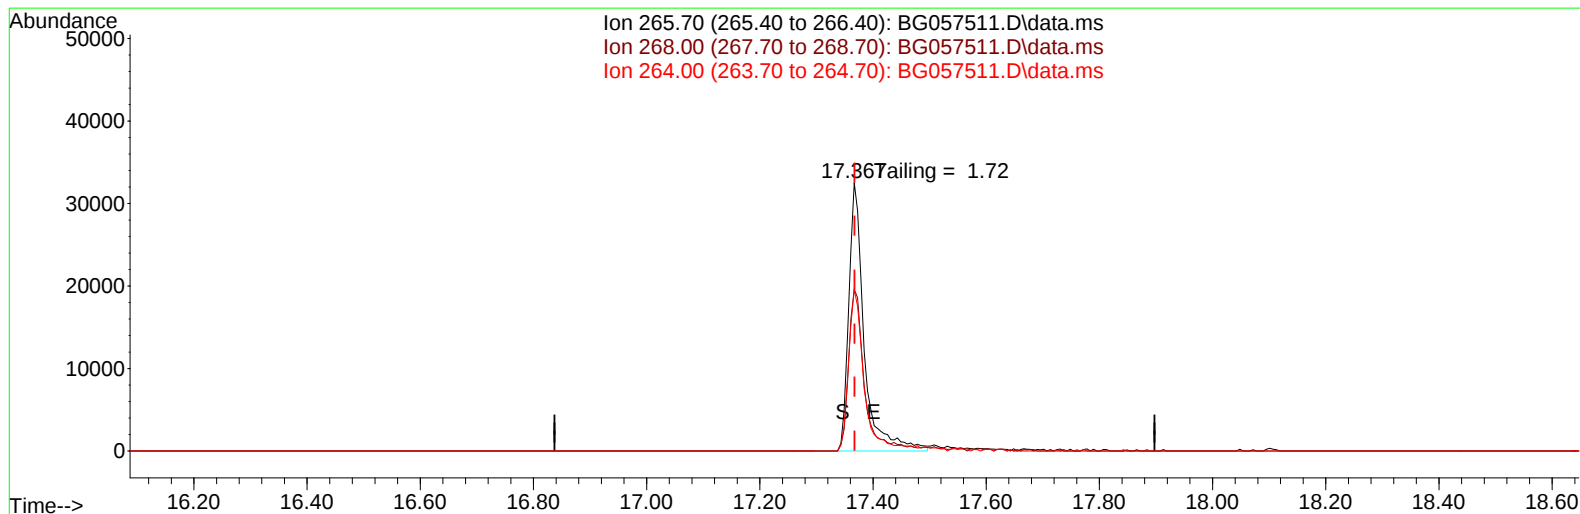

TIC: BG057511.D\data.ms

(70) Pentachlorophenol (C)

17.367min (-0.000) 62692.89 ng




response 61721

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	60.31
264.00	59.70	60.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052323\
Data File : BG057511.D
Acq On : 23 May 2023 9:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 23 11:23:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:19:55 2023
Response via : Initial Calibration

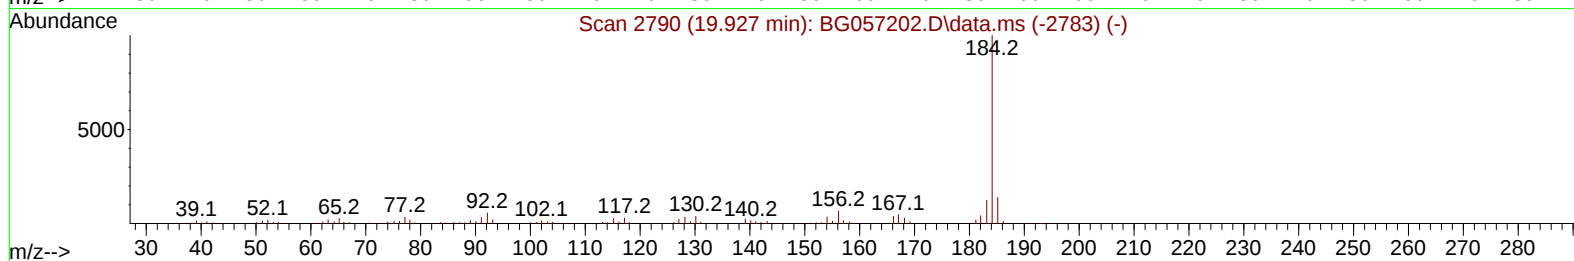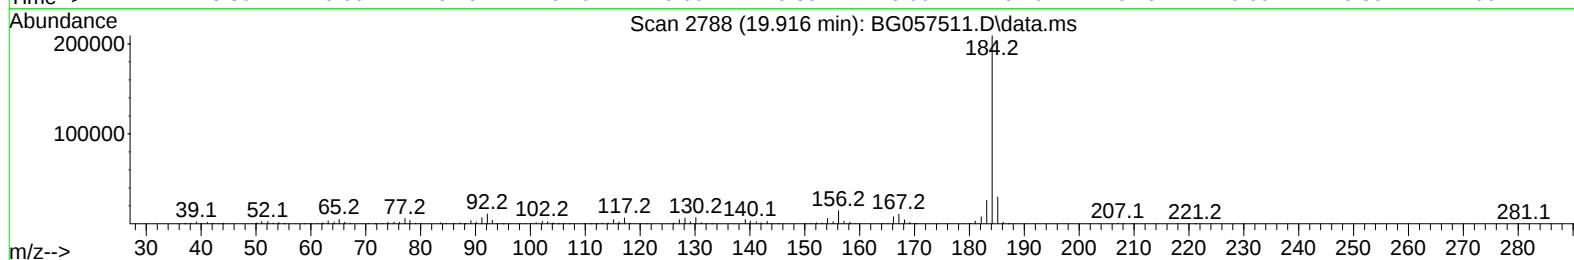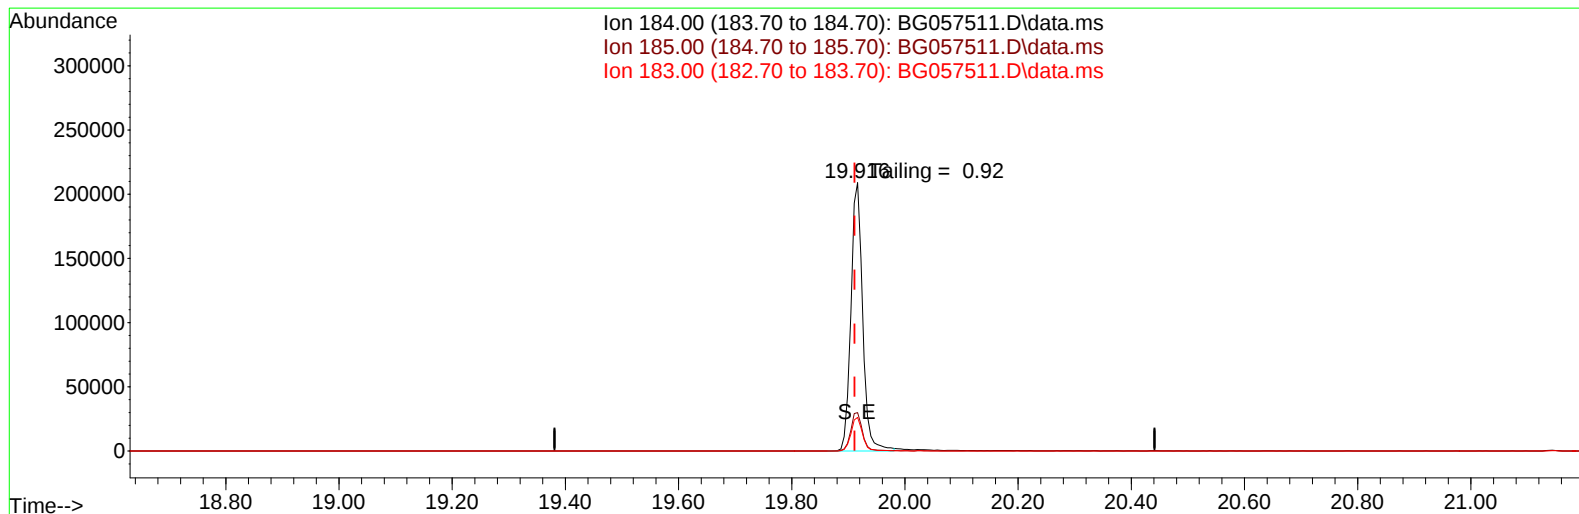

TIC: BG057511.D\data.ms

(77) Benzidine

19.916min (+ 0.005) 0.00 ng

response 302549

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.30
183.00	12.40	12.52
0.00	0.00	0.00