

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052324\
 Data File : BG061278.D
 Acq On : 23 May 2024 19:32
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc : SFAM-MDL-ME-SOIL-02
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020494

Quant Time: May 24 00:37:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 15:23:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	29147	20.000	ng/ul	0.00
20) Naphthalene-d8	10.684	136	141874	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.520	164	123129	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.270	188	321304	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.518	240	321044	20.000	ng/ul	0.00
88) Perylene-d12	24.603	264	366231	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	3713	7.129	ng/uL	0.00
4) Pyridine-d5	3.745	84	32533	17.558	ng/ul	0.00
7) Phenol-d5	7.065	99	46174	19.291	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.217	67	29056	19.313	ng/ul	0.00
11) 2-Chlorophenol-d4	7.423	132	34357	19.395	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	40913	20.046	ng/ul	0.00
21) Nitrobenzene-d5	9.039	128	20621	18.878	ng/ul	0.00
24) 2-Nitrophenol-d4	9.767	143	23860	18.664	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.314	165	47026	18.869	ng/ul	0.00
31) 4-Chloroaniline-d4	10.813	131	62625	19.207	ng/ul	0.00
46) Dimethylphthalate-d6	13.927	166	172545	18.068	ng/ul	0.00
49) Acenaphthylene-d8	14.215	160	187757	18.912	ng/ul	0.00
54) 4-Nitrophenol-d4	14.744	143	21585	18.282	ng/ul	0.00
60) Fluorene-d10	15.513	176	157585	19.113	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.649	200	33936	17.463	ng/ul	0.00
73) Anthracene-d10	17.370	188	264698	18.686	ng/ul	0.00
81) Pyrene-d10	19.656	212	313314	19.007	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.391	264	319029	18.120	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.375	88	3957	6.330	ng/uL	94
5) Pyridine	3.763	79	31522	17.200	ng/ul	92
6) Benzaldehyde	7.023	77	27690	22.124	ng/ul	97
8) Phenol	7.094	94	47311	19.399	ng/ul	96
10) Bis(2-Chloroethyl)ether	7.305	93	37126	20.812	ng/ul	88
12) 2-Chlorophenol	7.458	128	35859	19.155	ng/ul	98
13) 2-Methylphenol	8.339	108	37263	19.715	ng/ul	97
14) 2,2'-oxybis(1-Chloropr...	8.410	45	96919	20.117	ng/ul	98
16) Acetophenone	8.704	105	69145	19.851	ng/ul	93
17) N-Nitroso-di-n-propyla...	8.686	70	37153	19.399	ng/ul#	96
18) 4-Methylphenol	8.669	108	41923	20.020	ng/ul	94
19) Hexachloroethane	8.968	117	15039	18.055	ng/ul	93
22) Nitrobenzene	9.086	77	54018	18.030	ng/ul	99
23) Isophorone	9.609	82	109004	17.886	ng/ul	99
25) 2-Nitrophenol	9.797	139	25423	18.322	ng/ul	96
26) 2,4-Dimethylphenol	9.861	107	51710	18.807	ng/ul	97
27) Bis(2-Chloroethoxy)met...	10.090	93	58685	19.210	ng/ul#	98
29) 2,4-Dichlorophenol	10.337	162	45137	19.663	ng/ul	96
30) Naphthalene	10.731	128	141997	18.962	ng/ul	99
32) 4-Chloroaniline	10.837	127	60981	18.820	ng/ul	96
33) Hexachlorobutadiene	11.013	225	41108	18.321	ng/ul	98
34) Caprolactam	11.595	113	10934	12.450	ng/ul	79
35) 4-Chloro-3-methylphenol	11.976	107	56270	18.963	ng/ul#	86
36) 2-Methylnaphthalene	12.341	142	103293	19.021	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052324\
 Data File : BG061278.D
 Acq On : 23 May 2024 19:32
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc : SFAM-MDL-ME-SOIL-02
 ALS Vial : 14 Sample Multiplier: 1


Instrument :
 BNA_G
 ClientSampleId :
 SSTD020494


Quant Time: May 24 00:37:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 15:23:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.558	142	103605	18.590	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.711	216	76653	18.856	ng/ul	97
40) Hexachlorocyclopentadiene	12.687	237	37483	20.428	ng/ul#	86
41) 2,4,6-Trichlorophenol	12.958	196	43406	18.956	ng/ul	98
42) 2,4,5-Trichlorophenol	13.034	196	45899	19.035	ng/ul	94
43) 1,1'-Biphenyl	13.351	154	147235	18.493	ng/ul	97
44) 2-Chloronaphthalene	13.392	162	120222	19.187	ng/ul	97
45) 2-Nitroaniline	13.598	65	48257	18.661	ng/ul	97
47) Dimethylphthalate	13.974	163	177642	17.848	ng/ul	99
48) 2,6-Dinitrotoluene	14.097	165	37427	19.175	ng/ul	95
50) Acenaphthylene	14.244	152	208938	18.978	ng/ul	98
51) 3-Nitroaniline	14.426	138	33266	19.638	ng/ul	95
52) Acenaphthene	14.585	153	138480	19.175	ng/ul	99
53) 2,4-Dinitrophenol	14.650	184	18367	17.745	ng/ul	91
55) 4-Nitrophenol	14.761	109	24410	17.585	ng/ul	92
56) Dibenzofuran	14.920	168	194379	18.824	ng/ul	98
57) 2,4-Dinitrotoluene	14.891	165	54472	18.343	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.155	232	41187	18.728	ng/ul#	98
59) Diethylphthalate	15.343	149	180548	18.369	ng/ul	99
61) Fluorene	15.572	166	168891	18.904	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.560	204	100176	19.118	ng/ul	97
63) 4-Nitroaniline	15.590	138	34145	19.354	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.660	198	36066	17.709	ng/ul	96
67) N-Nitrosodiphenylamine	15.778	169	153251	18.977	ng/ul	98
68) 4-Bromophenyl-phenylether	16.459	248	69511	18.259	ng/ul	98
69) Hexachlorobenzene	16.583	284	79851	18.870	ng/ul	96
70) Atrazine	16.730	200	59590	18.645	ng/ul	98
71) Pentachlorophenol	16.929	266	26200	17.789	ng/ul	94
72) Phenanthrene	17.311	178	292367	18.748	ng/ul	99
74) Anthracene	17.399	178	300721	18.650	ng/ul	96
75) 1,2,3,4-Tetrachloroben...	13.322	216	79313	18.674	ng/ul	96
76) Pentachlorobenzene	14.844	250	86362	18.392	ng/ul	98
77) Carbazole	17.670	167	250057	19.066	ng/ul	99
78) Di-n-butylphthalate	18.234	149	309861	18.856	ng/ul	99
80) Fluoranthene	19.327	202	377252	19.077	ng/ul	99
82) Pyrene	19.685	202	389045	18.953	ng/ul	98
83) Butylbenzylphthalate	20.578	149	135717	19.247	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.418	252	139738	20.506	ng/ul	96
85) Benzo(a)anthracene	21.501	228	411211	18.563	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.412	149	196241	18.801	ng/ul	98
87) Chrysene	21.565	228	383859	18.819	ng/ul	99
89) Di-n-octyl phthalate	22.576	149	338758	18.489	ng/ul	100
90) Benzo(b)fluoranthene	23.627	252	394398	18.087	ng/ul	99
91) Benzo(k)fluoranthene	23.692	252	401231	18.126	ng/ul	96
93) Benzo(a)pyrene	24.462	252	378882	18.299	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.099	276	454695	18.159	ng/ul	98
95) Dibenzo(a,h)anthracene	28.157	278	382442	18.524	ng/ul	96
96) Benzo(g,h,i)perylene	29.192	276	364983	18.323	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: May 24 00:37:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 21 15:23:39 2024
Response via : Initial Calibration

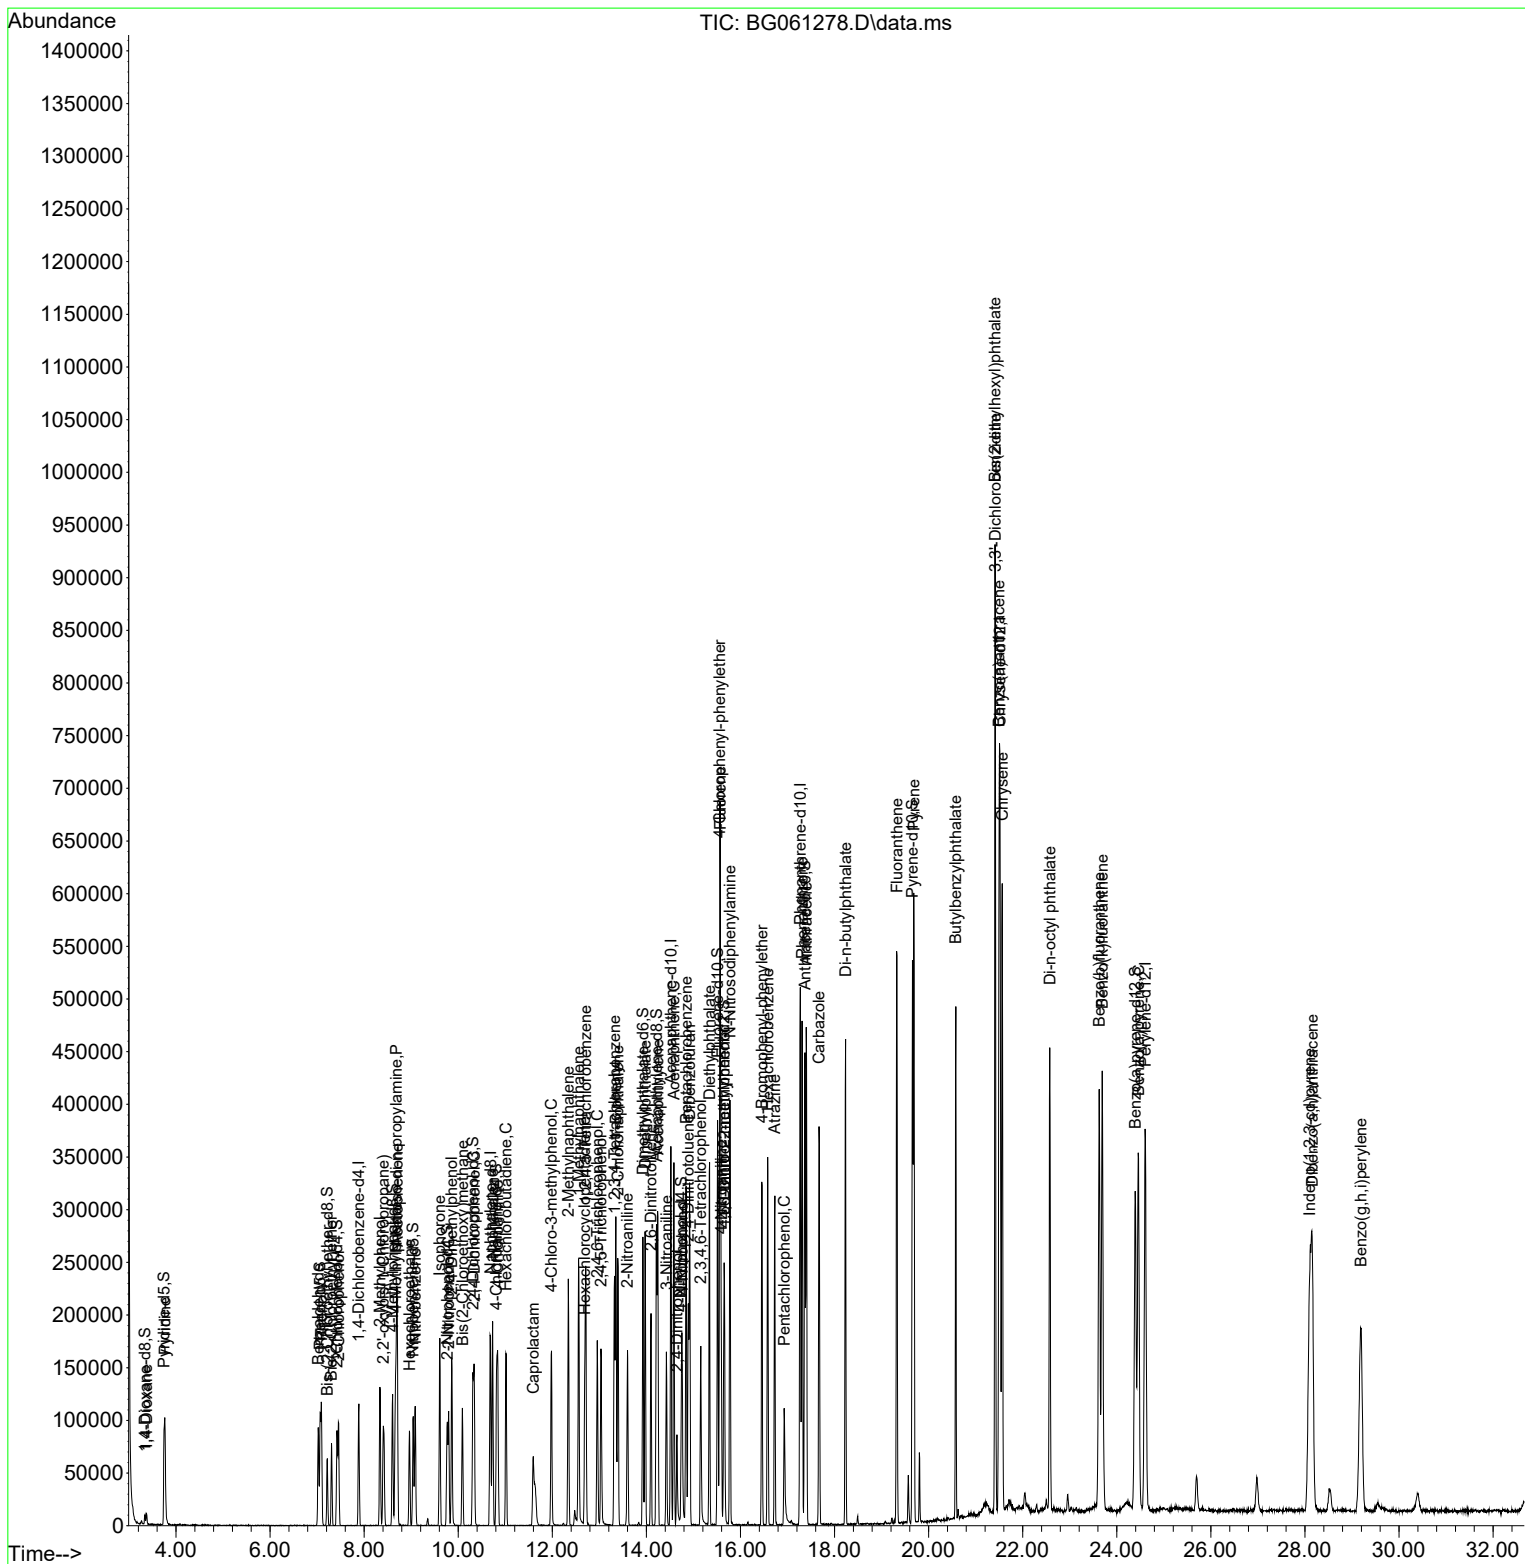



#2

1,4-Dioxane

Concen: 6.330 ng/uL

RT: 3.375 min Scan# 6

Delta R.T. 0.004 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion: 88 Resp: 3957

Ion Ratio Lower Upper

88 100

43 45.5 44.6 67.0

58 110.4 90.3 135.5

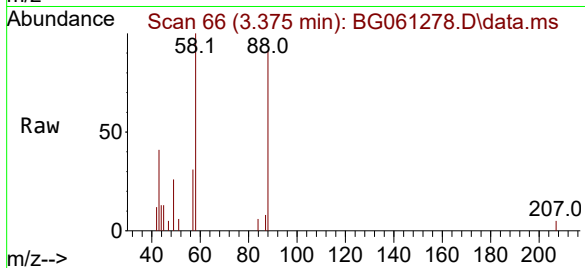

#5

Pyridine

Concen: 17.200 ng/uL

RT: 3.763 min Scan# 132

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion: 79 Resp: 31522


Ion Ratio Lower Upper

79 100

52 132.4 116.3 174.5

51 63.5 52.1 78.1




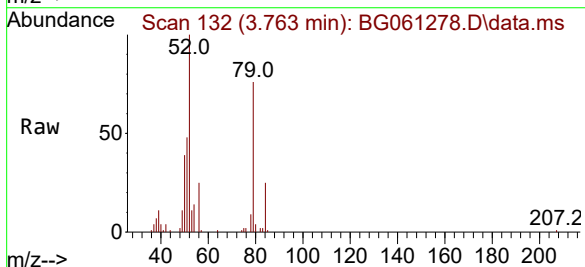




#6
Benzaldehyde
Concen: 22.124 ng/ul
RT: 7.023 min Scan# 687
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion: 77 Resp: 27690
Ion Ratio Lower Upper
77 100
105 90.4 71.0 106.6
106 83.9 63.4 95.2



#8
Phenol
Concen: 19.399 ng/ul
RT: 7.094 min Scan# 699
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion: 94 Resp: 47311
Ion Ratio Lower Upper
94 100
65 41.3 35.0 52.4
66 59.6 50.3 75.5





#10

Bis(2-Chloroethyl)ether

Concen: 20.812 ng/ul

RT: 7.305 min Scan# 7

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion: 93 Resp: 37126

Ion Ratio Lower Upper

93 100

63 91.1 86.2 129.2

95 32.7 25.8 38.8



#12

2-Chlorophenol

Concen: 19.155 ng/ul

RT: 7.458 min Scan# 761

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion:128 Resp: 35859


Ion Ratio Lower Upper

128 100

64 60.9 46.9 70.3

130 32.5 25.8 38.8

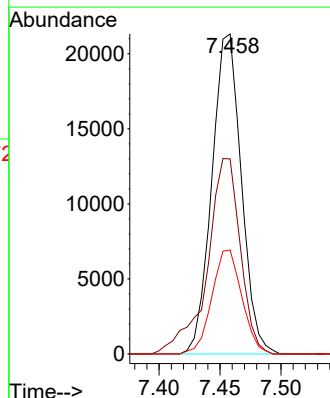



#13

2-Methylphenol

Concen: 19.715 ng/ul

RT: 8.339 min Scan# 911

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :





SSTD020494

Tgt Ion:108 Resp: 37263

Ion Ratio Lower Upper

108 100

107 89.9 69.5 104.3

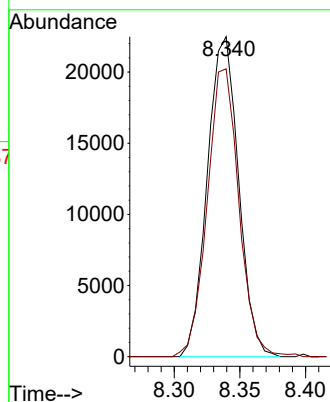

#14

2,2'-oxybis(1-Chloropropane)

Concen: 20.117 ng/ul

RT: 8.410 min Scan# 923

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion: 45 Resp: 96919


Ion Ratio Lower Upper

45 100

77 8.5 6.2 9.2

79 6.1 4.6 7.0









#16
Acetophenone
Concen: 19.851 ng/ul
RT: 8.704 min Scan# 91
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:105 Resp: 69145
Ion Ratio Lower Upper
105 100
77 79.7 70.4 105.6
51 50.0 38.4 57.6

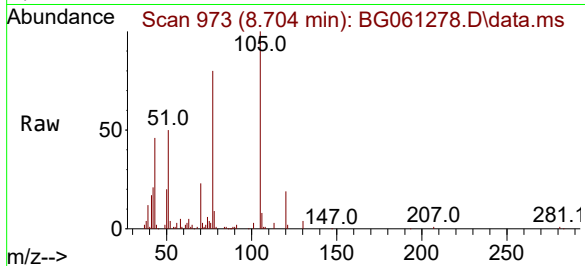

#17
N-Nitroso-di-n-propylamine
Concen: 19.399 ng/ul
RT: 8.686 min Scan# 970
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion: 70 Resp: 37153
Ion Ratio Lower Upper
70 100
42 100.5 83.2 124.8
101 10.6 6.6 9.8#
130 17.4 15.4 23.0



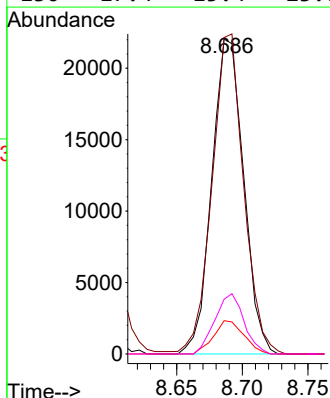
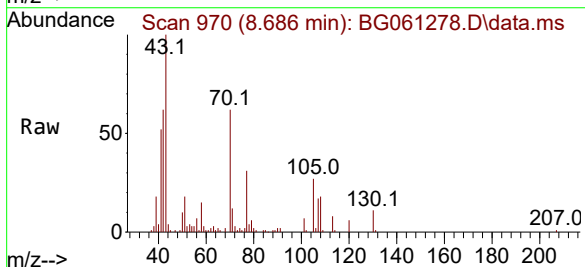




#18
4-Methylphenol
Concen: 20.020 ng/ul
RT: 8.669 min Scan# 90
Delta R.T. 0.004 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:108 Resp: 41923
Ion Ratio Lower Upper
108 100
107 104.8 89.3 133.9



#19
Hexachloroethane
Concen: 18.055 ng/ul
RT: 8.968 min Scan# 1018
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:117 Resp: 15039
Ion Ratio Lower Upper
117 100
201 141.8 110.8 166.2
199 94.1 65.1 97.7









#22
Nitrobenzene
Concen: 18.030 ng/ul
RT: 9.086 min Scan# 1038
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion: 77 Resp: 54018
Ion Ratio Lower Upper
77 100
123 41.1 32.7 49.1
65 16.8 14.2 21.2



#23
Isophorone
Concen: 17.886 ng/ul
RT: 9.609 min Scan# 1127
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion: 82 Resp: 109004
Ion Ratio Lower Upper
82 100
95 9.1 6.9 10.3
138 16.8 13.5 20.3









#25
2-Nitrophenol
Concen: 18.322 ng/ul
RT: 9.797 min Scan# 1158
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:139 Resp: 25423
Ion Ratio Lower Upper
139 100
65 66.1 56.1 84.1
109 40.9 33.8 50.6



#26
2,4-Dimethylphenol
Concen: 18.807 ng/ul
RT: 9.861 min Scan# 1170
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:107 Resp: 51710
Ion Ratio Lower Upper
107 100
121 45.2 36.4 54.6
122 78.8 65.8 98.8









#27
 Bis(2-Chloroethoxy)methane
 Concen: 19.210 ng/ul
 RT: 10.090 min Scan# 1209
 Delta R.T. -0.001 min
 Lab File: BG061278.D
 Acq: 23 May 2024 19:32




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020494


Tgt Ion: 93 Resp: 58685
 Ion Ratio Lower Upper
 93 100
 95 32.3 25.8 38.8
 123 11.8 7.2 10.8#

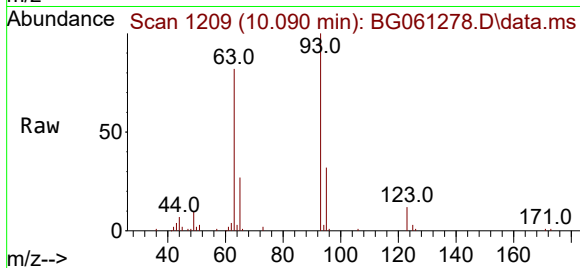

#29
 2,4-Dichlorophenol
 Concen: 19.663 ng/ul
 RT: 10.337 min Scan# 1251
 Delta R.T. -0.001 min
 Lab File: BG061278.D
 Acq: 23 May 2024 19:32

Tgt Ion:162 Resp: 45137
 Ion Ratio Lower Upper
 162 100
 164 69.3 58.4 87.6
 98 39.0 29.9 44.9




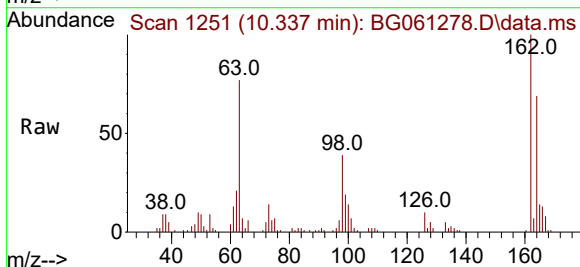




#30
Naphthalene
Concen: 18.962 ng/ul
RT: 10.731 min Scan# 1318
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:128 Resp: 141997
Ion Ratio Lower Upper
128 100
129 11.3 8.6 12.8
127 14.0 10.8 16.2



#32
4-Chloroaniline
Concen: 18.820 ng/ul
RT: 10.837 min Scan# 1336
Delta R.T. -0.007 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:127 Resp: 60981
Ion Ratio Lower Upper
127 100
129 30.0 25.9 38.9









#33
Hexachlorobutadiene
Concen: 18.321 ng/ul
RT: 11.013 min Scan# 11
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:225 Resp: 41108
Ion Ratio Lower Upper
225 100
223 66.9 53.8 80.8
227 60.2 50.2 75.2



#34
Caprolactam
Concen: 12.450 ng/ul
RT: 11.595 min Scan# 1465
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:113 Resp: 10934
Ion Ratio Lower Upper
113 100
55 291.5 199.0 298.4
56 212.3 150.6 226.0









#35
 4-Chloro-3-methylphenol
 Concen: 18.963 ng/ul
 RT: 11.976 min Scan# 1530
 Delta R.T. -0.007 min
 Lab File: BG061278.D
 Acq: 23 May 2024 19:32




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020494


Tgt Ion:107 Resp: 56270
 Ion Ratio Lower Upper
 107 100
 144 20.8 21.2 31.8#
 142 64.0 61.6 92.4

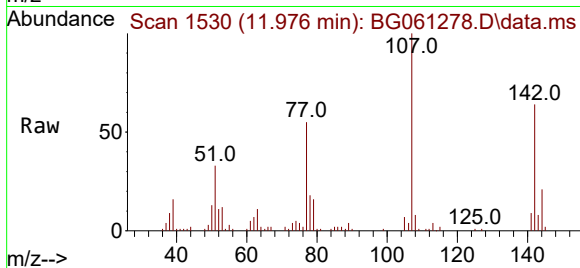

#36
 2-Methylnaphthalene
 Concen: 19.021 ng/ul
 RT: 12.341 min Scan# 1592
 Delta R.T. -0.001 min
 Lab File: BG061278.D
 Acq: 23 May 2024 19:32

Tgt Ion:142 Resp: 103293
 Ion Ratio Lower Upper
 142 100
 141 92.4 72.2 108.2

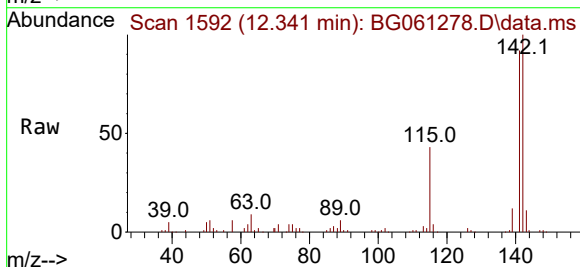



#37

1-Methylnaphthalene

Concen: 18.590 ng/ul

RT: 12.558 min Scan# 1

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:142 Resp: 103605

Ion Ratio Lower Upper

142 100

141 94.8 75.5 113.3

116 4.4 4.0 6.0



#39

1,2,4,5-Tetrachlorobenzene

Concen: 18.856 ng/ul

RT: 12.711 min Scan# 1655

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Tgt Ion:216 Resp: 76653




Ion Ratio Lower Upper


216 100

214 78.0 64.5 96.7

179 19.9 16.0 24.0

108 14.4 9.9 14.9



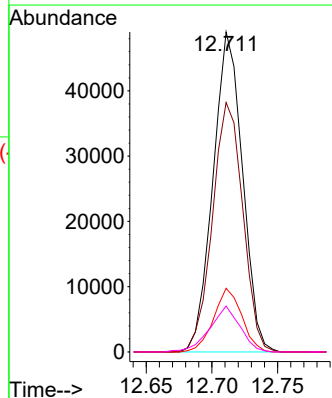





#40
Hexachlorocyclopentadiene
Concen: 20.428 ng/ul
RT: 12.687 min Scan# 1651
Delta R.T. -0.007 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:237 Resp: 37483
Ion Ratio Lower Upper
237 100
235 68.1 45.4 68.2
272 10.9 11.4 17.0#



#41
2,4,6-Trichlorophenol
Concen: 18.956 ng/ul
RT: 12.958 min Scan# 1697
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:196 Resp: 43406
Ion Ratio Lower Upper
196 100
198 100.1 78.5 117.7
200 33.1 26.1 39.1





#42

2,4,5-Trichlorophenol

Concen: 19.035 ng/ul

RT: 13.034 min Scan# 1

Delta R.T. -0.007 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:196 Resp: 45899

Ion Ratio Lower Upper

196 100

198 90.9 77.4 116.2

200 30.3 21.0 31.6



#43

1,1'-Biphenyl

Concen: 18.493 ng/ul

RT: 13.351 min Scan# 1764

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion:154 Resp: 147235


Ion Ratio Lower Upper

154 100

153 40.9 31.2 46.8

76 10.5 8.5 12.7




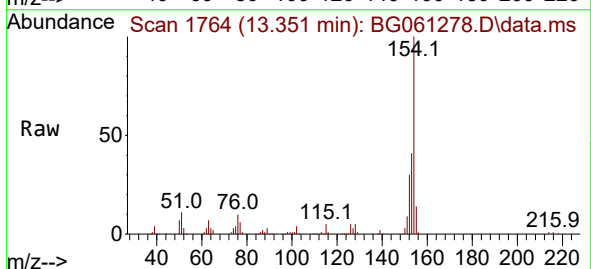




#44
2-Chloronaphthalene
Concen: 19.187 ng/ul
RT: 13.392 min Scan# 1771
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:162 Resp: 120222
Ion Ratio Lower Upper
162 100
164 35.6 26.8 40.2
127 41.7 31.9 47.9



#45
2-Nitroaniline
Concen: 18.661 ng/ul
RT: 13.598 min Scan# 1806
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion: 65 Resp: 48257
Ion Ratio Lower Upper
65 100
92 56.7 46.2 69.4
138 78.2 65.0 97.6

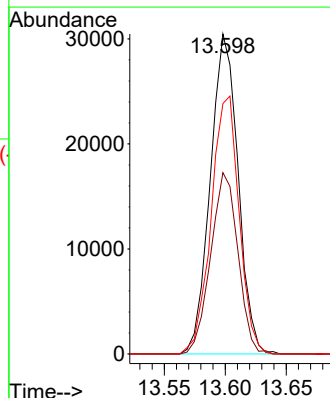



#47

Dimethylphthalate

Concen: 17.848 ng/ul

RT: 13.974 min Scan# 1870

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:163 Resp: 177642

Ion Ratio Lower Upper

163 100

194 3.8 3.1 4.7

164 10.3 8.1 12.1



#48

2,6-Dinitrotoluene

Concen: 19.175 ng/ul

RT: 14.097 min Scan# 1891

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion:165 Resp: 37427


Ion Ratio Lower Upper

165 100

89 62.0 46.0 69.0

121 21.3 17.9 26.9









#50
Acenaphthylene
Concen: 18.978 ng/ul
RT: 14.244 min Scan# 1916
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:152 Resp: 208938
Ion Ratio Lower Upper
152 100
151 21.2 16.2 24.2
153 13.6 10.2 15.4



#51
3-Nitroaniline
Concen: 19.638 ng/ul
RT: 14.426 min Scan# 1947
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:138 Resp: 33266
Ion Ratio Lower Upper
138 100
108 11.4 10.1 15.1
92 127.5 97.6 146.4









#52
Acenaphthene
Concen: 19.175 ng/ul
RT: 14.585 min Scan# 1974
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:153 Resp: 138480
Ion Ratio Lower Upper
153 100
152 48.6 37.8 56.8
154 85.8 69.0 103.6



#53
2,4-Dinitrophenol
Concen: 17.745 ng/ul
RT: 14.650 min Scan# 1985
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:184 Resp: 18367
Ion Ratio Lower Upper
184 100
63 82.9 61.3 91.9
154 77.1 55.0 82.4









#55
4-Nitrophenol
Concen: 17.585 ng/ul
RT: 14.761 min Scan# 2004
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:109 Resp: 24410
Ion Ratio Lower Upper
109 100
139 102.9 74.9 112.3
65 122.9 104.0 156.0

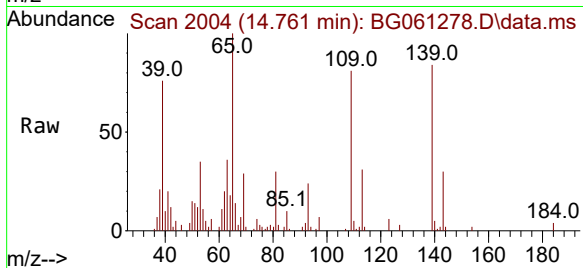

#56
Dibenzofuran
Concen: 18.824 ng/ul
RT: 14.920 min Scan# 2031
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:168 Resp: 194379
Ion Ratio Lower Upper
168 100
139 40.3 33.4 50.2

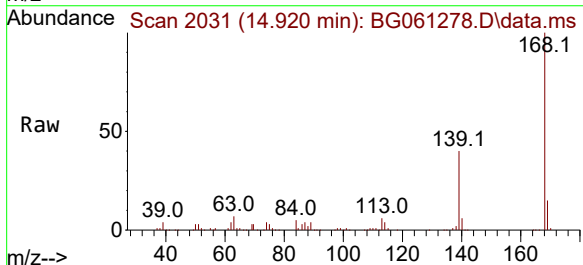



#57

2,4-Dinitrotoluene

Concen: 18.343 ng/ul

RT: 14.891 min Scan# 20

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:165 Resp: 54472

Ion Ratio Lower Upper

165 100

63 52.3 43.4 65.2

182 2.7 2.0 3.0



#58

2,3,4,6-Tetrachlorophenol

Concen: 18.728 ng/ul

RT: 15.155 min Scan# 2071

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Tgt Ion:232 Resp: 41187




Ion Ratio Lower Upper


232 100

131 38.2 30.2 45.2

130 0.0 1.8 2.6#

166 24.9 21.0 31.6


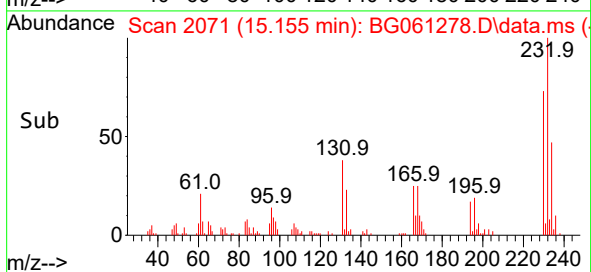






#59
Diethylphthalate
Concen: 18.369 ng/ul
RT: 15.343 min Scan# 2103
Delta R.T. 0.004 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:149 Resp: 180548
Ion Ratio Lower Upper
149 100
177 23.9 19.1 28.7
150 13.1 11.0 16.4



#61
Fluorene
Concen: 18.904 ng/ul
RT: 15.572 min Scan# 2142
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:166 Resp: 168891
Ion Ratio Lower Upper
166 100
165 102.1 81.8 122.8
167 13.2 10.6 16.0





#62

4-Chlorophenyl-phenylether

Concen: 19.118 ng/ul

RT: 15.560 min Scan# 2141

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:204 Resp: 100176

Ion Ratio Lower Upper

204 100

206 32.0 26.3 39.5

141 56.5 43.0 64.6



#63

4-Nitroaniline

Concen: 19.354 ng/ul

RT: 15.590 min Scan# 2145

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion:138 Resp: 34145


Ion Ratio Lower Upper

138 100

92 61.4 48.6 73.0

108 119.8 95.5 143.3



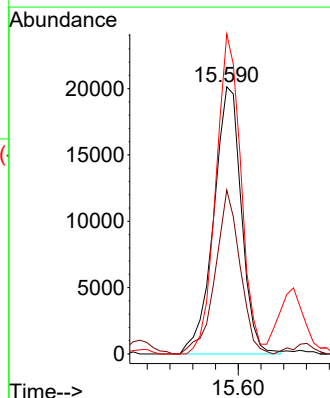





#66
4,6-Dinitro-2-methylphenol
Concen: 17.709 ng/ul
RT: 15.660 min Scan# 2158
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:198 Resp: 36066
Ion Ratio Lower Upper
198 100
182 3.1 2.9 4.3
77 25.7 22.3 33.5



#67
N-Nitrosodiphenylamine
Concen: 18.977 ng/ul
RT: 15.778 min Scan# 2177
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:169 Resp: 153251
Ion Ratio Lower Upper
169 100
168 67.1 51.9 77.9
167 35.6 29.4 44.2



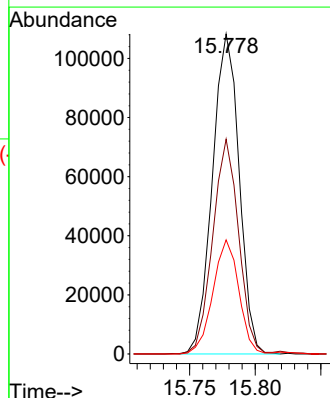





#68
4-Bromophenyl-phenylether
Concen: 18.259 ng/ul
RT: 16.459 min Scan# 21
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:248 Resp: 69511
Ion Ratio Lower Upper
248 100
250 101.2 79.4 119.2
141 65.3 50.2 75.4



#69
Hexachlorobenzene
Concen: 18.870 ng/ul
RT: 16.583 min Scan# 2314
Delta R.T. 0.004 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:284 Resp: 79851
Ion Ratio Lower Upper
284 100
142 26.3 21.2 31.8
249 32.2 28.7 43.1

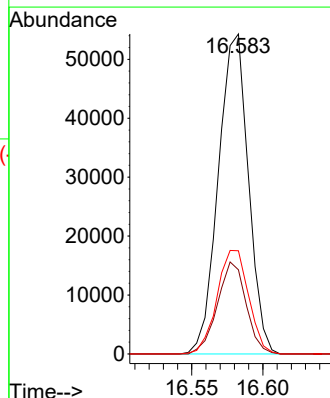



#70

Atrazine

Concen: 18.645 ng/ul

RT: 16.730 min Scan# 21

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:200 Resp: 59590

Ion Ratio Lower Upper

200 100

173 21.2 15.9 23.9

215 47.3 37.3 55.9



#71

Pentachlorophenol

Concen: 17.789 ng/ul

RT: 16.929 min Scan# 2373

Delta R.T. -0.007 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion:266 Resp: 26200


Ion Ratio Lower Upper

266 100

264 61.7 41.9 62.9

268 65.8 52.6 79.0





#72

Phenanthrene

Concen: 18.748 ng/ul

RT: 17.311 min Scan# 2438

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:178 Resp: 292367

Ion Ratio Lower Upper

178 100

179 15.1 12.7 19.1

176 19.3 15.5 23.3



#74

Anthracene

Concen: 18.650 ng/ul

RT: 17.399 min Scan# 2453

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion:178 Resp: 300721


Ion Ratio Lower Upper

178 100

179 16.2 11.8 17.6

176 20.2 14.9 22.3









#75
1,2,3,4-Tetrachlorobenzene
Concen: 18.674 ng/uL
RT: 13.322 min Scan# 1759
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:216 Resp: 79313
Ion Ratio Lower Upper
216 100
214 80.5 60.0 90.0
218 48.4 38.5 57.7



#76
Pentachlorobenzene
Concen: 18.392 ng/uL
RT: 14.844 min Scan# 2018
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:250 Resp: 86362
Ion Ratio Lower Upper
250 100
248 63.6 52.6 79.0
252 66.5 54.7 82.1







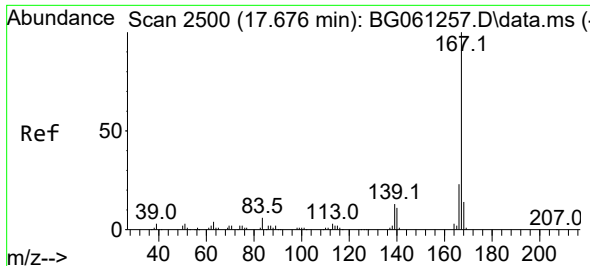

#77
 Carbazole
 Concen: 19.066 ng/ul
 RT: 17.670 min Scan# 2499
 Delta R.T. -0.007 min
 Lab File: BG061278.D
 Acq: 23 May 2024 19:32




Instrument :
 BNA_G
 ClientSampleId :
 SST020494


Tgt Ion:167 Resp: 250057
 Ion Ratio Lower Upper
 167 100
 166 22.6 18.6 28.0
 139 13.1 10.6 15.8

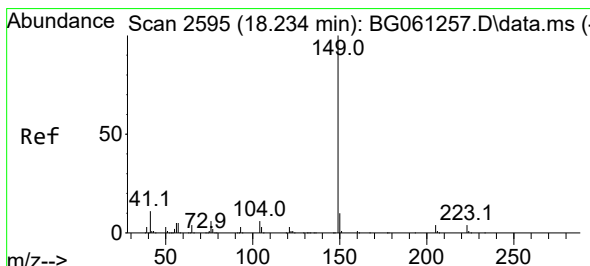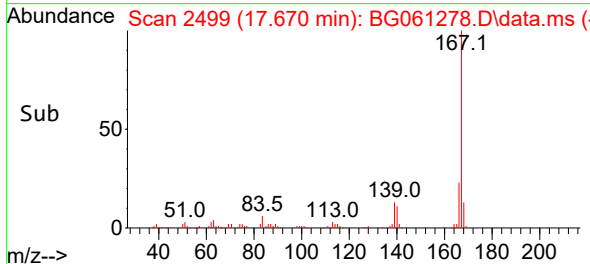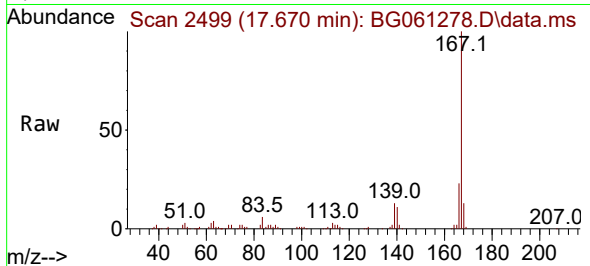

#78
 Di-n-butylphthalate
 Concen: 18.856 ng/ul
 RT: 18.234 min Scan# 2595
 Delta R.T. -0.001 min
 Lab File: BG061278.D
 Acq: 23 May 2024 19:32

Tgt Ion:149 Resp: 309861
 Ion Ratio Lower Upper
 149 100
 150 9.5 7.8 11.8
 104 5.5 4.8 7.2


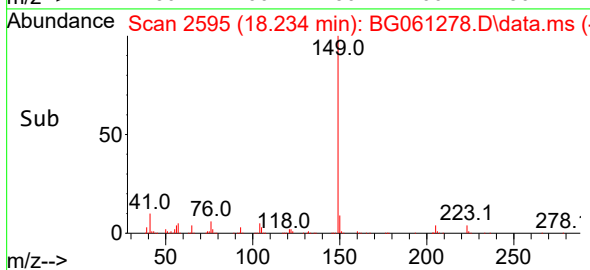

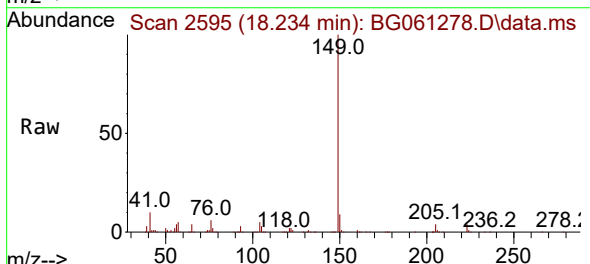




#80
Fluoranthene
Concen: 19.077 ng/u1
RT: 19.327 min Scan# 21
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32




Instrument :
BNA_G
ClientSampleId :
SSTD020494


Tgt Ion:202 Resp: 377252
Ion Ratio Lower Upper
202 100
101 6.1 4.8 7.2
100 4.6 4.1 6.1



#82
Pyrene
Concen: 18.953 ng/u1
RT: 19.685 min Scan# 2842
Delta R.T. -0.001 min
Lab File: BG061278.D
Acq: 23 May 2024 19:32

Tgt Ion:202 Resp: 389045
Ion Ratio Lower Upper
202 100
101 8.1 5.7 8.5
100 6.4 5.1 7.7





#83

Butylbenzylphthalate

Concen: 19.247 ng/ul

RT: 20.578 min Scan# 2994

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:149 Resp: 135717

Ion Ratio Lower Upper

149 100

91 73.5 54.8 82.2

206 25.2 19.4 29.0



#84

3,3'-Dichlorobenzidine

Concen: 20.506 ng/ul

RT: 21.418 min Scan# 3137

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion:252 Resp: 139738


Ion Ratio Lower Upper

252 100

254 62.7 52.7 79.1

126 6.8 5.0 7.6





#85

Benzo(a)anthracene

Concen: 18.563 ng/ul

RT: 21.501 min Scan# 3151

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:228 Resp: 411211

Ion Ratio Lower Upper

228 100

229 19.1 15.2 22.8

226 27.3 21.4 32.2



#86

Bis(2-ethylhexyl)phthalate

Concen: 18.801 ng/ul

RT: 21.412 min Scan# 3136

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion:149 Resp: 196241


Ion Ratio Lower Upper

149 100

167 27.3 21.1 31.7

279 4.4 3.3 4.9





#87

Chrysene

Concen: 18.819 ng/ul

RT: 21.565 min Scan# 3162

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:228 Resp: 383859

Ion Ratio Lower Upper

228 100

226 29.9 23.4 35.0

229 19.1 15.4 23.2



#89

Di-n-octyl phthalate

Concen: 18.489 ng/ul




RT: 22.576 min Scan# 3334


Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Tgt Ion:149 Resp: 338758





#90

Benzo(b)fluoranthene

Concen: 18.087 ng/ul

RT: 23.627 min Scan# 3513

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:252 Resp: 394398

Ion Ratio Lower Upper

252 100

253 21.9 17.8 26.8

125 5.9 4.6 6.8



#91

Benzo(k)fluoranthene

Concen: 18.126 ng/ul

RT: 23.692 min Scan# 3524

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion:252 Resp: 401231


Ion Ratio Lower Upper

252 100

253 22.5 16.0 24.0

125 5.5 4.3 6.5





#93

Benzo(a)pyrene

Concen: 18.299 ng/ul

RT: 24.462 min Scan# 3

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:252 Resp: 378882

Ion Ratio Lower Upper

252 100

253 20.7 16.4 24.6

125 6.3 4.3 6.5



#94

Indeno(1,2,3-cd)pyrene

Concen: 18.159 ng/ul

RT: 28.099 min Scan# 4274

Delta R.T. -0.007 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32




Tgt Ion:276 Resp: 454695


Ion Ratio Lower Upper

276 100

138 11.9 8.6 13.0

277 24.1 19.7 29.5





#95

Dibenzo(a,h)anthracene

Concen: 18.524 ng/ul

RT: 28.157 min Scan# 41

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Instrument :

BNA_G

ClientSampleId :

SSTD020494





Tgt Ion:278 Resp: 382442

Ion Ratio Lower Upper

278 100

139 8.5 6.4 9.6

279 22.7 19.9 29.9



#96

Benzo(g,h,i)perylene

Concen: 18.323 ng/ul

RT: 29.192 min Scan# 4460

Delta R.T. -0.001 min

Lab File: BG061278.D

Acq: 23 May 2024 19:32

Tgt Ion:276 Resp: 364983

Ion Ratio Lower Upper

276 100

138 11.7 8.7 13.1

277 23.1 18.2 27.2

