
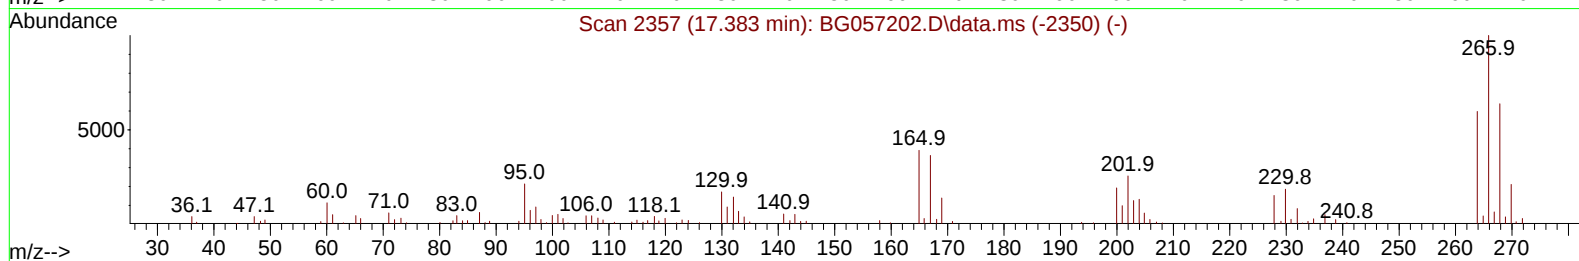
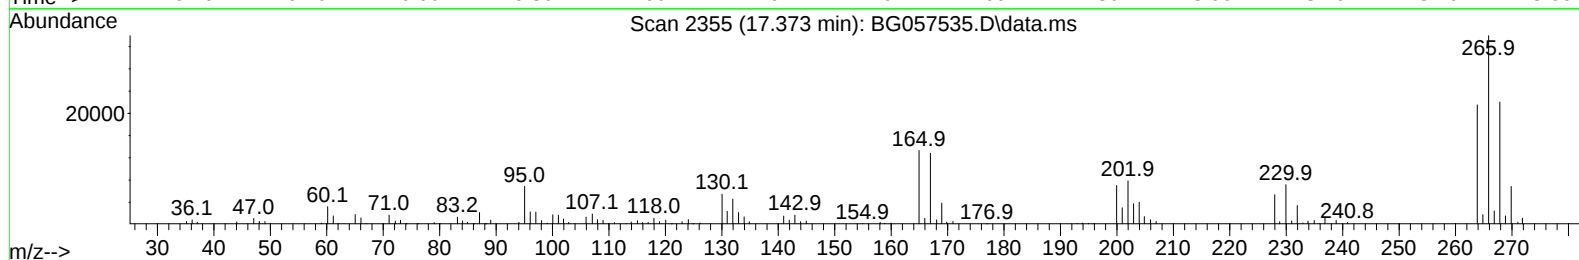


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
Data File : BG057535.D
Acq On : 24 May 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 16:09:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 12:22:35 2023
Response via : Initial Calibration

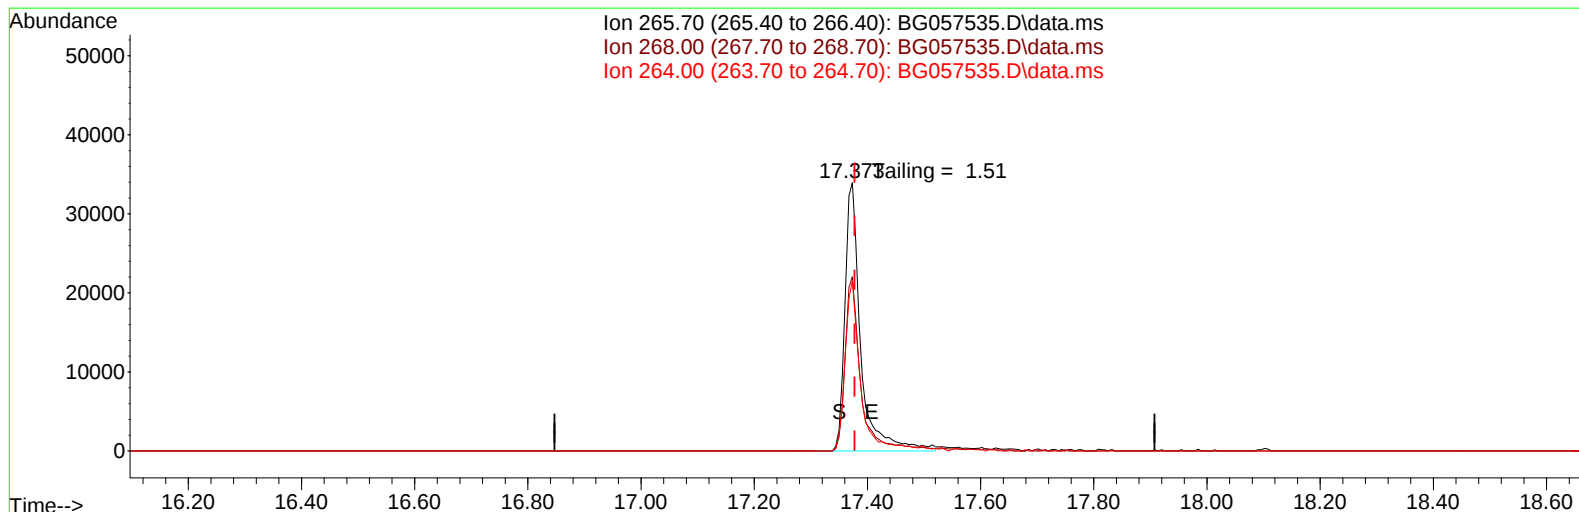

TIC: BG057535.D\data.ms

(70) Pentachlorophenol (C)




17.373min (-0.004) 36634.42 ng

response 65621

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.94
264.00	59.70	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
Data File : BG057535.D
Acq On : 24 May 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 16:09:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 12:22:35 2023
Response via : Initial Calibration

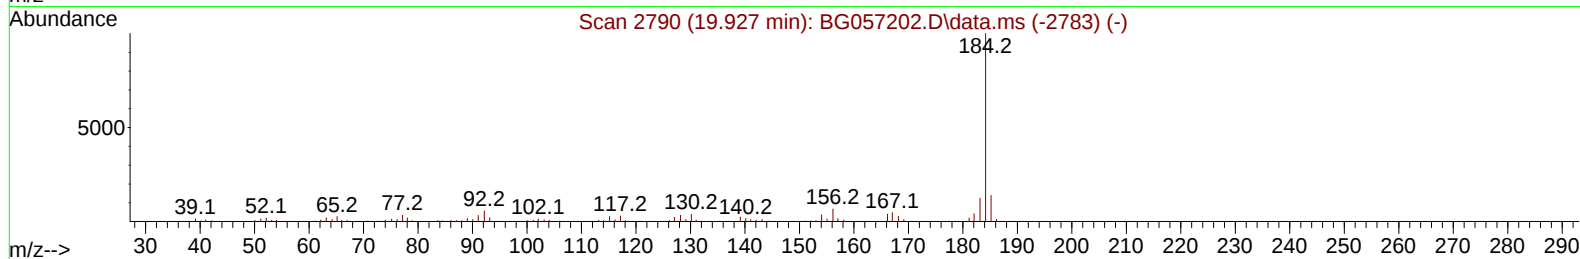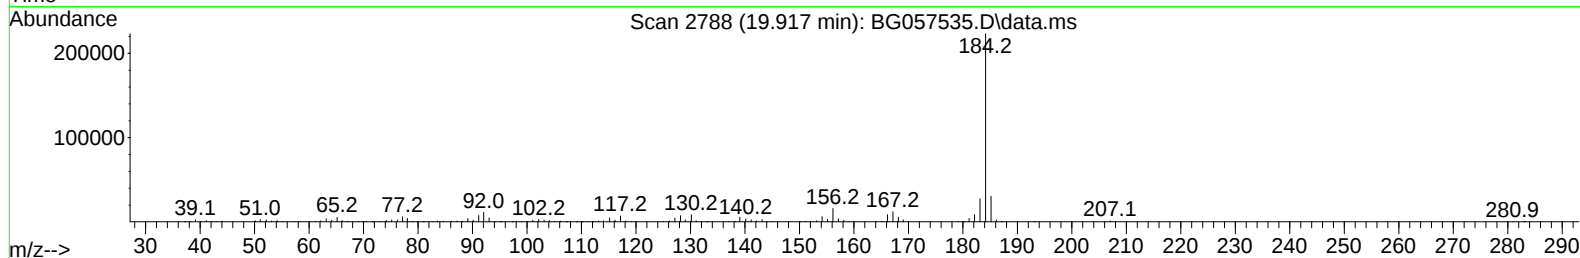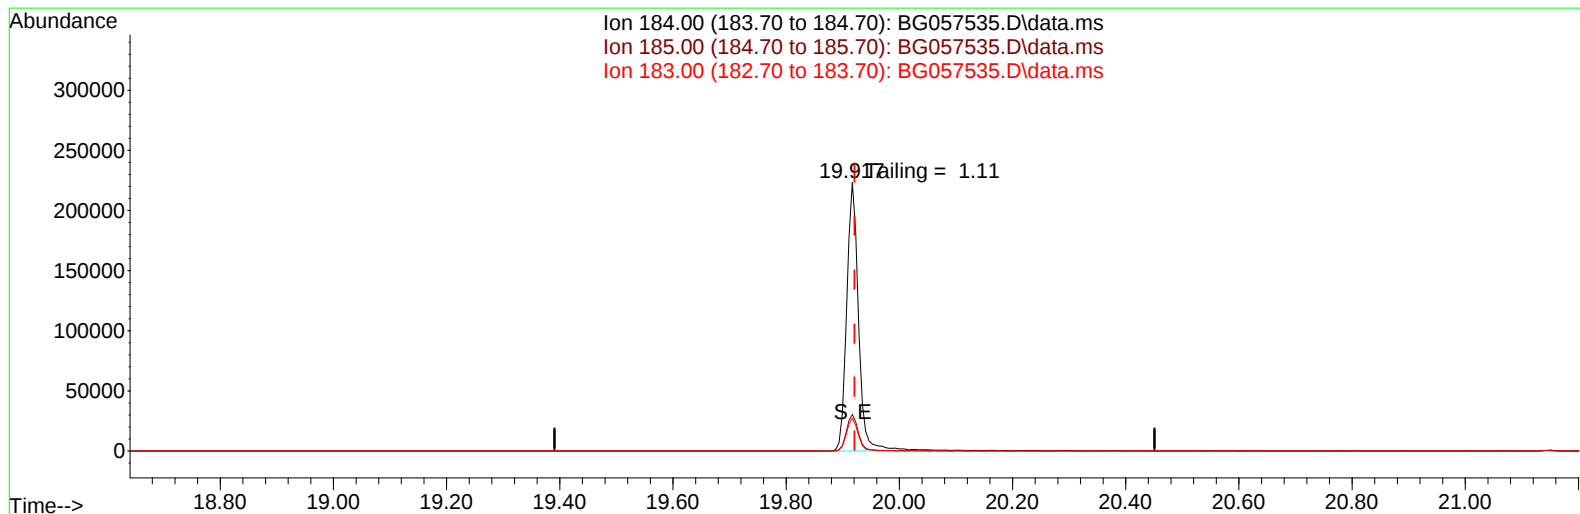

TIC: BG057535.D\data.ms

(77) Benzidine

19.917min (-0.004) 0.00 ng

response 325978

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.61
183.00	12.40	12.30
0.00	0.00	0.00