

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
 Data File : BG057550.D
 Acq On : 25 May 2023 1:47
 Operator : CG/JU
 Sample : 02899-04 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057550.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.394	309	316	321	rBV2	2456	3532	1.03%	0.171%
2	5.882	392	399	406	rBV	42053	71165	20.74%	3.446%
3	7.509	669	676	686	rBV	44949	80418	23.44%	3.894%
4	8.355	814	820	829	rBV	82704	138151	40.27%	6.689%
5	9.535	1014	1021	1029	rBV	27518	48616	14.17%	2.354%
6	11.192	1296	1303	1313	rBV	107965	192934	56.24%	9.341%
7	13.595	1706	1712	1723	rVB	85212	131607	38.36%	6.372%
8	14.975	1939	1947	1955	rBV	179069	280901	81.88%	13.601%
9	16.309	2170	2174	2178	rBV3	6584	8644	2.52%	0.419%
10	16.455	2193	2199	2207	rBV2	60778	94449	27.53%	4.573%
11	17.713	2405	2413	2418	rBV	221863	343053	100.00%	16.610%
12	17.754	2418	2420	2426	rVB	15329	20807	6.07%	1.007%
13	17.842	2433	2435	2438	rBV3	4805	4278	1.25%	0.207%
14	18.118	2479	2482	2484	rBV3	3105	4158	1.21%	0.201%
15	18.553	2552	2556	2558	rBV4	7855	10849	3.16%	0.525%
16	18.700	2579	2581	2584	rVB4	4125	3498	1.02%	0.169%
17	19.070	2640	2644	2648	rBV6	6149	10647	3.10%	0.516%
18	19.745	2755	2759	2764	rBV	42653	55078	16.06%	2.667%
19	20.109	2817	2821	2826	rVB	40055	55553	16.19%	2.690%
20	20.280	2845	2850	2854	rBV	154686	201043	58.60%	9.734%
21	22.019	3141	3146	3152	rVB	180213	305973	89.19%	14.815%




Sum of corrected areas: 2065354

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
Data File : BG057550.D
Acq On : 25 May 2023 1:47
Operator : CG/JU
Sample : 02899-04 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

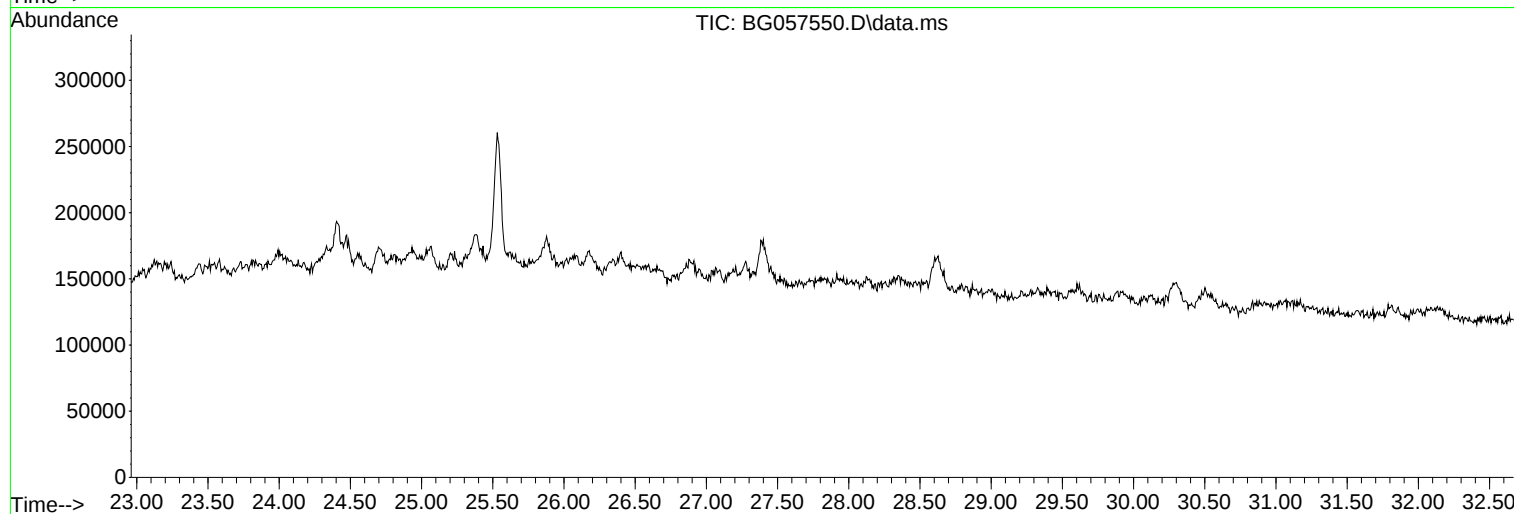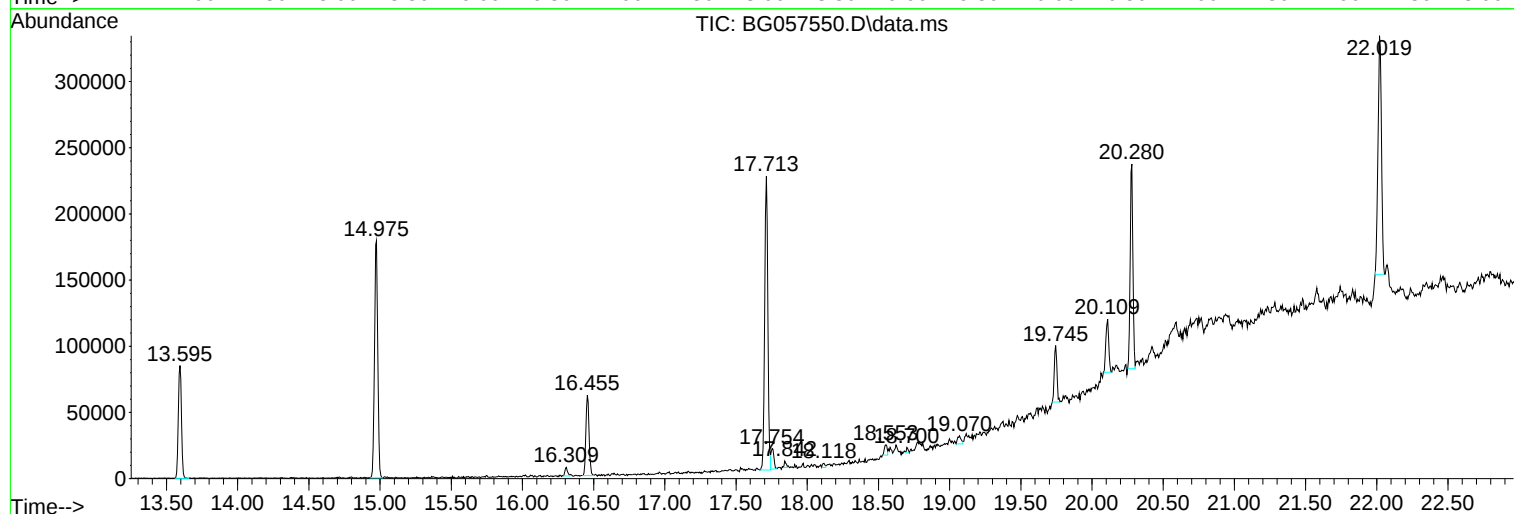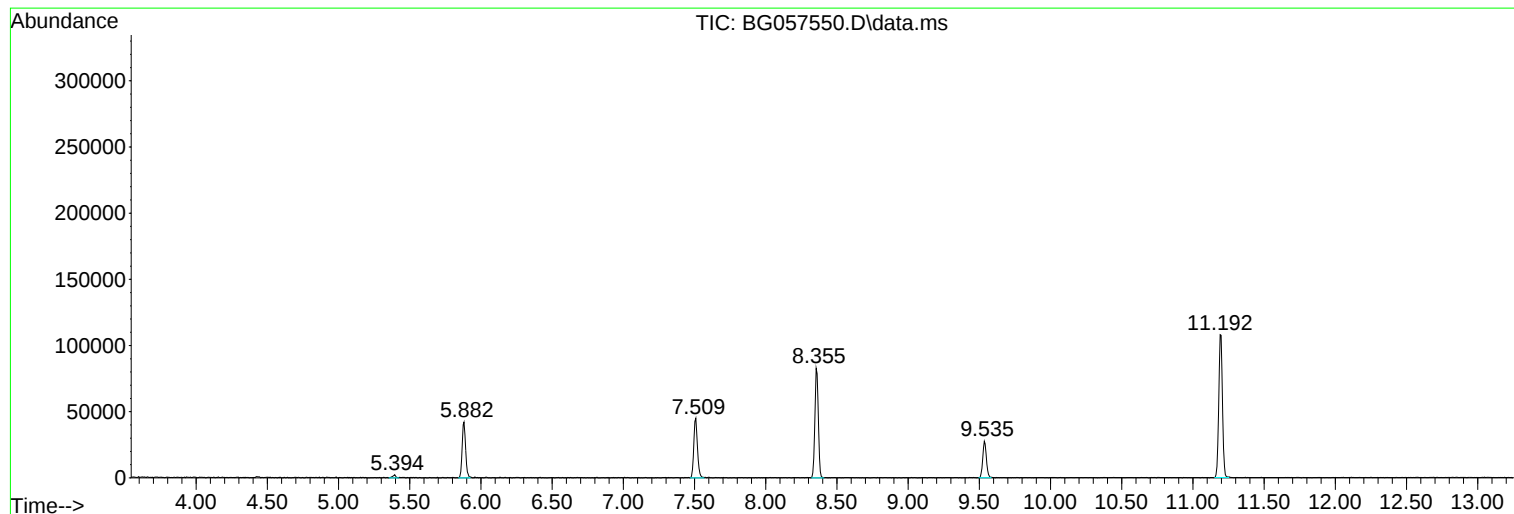

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
Data File : BG057550.D
Acq On : 25 May 2023 1:47
Operator : CG/JU
Sample : 02899-04 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
Data File : BG057550.D
Acq On : 25 May 2023 1:47
Operator : CG/JU
Sample : 02899-04 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------