
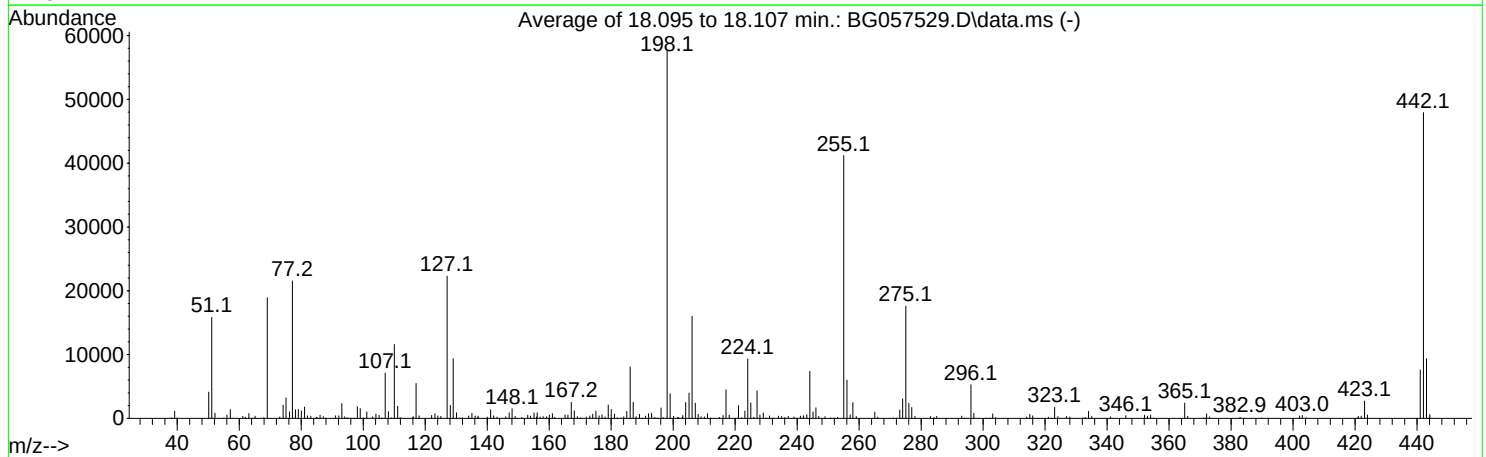


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
Data File : BG057529.D
Acq On : 24 May 2023 9:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 25 10:58:38 2023

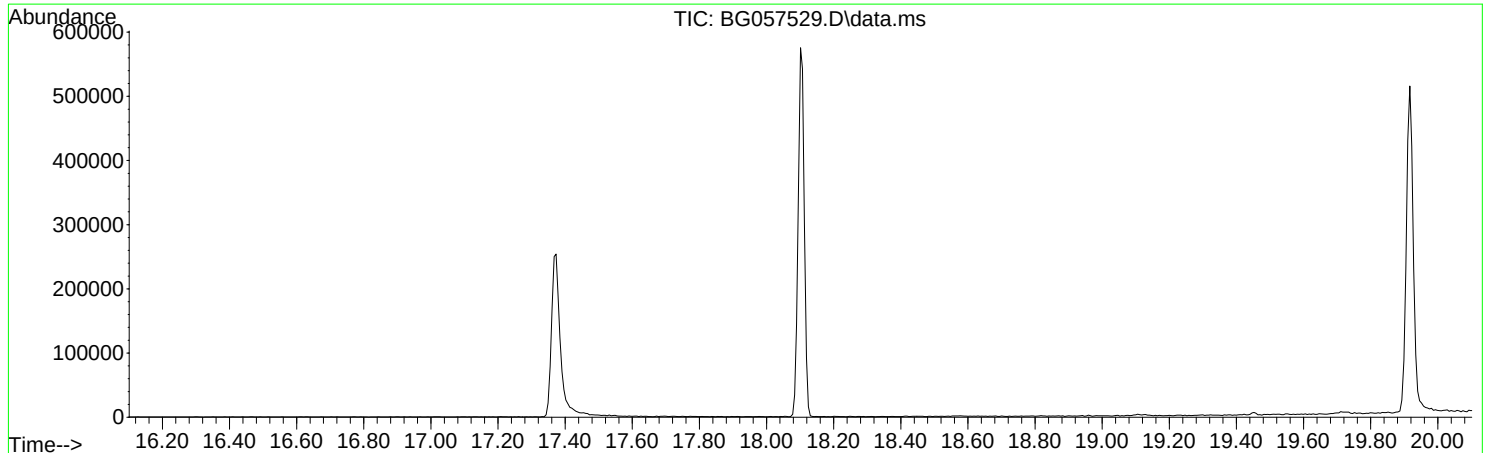

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	15832	PASS
68	69	0.00	2	0.6	121	PASS
69	198	0.00	100	32.8	18907	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.7	22304	PASS
197	198	0.00	2	0.2	130	PASS
198	198	100	100	100.0	57661	PASS
199	198	5	9	6.7	3860	PASS
275	198	10	60	30.5	17595	PASS
365	198	1	100	4.2	2411	PASS
441	198	0.01	100	13.2	7593	PASS
442	442	50	100	100.0	47925	PASS
443	442	15	24	19.5	9351	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/24/2023	BNA_G	<u>BG057529.D</u>
Compound Name	Response	Retention Time
DDT	161547	21.15
DDD	4283	20.692
DDE	388	20.187
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4671	166218	2.81

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
Data File : BG057529.D
Acq On : 24 May 2023 9:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 24 12:36:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 12:22:35 2023
Response via : Initial Calibration

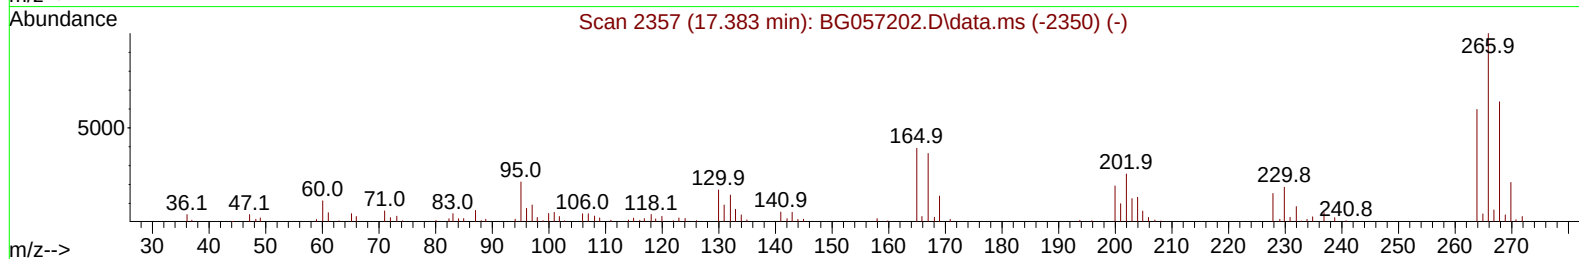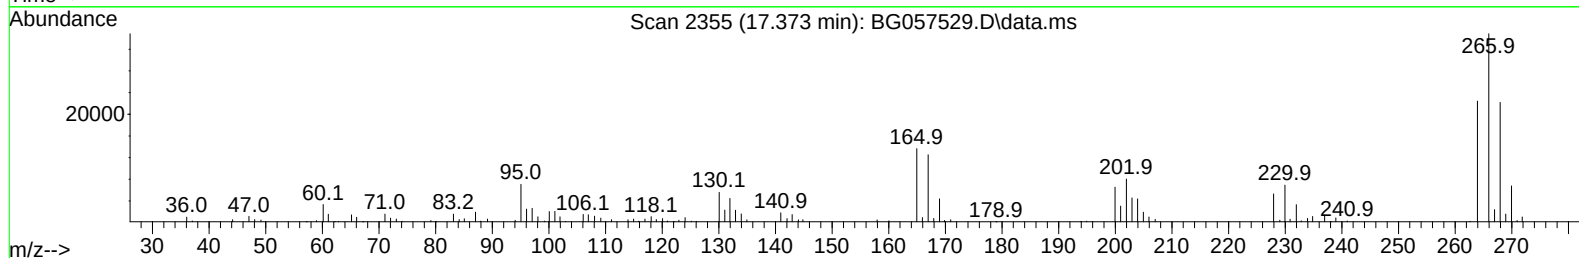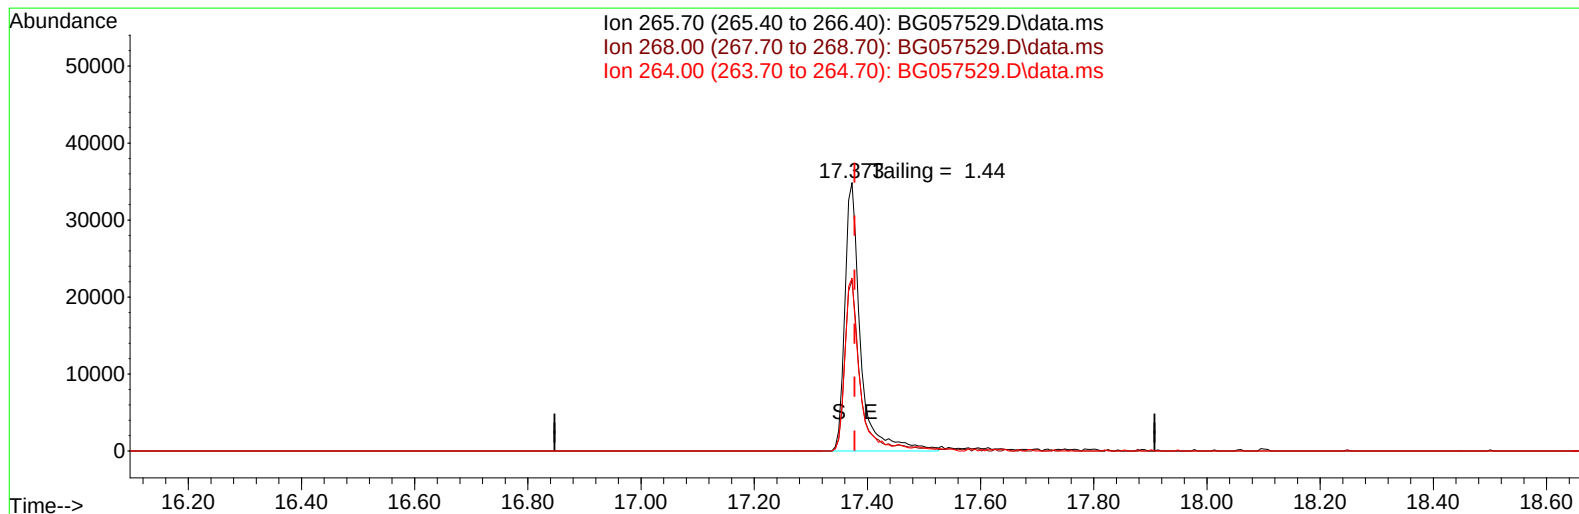

TIC: BG057529.D\data.ms

(70) Pentachlorophenol (C)

17.373min (-0.004) 28619.11 ng




response 67308

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.65
264.00	59.70	64.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
Data File : BG057529.D
Acq On : 24 May 2023 9:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 24 12:36:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 12:22:35 2023
Response via : Initial Calibration

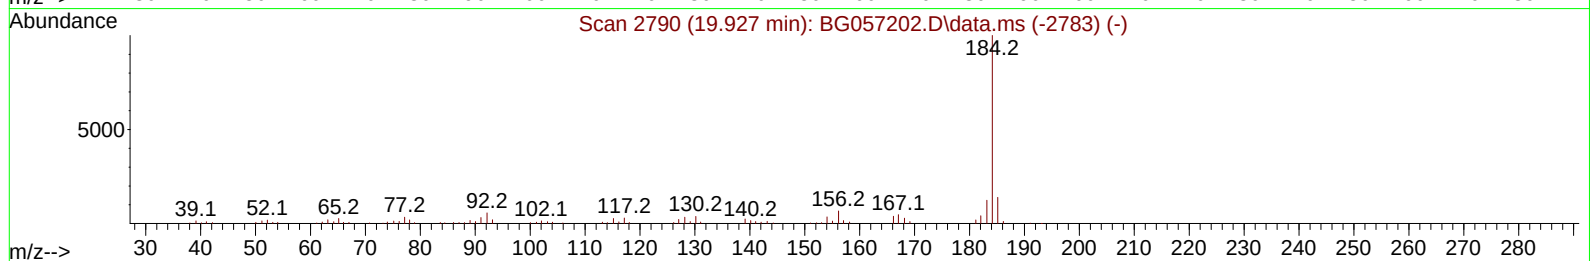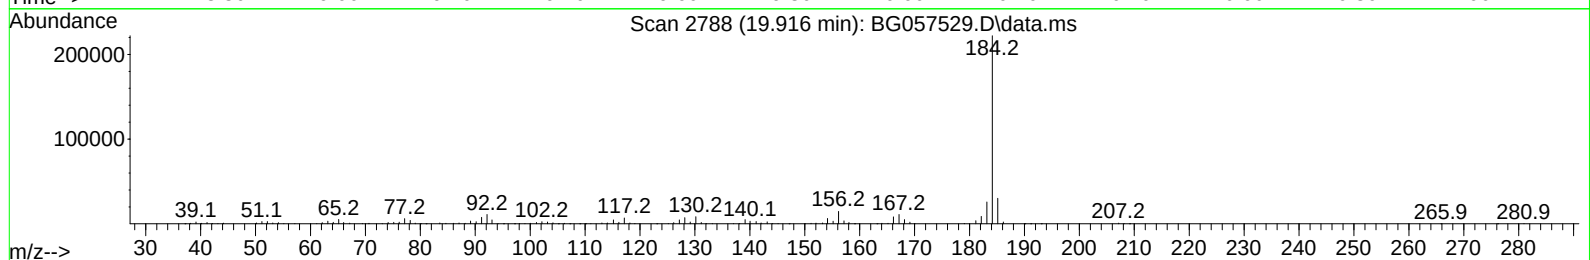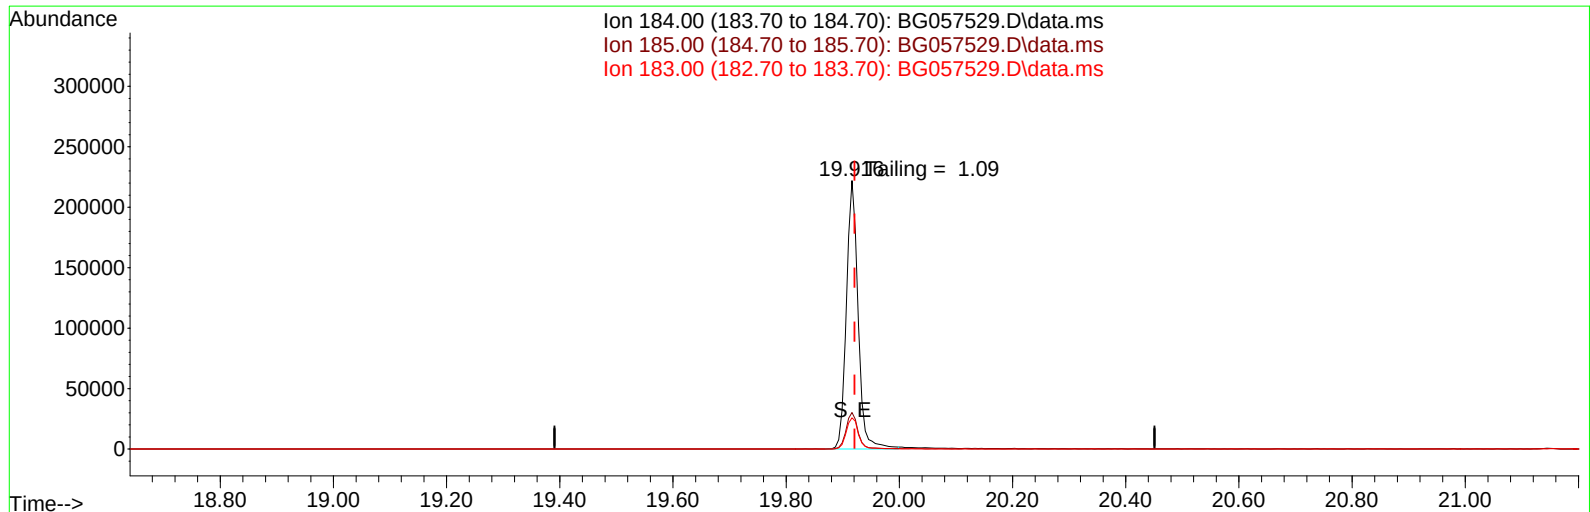

TIC: BG057529.D\data.ms

(77) Benzidine

19.916min (-0.004) 0.00 ng

response 324609

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.60
183.00	12.40	11.66
0.00	0.00	0.00