
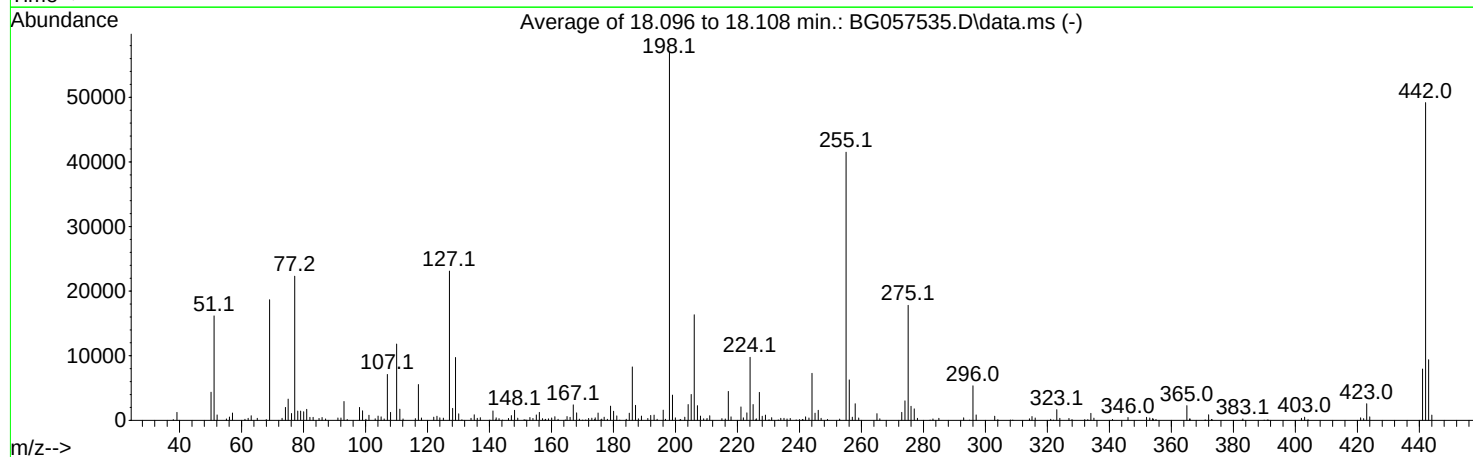


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
Data File : BG057535.D
Acq On : 24 May 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 25 10:58:38 2023

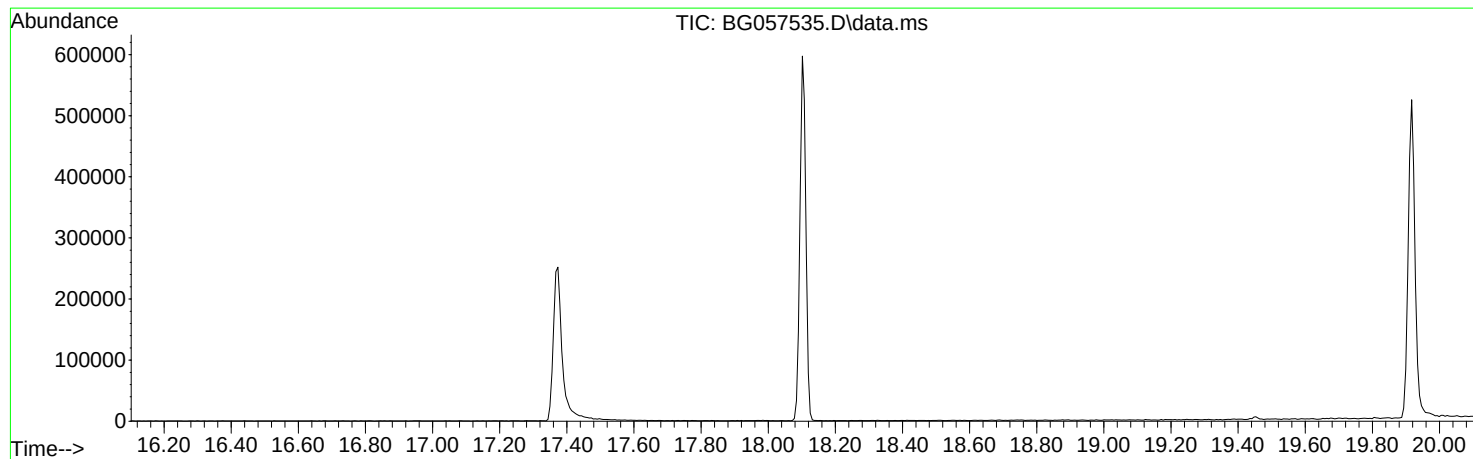

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	16167	PASS
68	69	0.00	2	0.7	129	PASS
69	198	0.00	100	32.8	18677	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.6	23107	PASS
197	198	0.00	2	0.3	172	PASS
198	198	100	100	100.0	56933	PASS
199	198	5	9	6.9	3902	PASS
275	198	10	60	31.3	17815	PASS
365	198	1	100	4.0	2280	PASS
441	198	0.01	100	14.0	7954	PASS
442	442	50	100	100.0	49187	PASS
443	442	15	24	19.1	9378	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/24/2023	BNA_G	<u>BG057535.D</u>
Compound Name	Response	Retention Time
DDT	182150	21.151
DDD	4662	20.692
DDE	650	20.187
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5312	187462	2.83

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
Data File : BG057535.D
Acq On : 24 May 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 24 16:09:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 12:22:35 2023
Response via : Initial Calibration

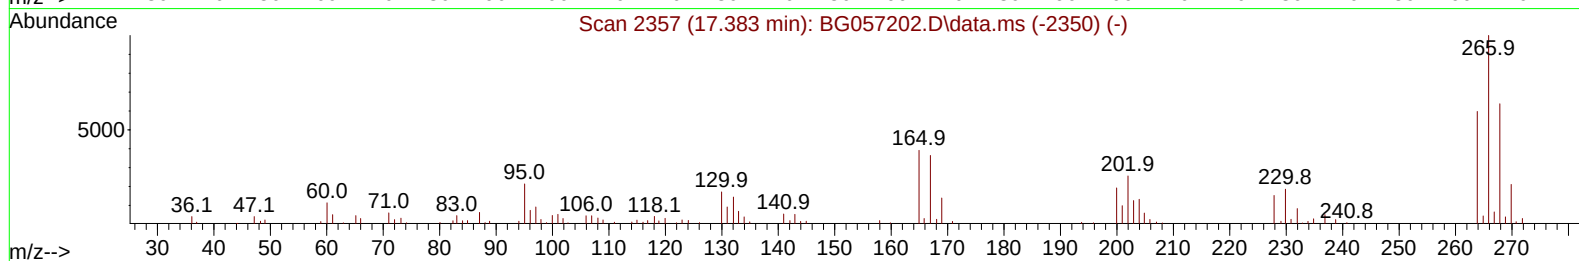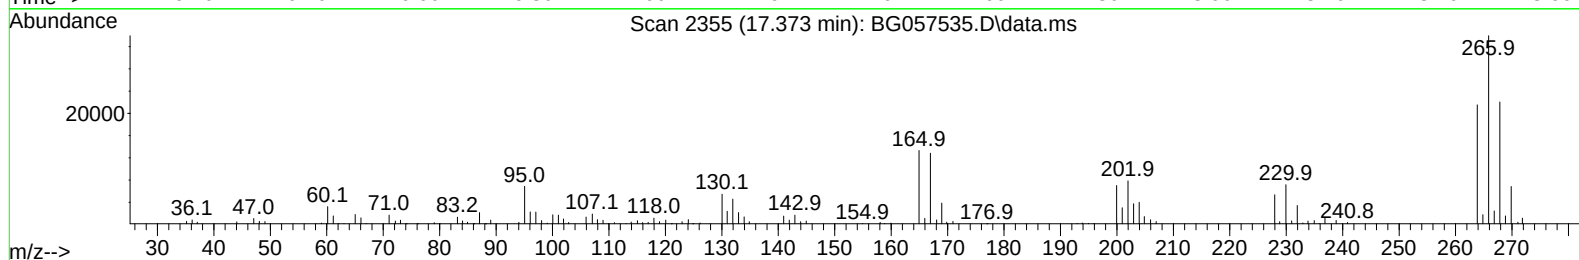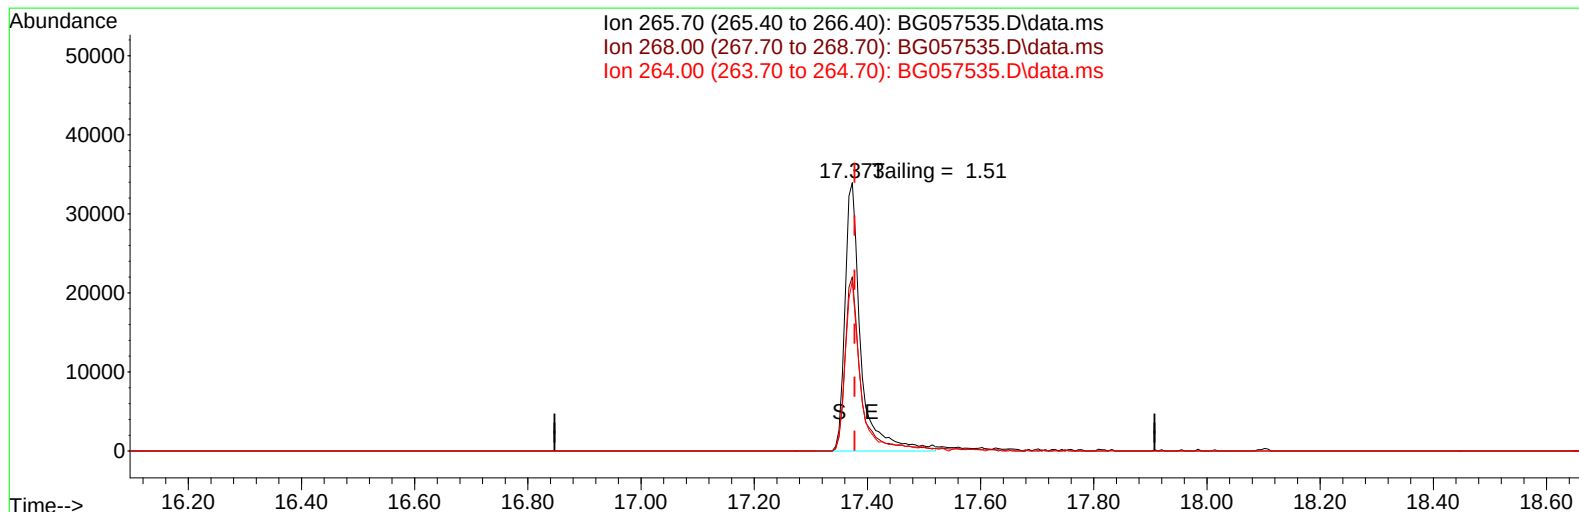

TIC: BG057535.D\data.ms

(70) Pentachlorophenol (C)

17.373min (-0.004) 36634.42 ng




response 65621

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.94
264.00	59.70	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052423\
 Data File : BG057535.D
 Acq On : 24 May 2023 14:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: May 24 16:09:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 12:22:35 2023
 Response via : Initial Calibration

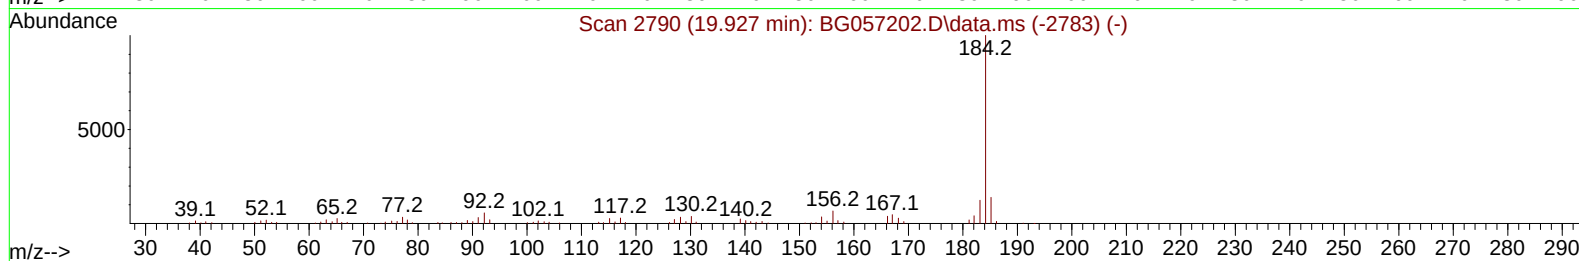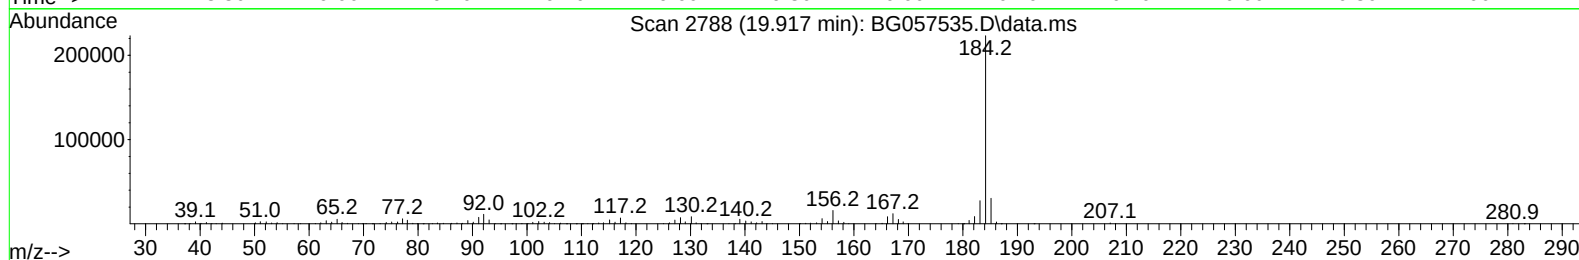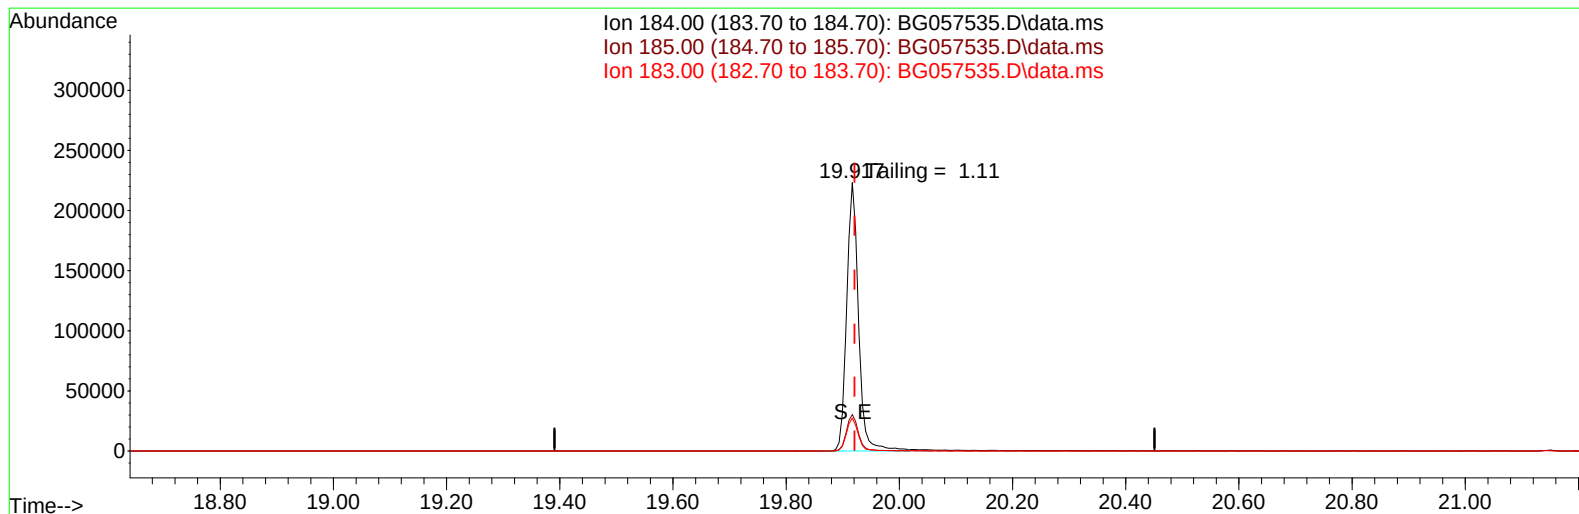

TIC: BG057535.D\data.ms

(77) Benzidine

19.917min (-0.004) 0.00 ng

response 325978

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.61
183.00	12.40	12.30
0.00	0.00	0.00