
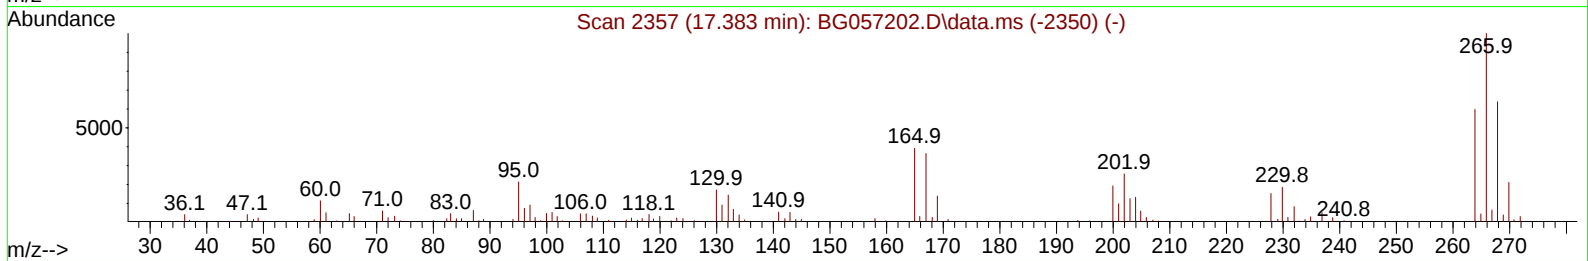
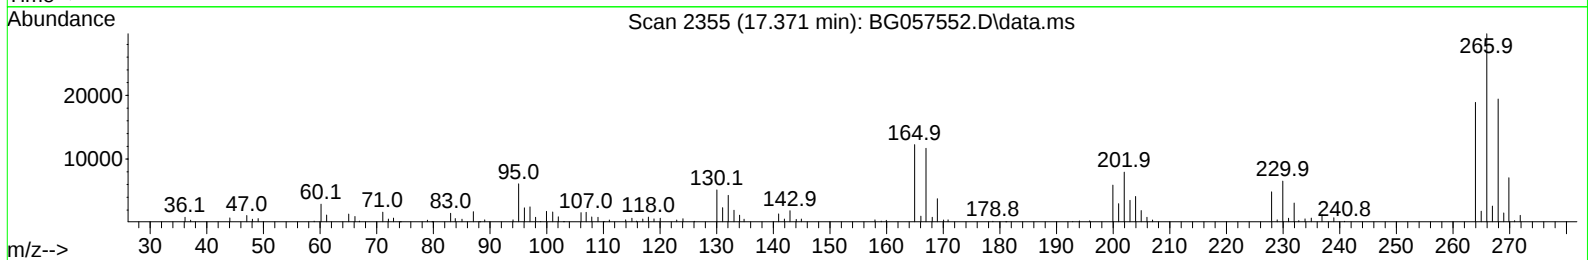


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052523\
Data File : BG057552.D
Acq On : 25 May 2023 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 12:44:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 10:58:38 2023
Response via : Initial Calibration

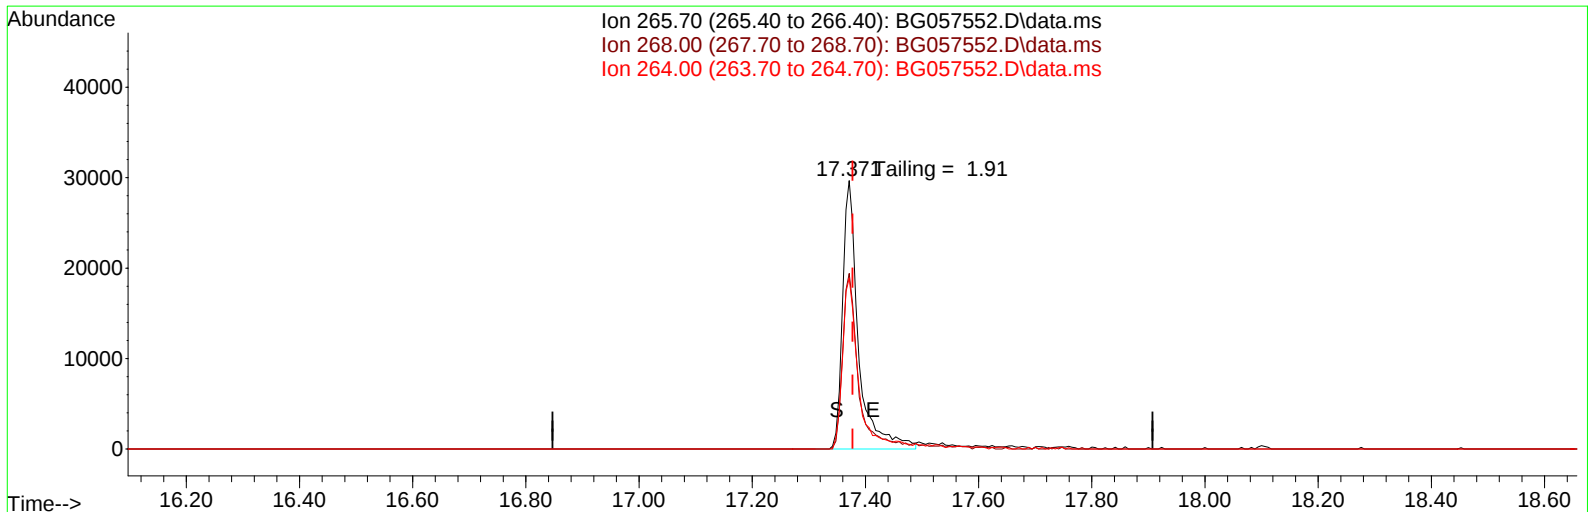

TIC: BG057552.D\data.ms

(70) Pentachlorophenol (C)




17.371min (-0.006) 29518.10 ng

response 58121

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.44
264.00	59.70	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052523\
Data File : BG057552.D
Acq On : 25 May 2023 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 12:44:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 10:58:38 2023
Response via : Initial Calibration

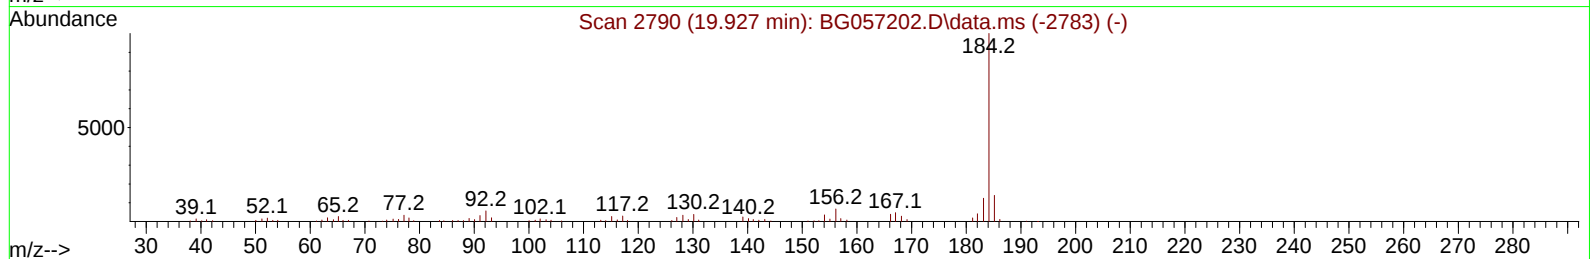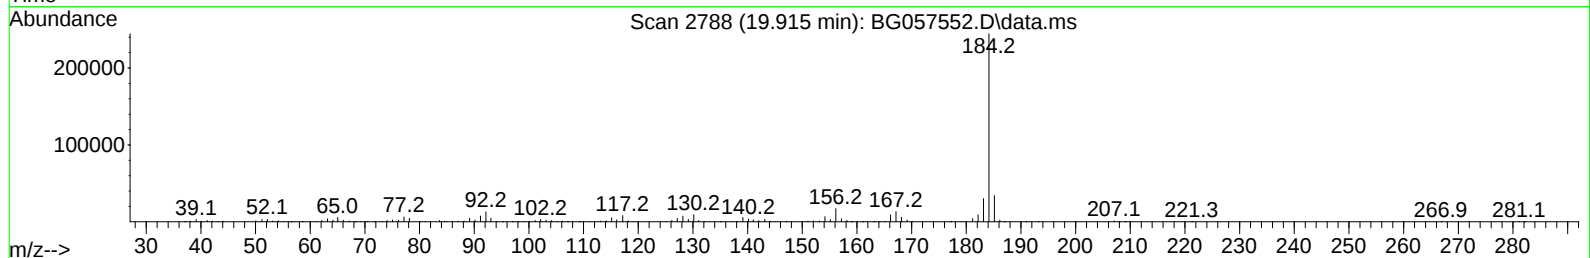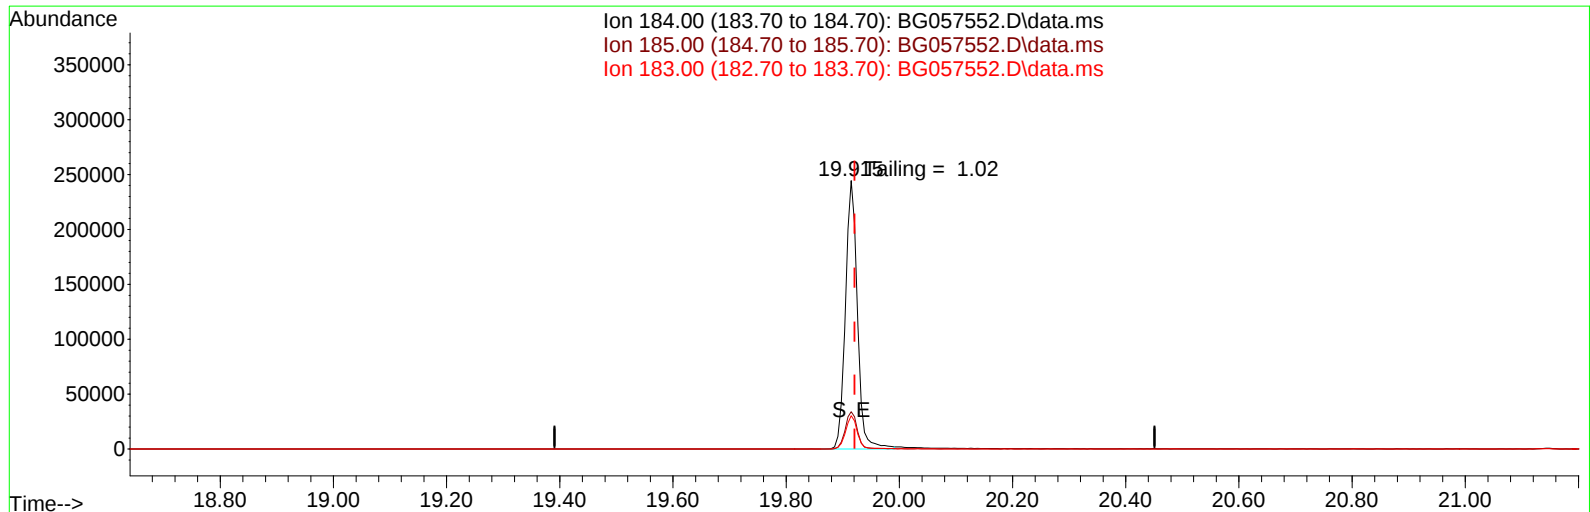

TIC: BG057552.D\data.ms

(77) Benzidine**19.915min (-0.006) 303130.07 ng****response 365953**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.91
183.00	12.40	12.44
0.00	0.00	0.00