
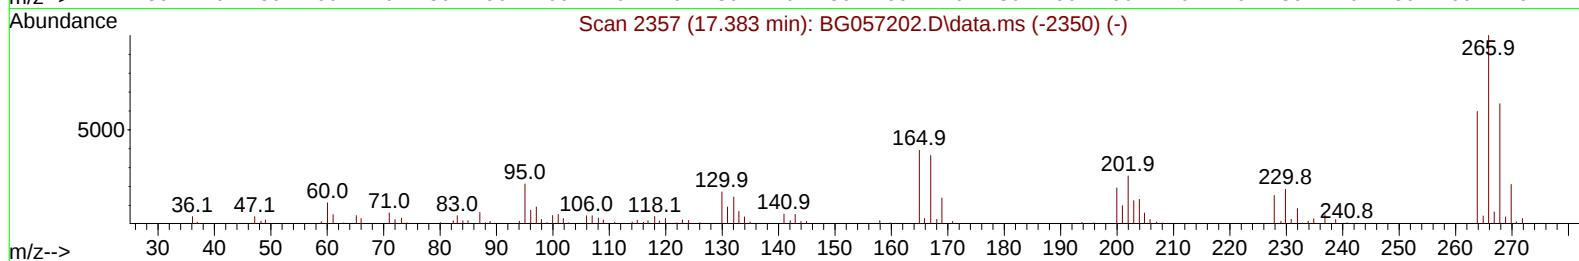
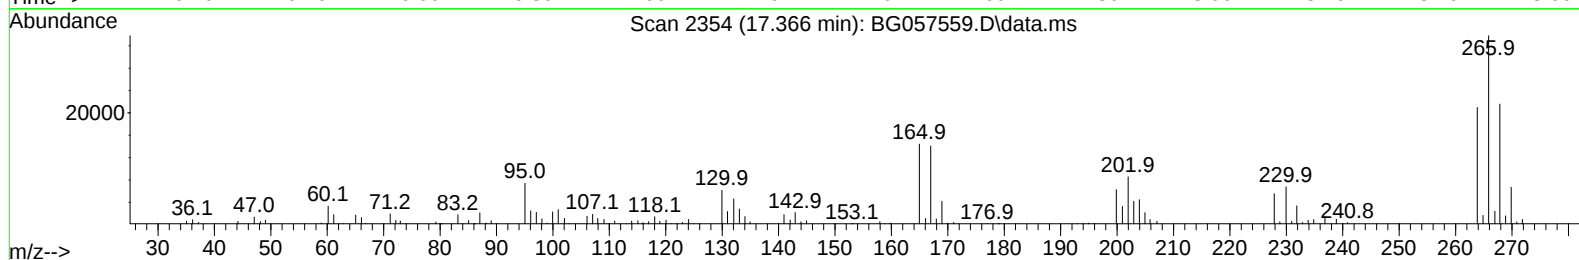


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052523\
Data File : BG057559.D
Acq On : 25 May 2023 15:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 16:56:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 10:58:38 2023
Response via : Initial Calibration

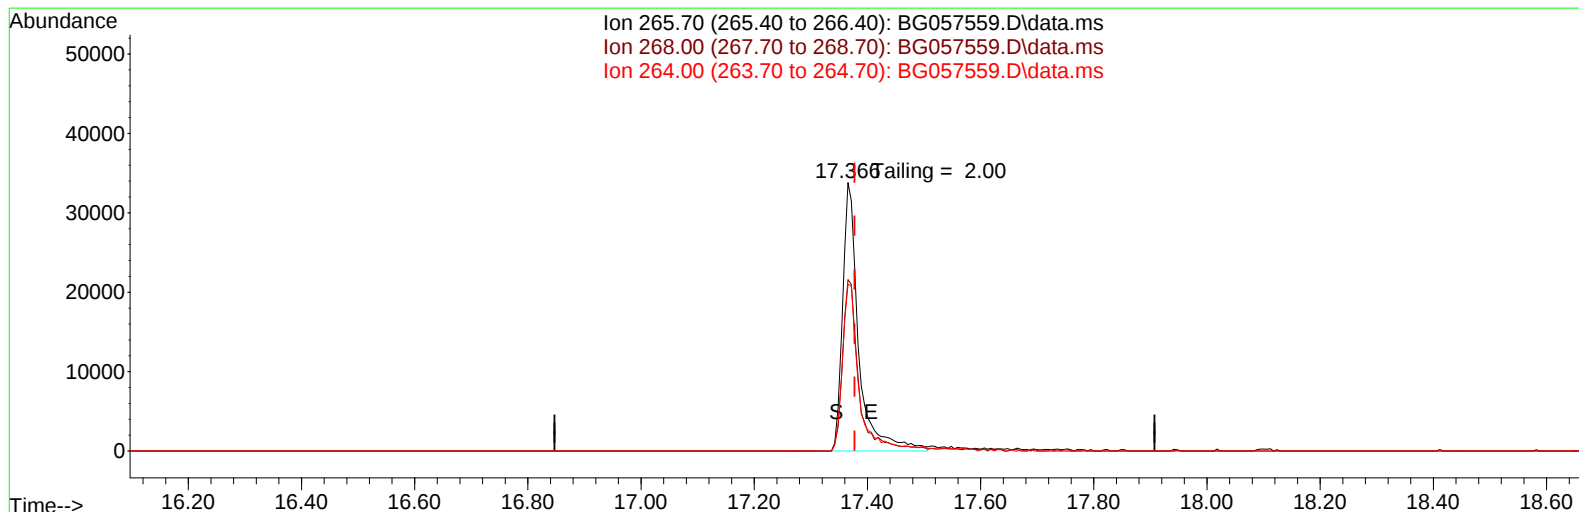

TIC: BG057559.D\data.ms

(70) Pentachlorophenol (C)




17.366min (-0.011) 30289.11 ng

response **67094**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.84
264.00	59.70	62.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052523\
Data File : BG057559.D
Acq On : 25 May 2023 15:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 16:56:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 10:58:38 2023
Response via : Initial Calibration

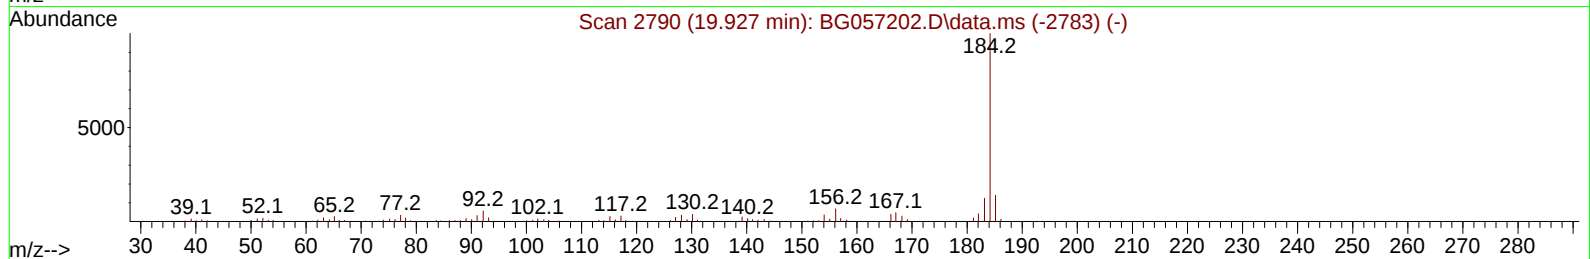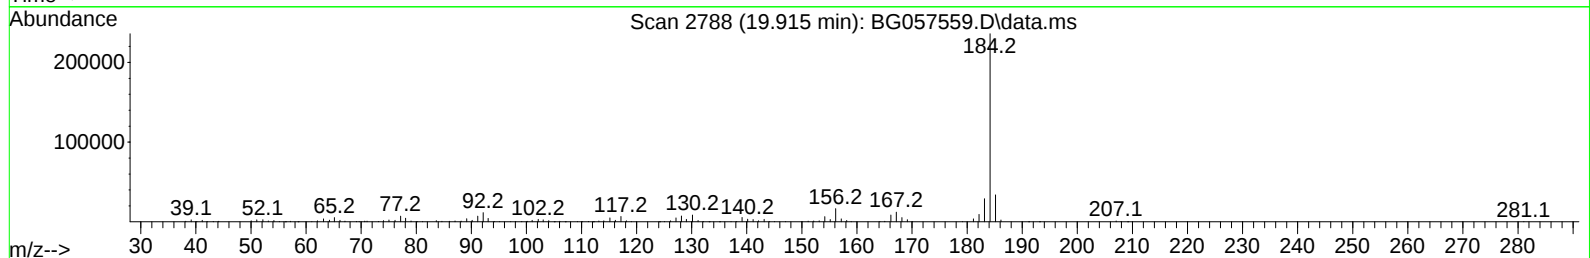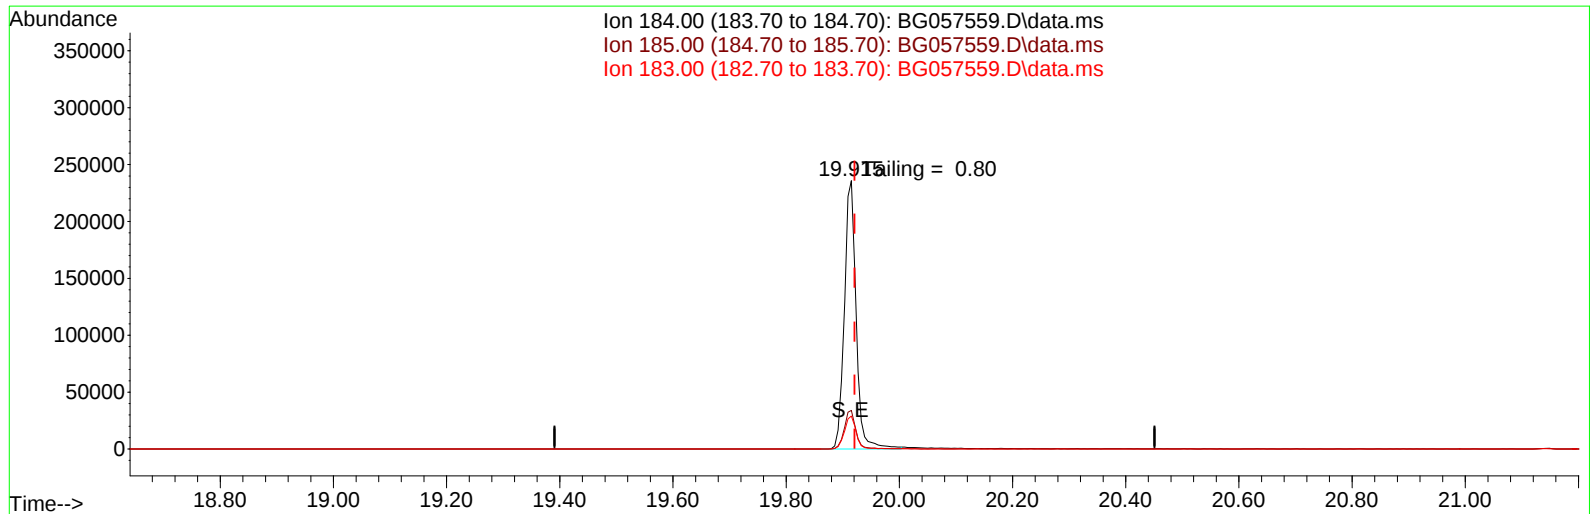

TIC: BG057559.D\data.ms

(77) Benzidine

19.915min (-0.005) 0.00 ng

response 343679

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.38
183.00	12.40	12.32
0.00	0.00	0.00