
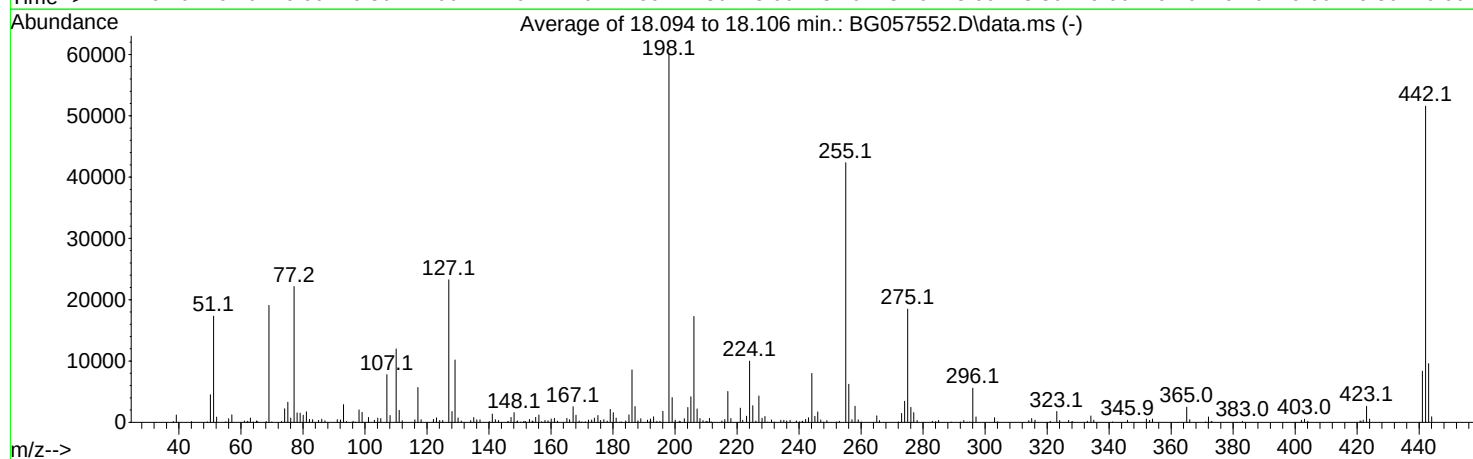


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052523\
Data File : BG057552.D
Acq On : 25 May 2023 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 26 02:58:05 2023

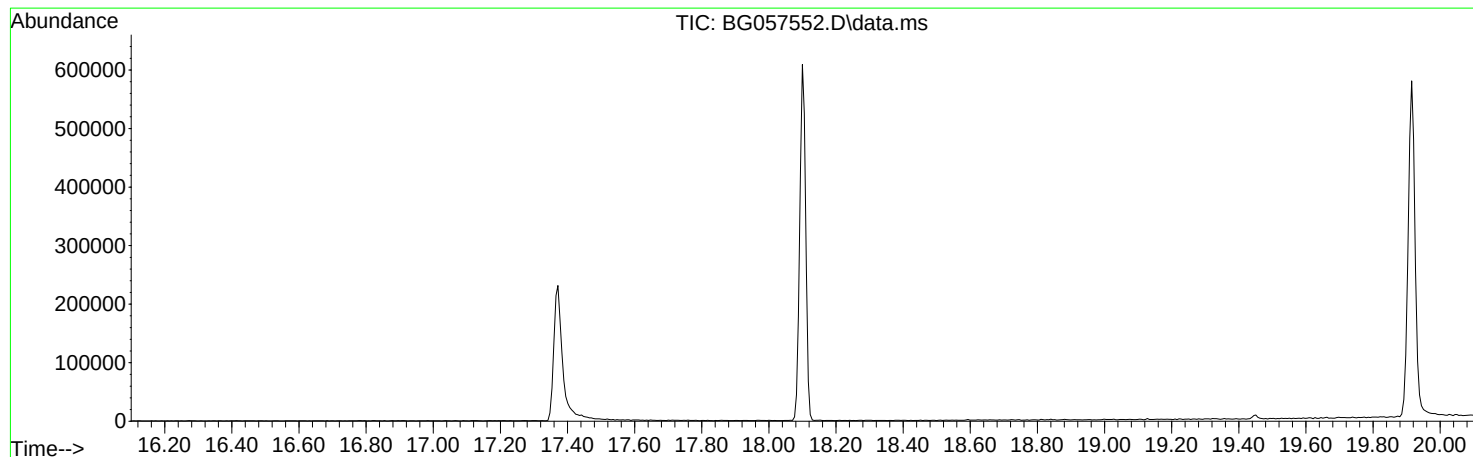

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	17327	PASS
68	69	0.00	2	0.7	129	PASS
69	198	0.00	100	31.8	19085	PASS
70	69	0.00	2	0.4	69	PASS
127	198	10	80	38.8	23261	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59997	PASS
199	198	5	9	6.7	4046	PASS
275	198	10	60	30.8	18473	PASS
365	198	1	100	4.2	2493	PASS
441	198	0.01	100	13.9	8348	PASS
442	442	50	100	100.0	51579	PASS
443	442	15	24	18.6	9581	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/25/2023	BNA_G	<u>BG057552.D</u>
Compound Name	Response	Retention Time
DDT	171882	21.143
DDD	5680	20.69
DDE	552	20.191
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6232	178114	3.50

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052523\
Data File : BG057552.D
Acq On : 25 May 2023 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 25 12:44:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 10:58:38 2023
Response via : Initial Calibration

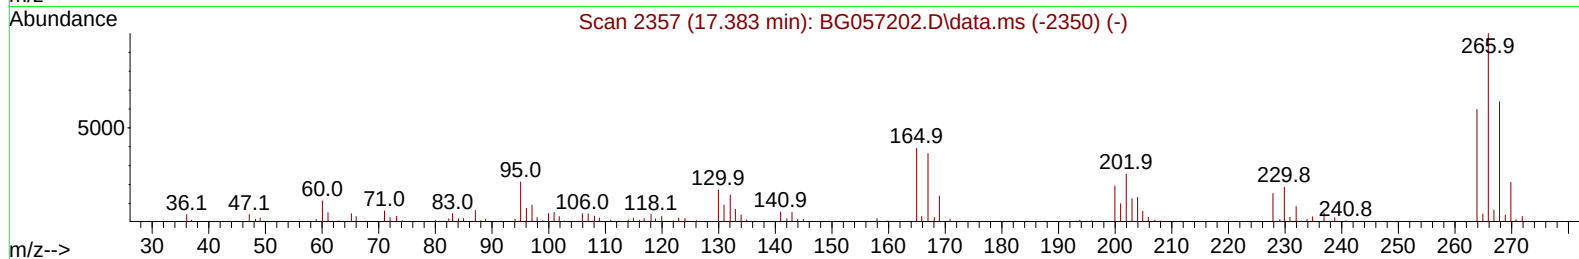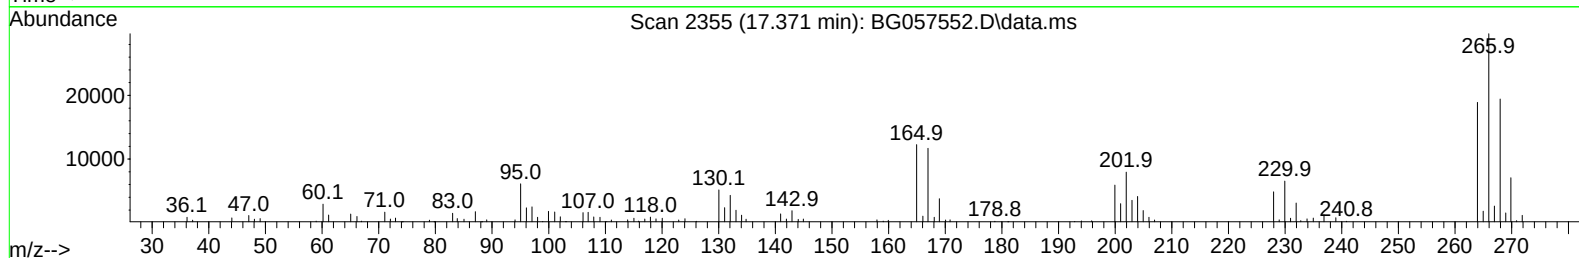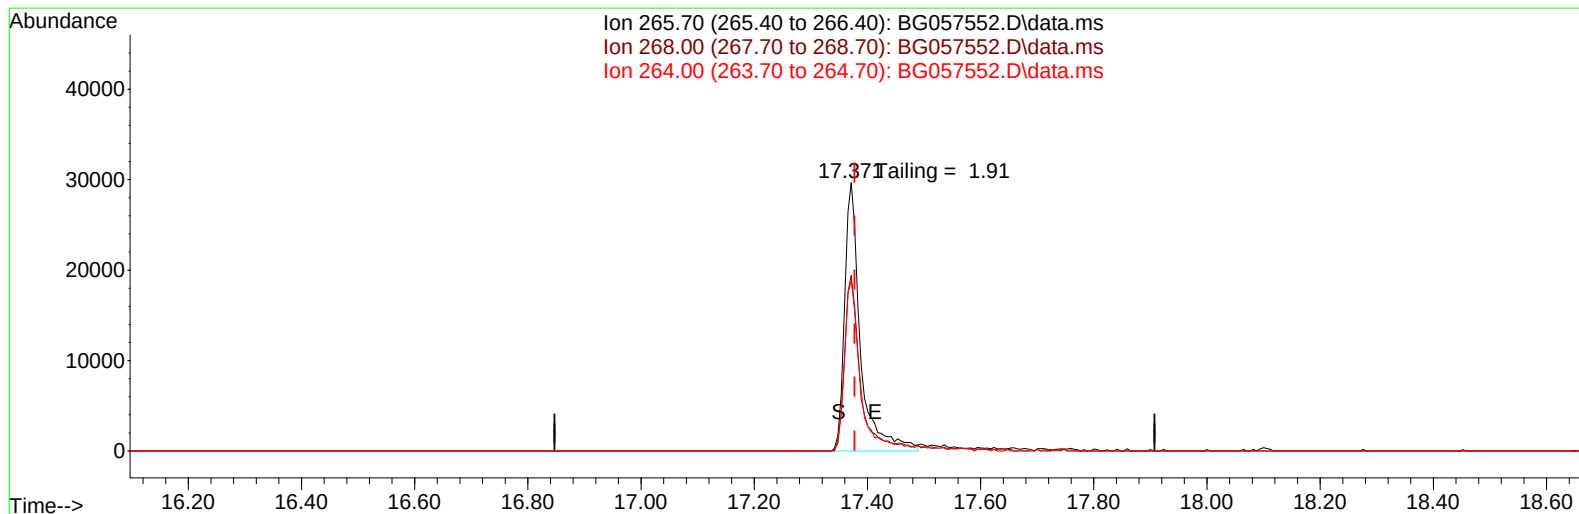

TIC: BG057552.D\data.ms

(70) Pentachlorophenol (C)

17.371min (-0.006) 29518.10 ng




response 58121

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.44
264.00	59.70	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052523\
Data File : BG057552.D
Acq On : 25 May 2023 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 25 12:44:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 10:58:38 2023
Response via : Initial Calibration

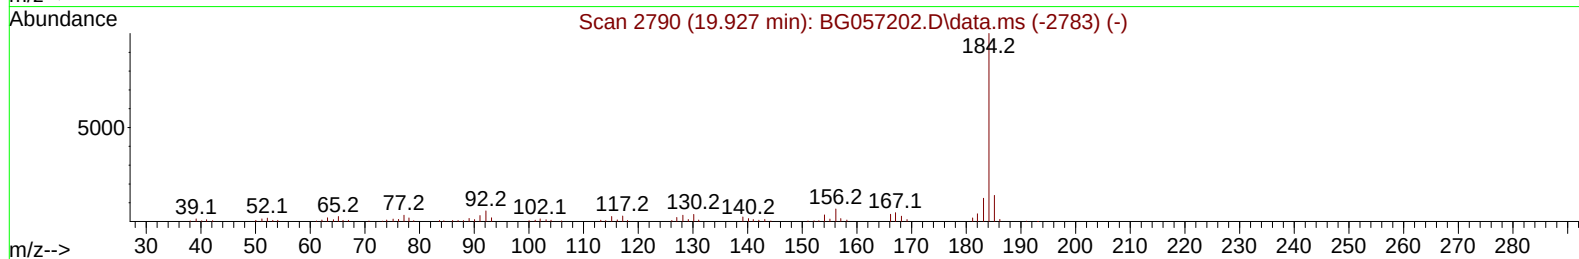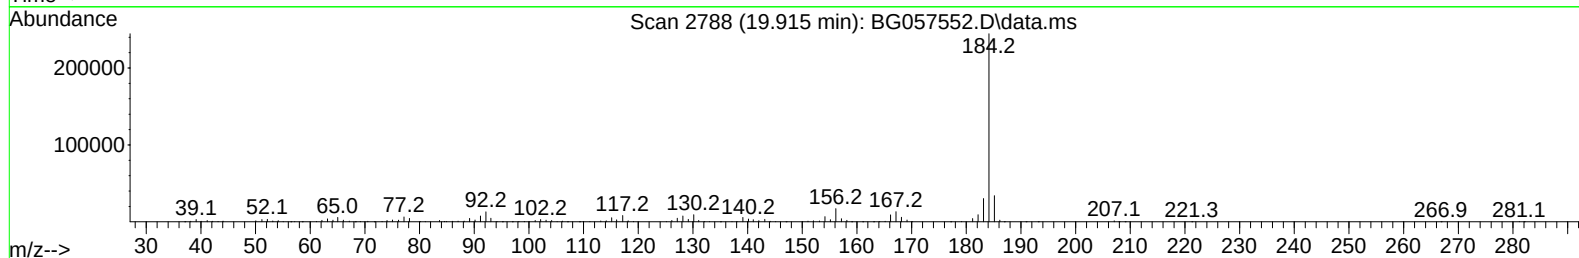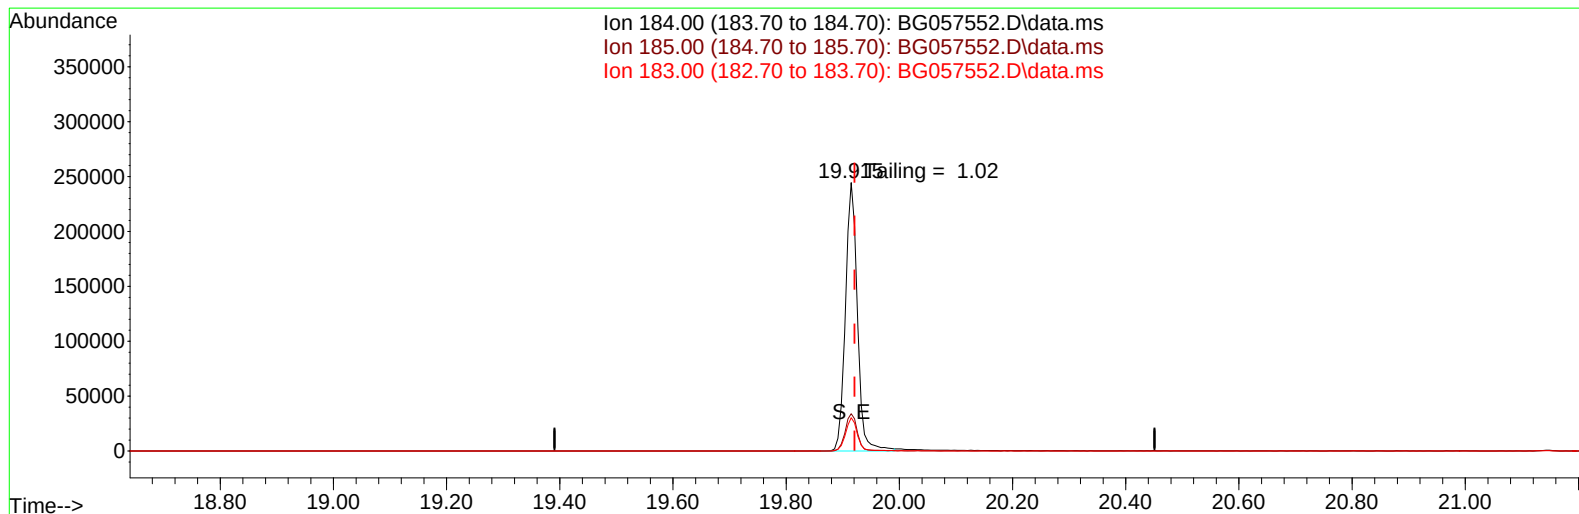

TIC: BG057552.D\data.ms

(77) Benzidine

19.915min (-0.006) 303130.07 ng

response 365953

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.91
183.00	12.40	12.44
0.00	0.00	0.00