
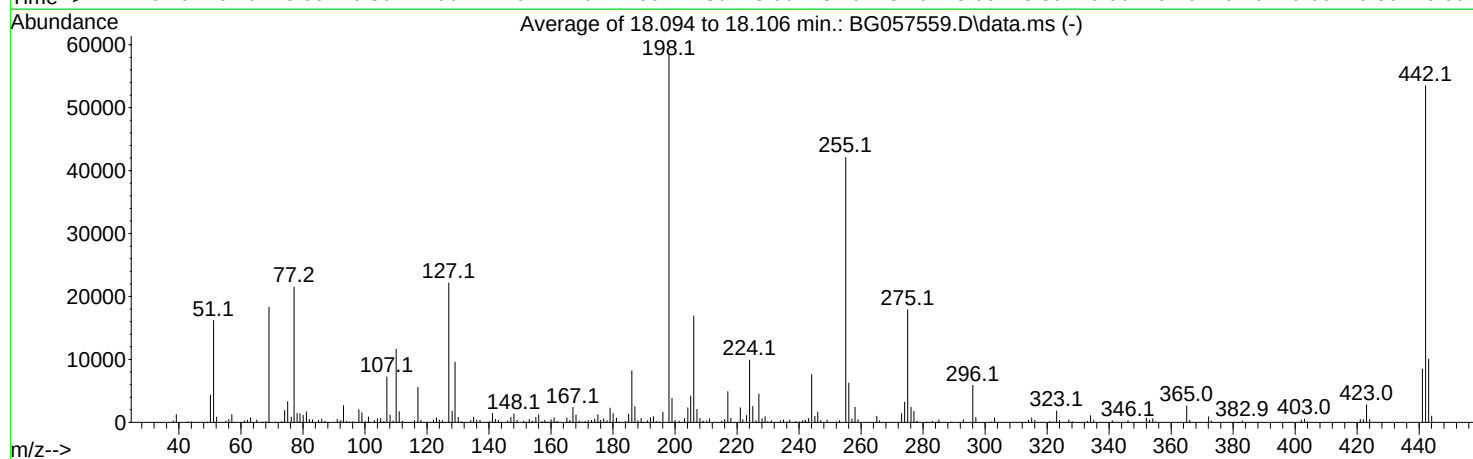


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052523\
 Data File : BG057559.D
 Acq On : 25 May 2023 15:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 26 02:58:05 2023

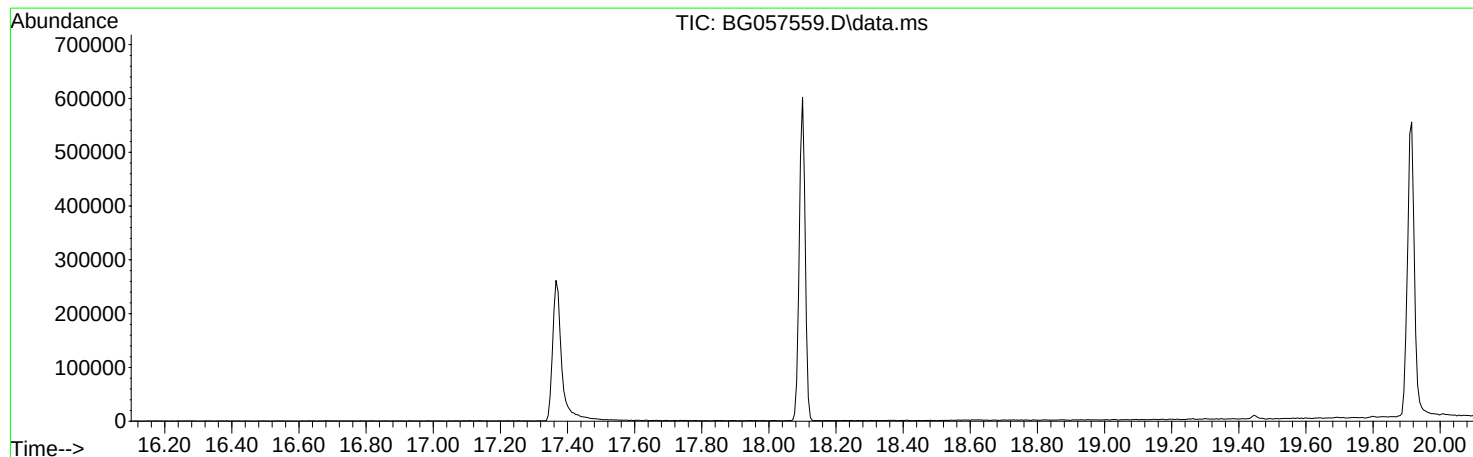

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	16192	PASS
68	69	0.00	2	0.9	163	PASS
69	198	0.00	100	31.3	18317	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.9	22144	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58453	PASS
199	198	5	9	6.5	3803	PASS
275	198	10	60	30.6	17876	PASS
365	198	1	100	4.5	2607	PASS
441	198	0.01	100	14.5	8479	PASS
442	442	50	100	100.0	53488	PASS
443	442	15	24	18.8	10032	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/25/2023	BNA_G	<u>BG057559.D</u>
Compound Name	Response	Retention Time
DDT	189114	21.143
DDD	5291	20.685
DDE	481	20.18
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5772	194886	2.96

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052523\
Data File : BG057559.D
Acq On : 25 May 2023 15:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 25 16:56:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 10:58:38 2023
Response via : Initial Calibration

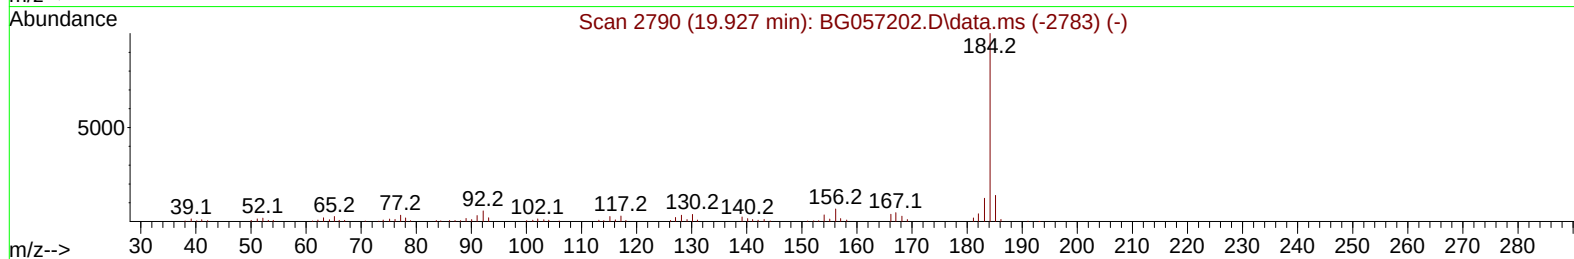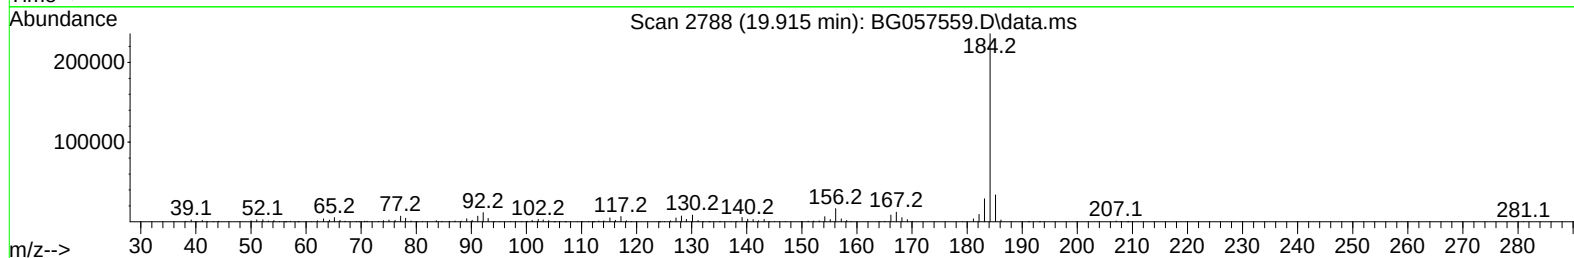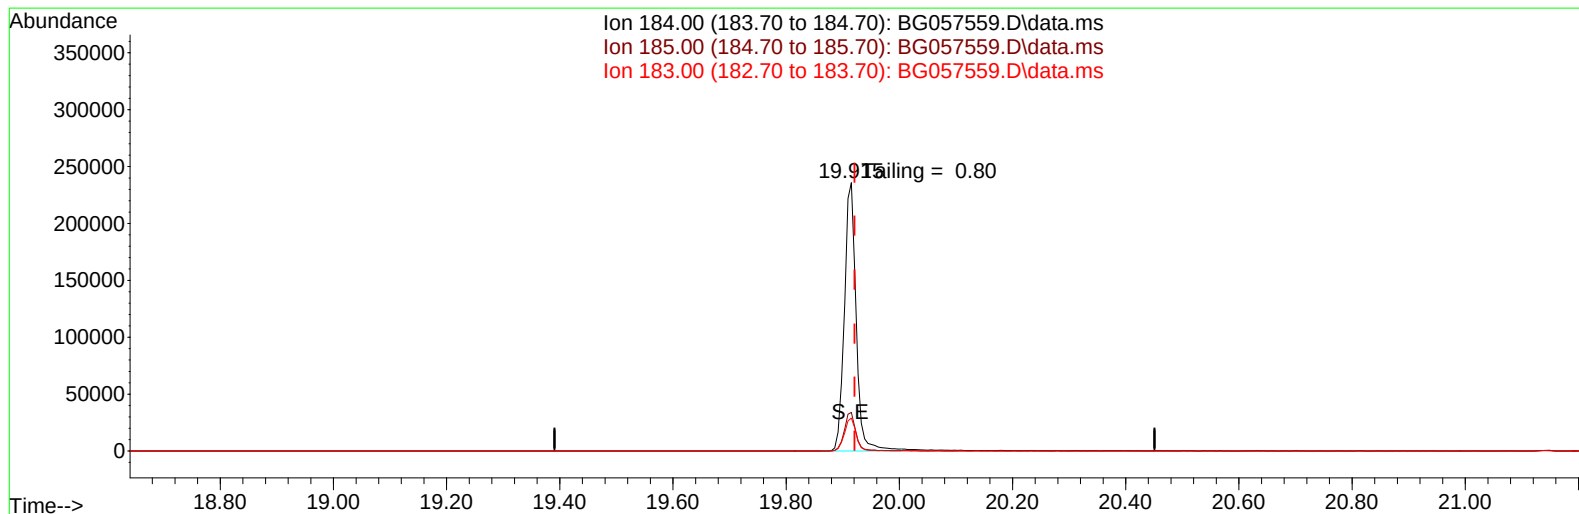

TIC: BG057559.D\data.ms

(77) Benzidine

19.915min (-0.005) 0.00 ng

response 343679

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.38
183.00	12.40	12.32
0.00	0.00	0.00