


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052615\
 Data File : BG017276.D
 Acq On : 26 May 2015 13:16
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 16:12:13 2015

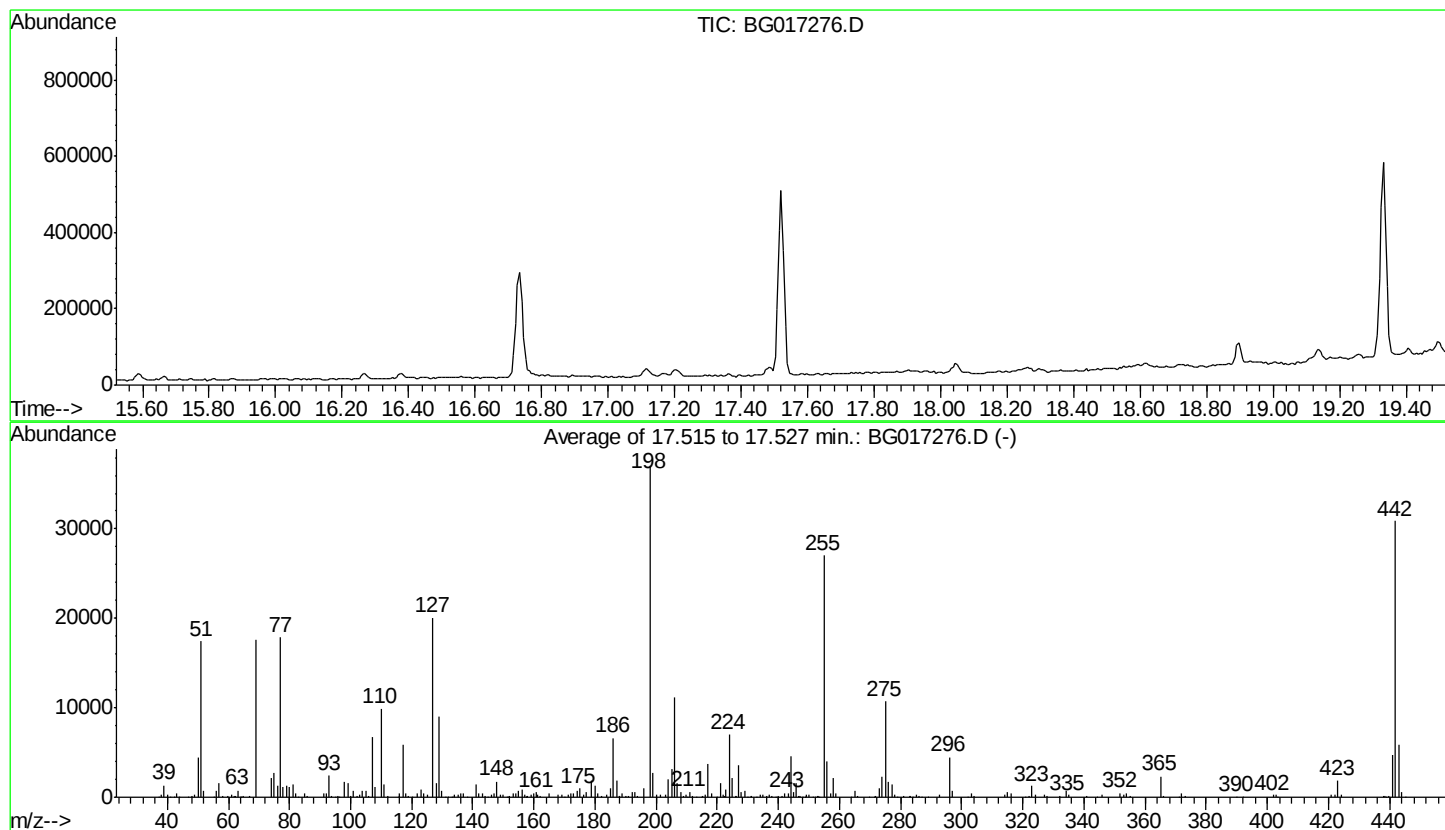

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	17424	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.3	17544	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.1	20043	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	37082	PASS
199	198	5	9	7.4	2748	PASS
275	198	10	60	28.9	10720	PASS
365	198	1	100	6.3	2328	PASS
441	442	0.01	24	15.3	4721	PASS
442	198	50	100	83.3	30890	PASS
443	442	15	24	18.8	5812	PASS