

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
 Data File : BG022073.D
 Acq On : 26 May 2016 9:40
 Operator : UM/SJ
 Sample : H3201-10 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZG9

Manual Integrations
 APPROVED

sohil
 5/27/2016 7:40:22 PM

Quant Time: May 27 04:56:23 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 27 04:32:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	30852	20.00	ng/ul	0.00
18) Naphthalene-d8	10.97	136	165647	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	97883	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.52	188	189455	20.00	ng/ul	0.00
75) Chrysene-d12	21.80	240	147200	20.00	ng/ul	0.00
83) Perylene-d12	25.13	264	147386	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.32	99	6130	2.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	2791	1.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	5841	2.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	4722	2.00	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	2348m	1.92	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	3105m	2.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	4918	2.11	ng/ul	0.00
29) 4-Chloroaniline-d4	11.13	131	3915m	1.54	ng/ul	0.02
43) Dimethylphthalate-d6	14.18	166	21004	2.86	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	29727	2.90	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
57) Fluorene-d10	15.77	176	20036	2.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	849	0.86	ng/ul	0.00
70) Anthracene-d10	17.62	188	32067	3.53	ng/ul	0.00
76) Pyrene-d10	19.90	212	28789	3.47	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.89	264	23243	3.40	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.22	163	9292	1.26	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
Data File : BG022073.D
Acq On : 26 May 2016 9:40
Operator : UM/SJ
Sample : H3201-10 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BCZG9

Manual Integrations
APPROVED

sohil
5/27/2016 7:40:22 PM

Quant Time: May 27 04:56:23 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 27 04:32:27 2016
Response via : Initial Calibration

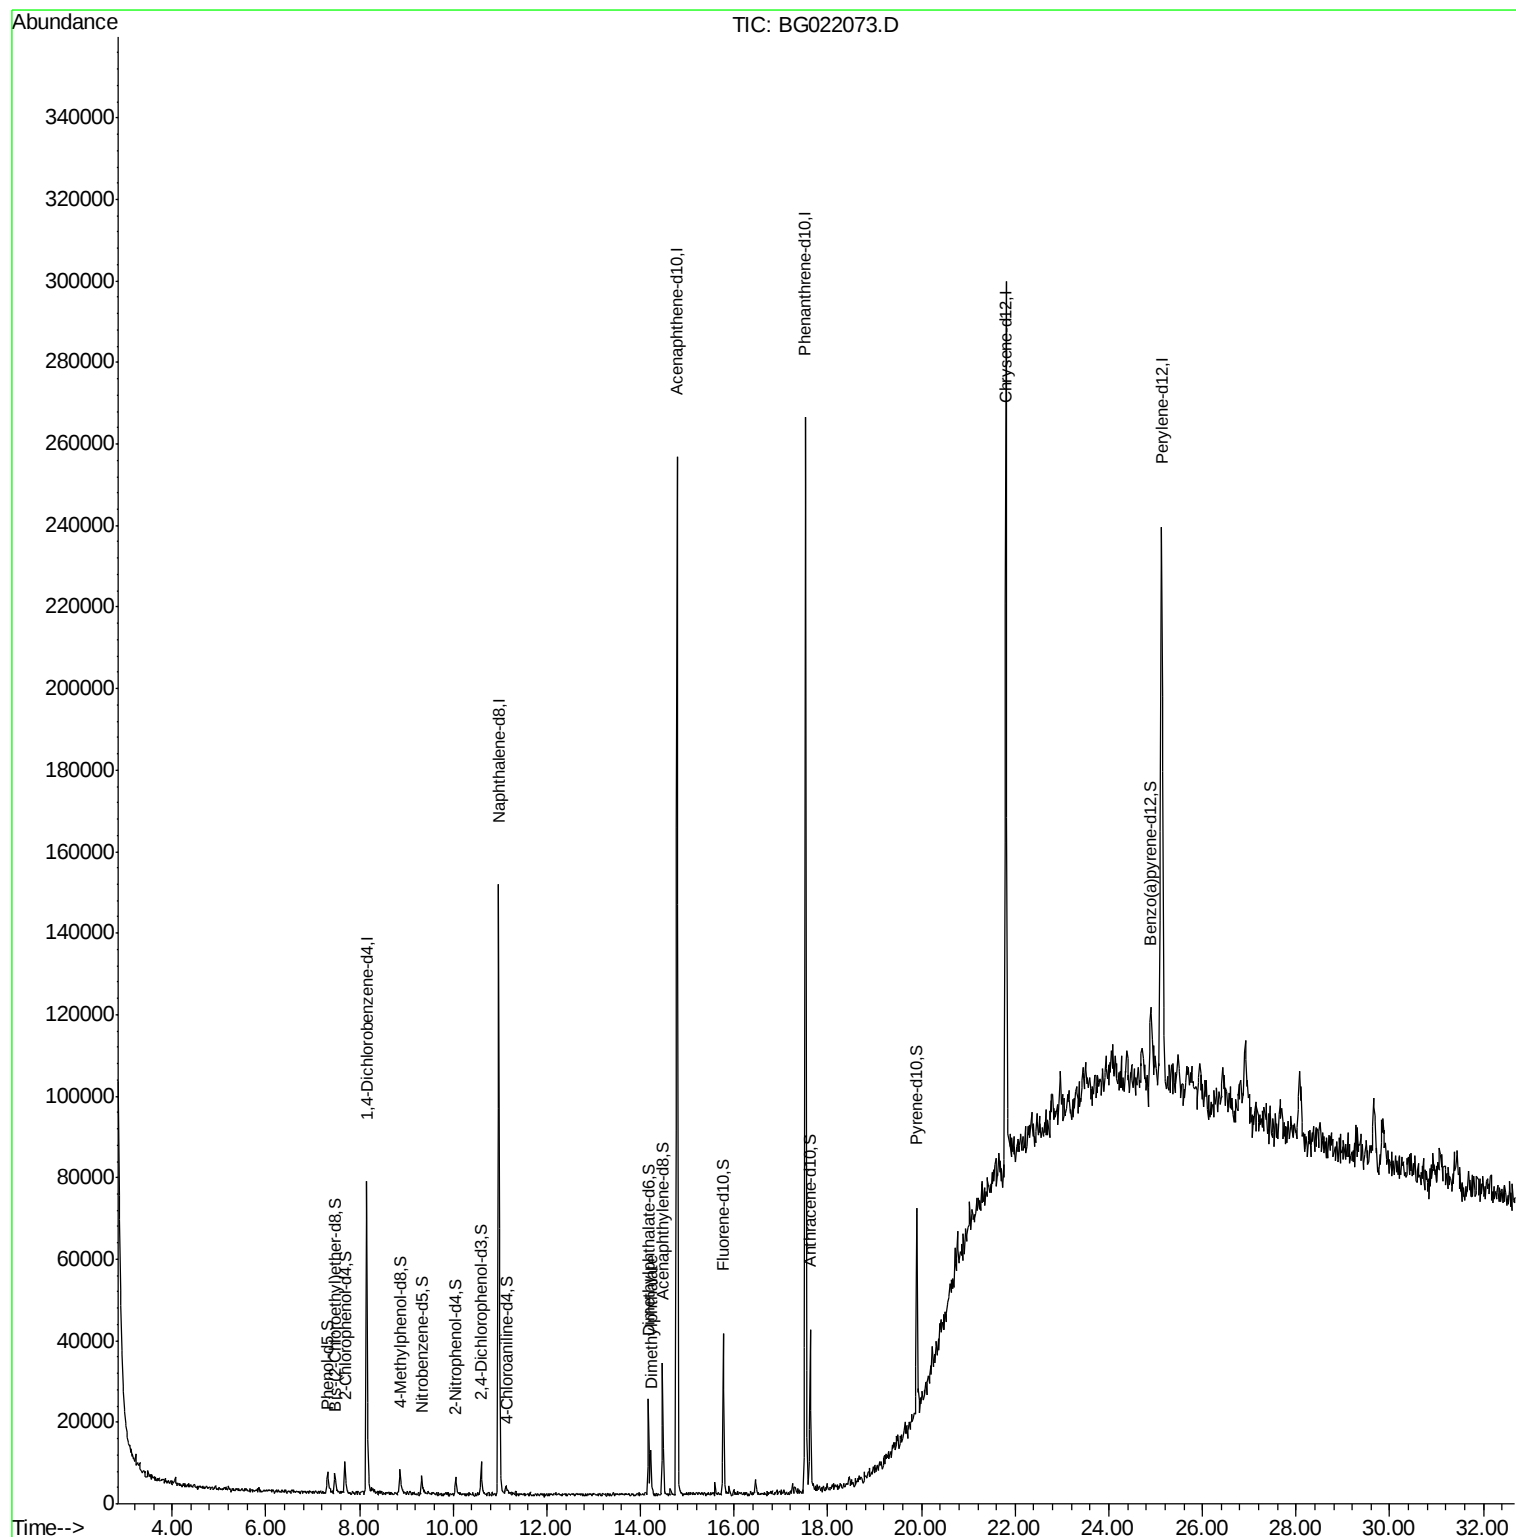

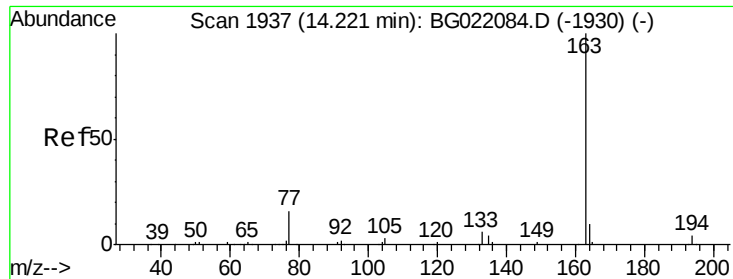

#44

Dimethylphthalate

Concen: 1.26 ng/ul

RT: 14.22 min Scan# 1937

Delta R.T. 0.00 min

Lab File: BG022073.D

Acq: 26 May 2016 9:40

Instrument :

BNA_G

ClientSampleId :

BCZG9

Tot Ion:	163	Resp:	9292
Ion Ratio	Lower	Upper	
163	100		
194	5.1	3.4	5.2
164	9.9	8.8	13.2

Manual Integrations
APPROVED

sohil
5/27/2016 7:40:22 PM

