

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
 Data File : BG022097.D
 Acq On : 27 May 2016 1:52
 Operator : UM/SJ
 Sample : H3201-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZG9

Quant Time: May 27 05:52:53 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 27 05:50:42 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	72572	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	341647	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	178034	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.53	188	315454	20.00	ng/ul	0.00
75) Chrysene-d12	21.81	240	290683	20.00	ng/ul	0.00
83) Perylene-d12	25.16	264	280828	20.00	ng/ul	0.04

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	1312	0.94	ng/uL	0.00
5) Phenol-d5	7.32	99	69236	10.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	34333	9.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	64919	11.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	51940	9.34	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	30318	12.03	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	33821	12.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.61	165	56774	11.79	ng/ul	0.02
29) 4-Chloroaniline-d4	11.11	131	31246	5.96	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	169883	12.70	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	228231	12.22	ng/ul	0.00
51) 4-Nitrophenol-d4	15.01	143	18145	7.88	ng/ul	0.02
57) Fluorene-d10	15.77	176	152975	12.22	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	8004	4.85	ng/ul	0.00
70) Anthracene-d10	17.63	188	200850	13.27	ng/ul	0.00
76) Pyrene-d10	19.90	212	184787	11.27	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.94	264	162268	12.45	ng/ul	0.04


Target Compounds					Ovalue
44) Dimethylphthalate	14.22	163	72823	5.42	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
Data File : BG022097.D
Acq On : 27 May 2016 1:52
Operator : UM/SJ
Sample : H3201-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCZG9

Quant Time: May 27 05:52:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 27 05:50:42 2016
Response via : Initial Calibration

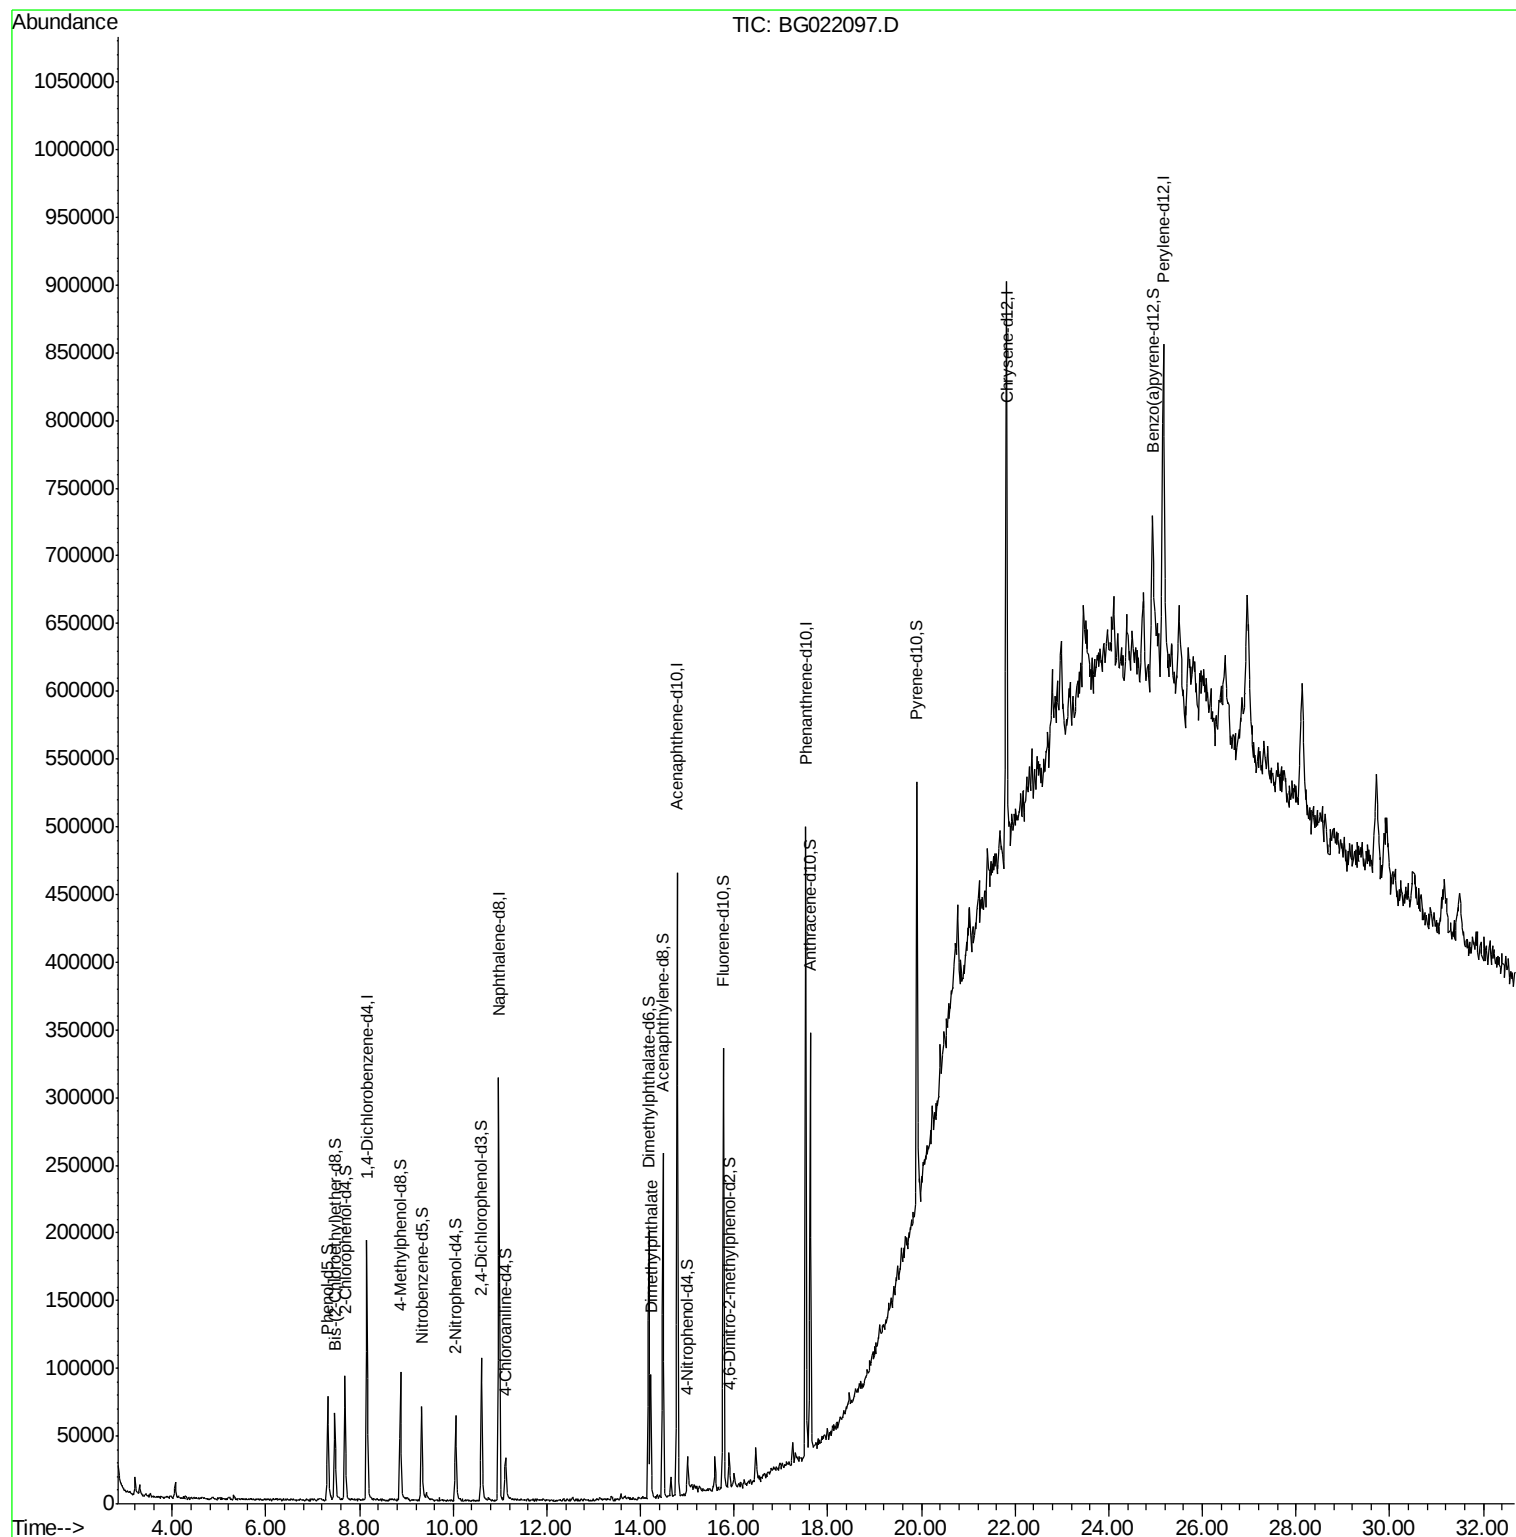

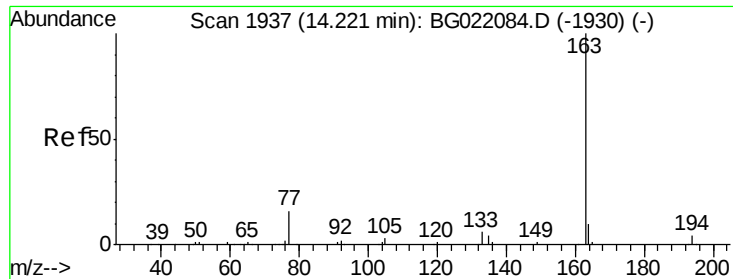

#44

Dimethylphthalate

Concen: 5.42 ng/ul

RT: 14.22 min Scan# 1938

Delta R.T. 0.00 min

Lab File: BG022097.D

Acq: 27 May 2016 1:52

Instrument :

BNA_G

ClientSampleId :

BCZG9

Tot Ion:163 Resp: 72823

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2

164 10.9 8.8 13.2

