

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
 Data File : BG022073.D
 Acq On : 26 May 2016 9:40
 Operator : UM/SJ
 Sample : H3201-10 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZG9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.203	400	402	405	rBV3	898	714	0.16%	0.031%
2	5.726	489	491	495	rBV3	529	819	0.18%	0.036%
3	6.126	558	559	565	rBV4	684	1161	0.25%	0.051%
4	6.202	569	572	573	rBV3	579	642	0.14%	0.028%
5	6.748	663	665	667	rBV	542	591	0.13%	0.026%
6	7.013	708	710	713	rBV3	637	733	0.16%	0.032%
7	7.125	726	729	732	rBV4	608	701	0.15%	0.031%
8	7.324	756	763	770	rBV2	5288	12110	2.63%	0.534%
9	7.471	782	788	795	rBV3	4999	10770	2.34%	0.475%
10	7.689	820	825	836	rVB3	7665	15970	3.47%	0.704%
11	7.806	843	845	848	rVB4	541	610	0.13%	0.027%
12	7.918	861	864	865	rBV	521	602	0.13%	0.027%
13	7.935	865	867	870	rVB2	719	653	0.14%	0.029%
14	7.971	870	873	875	rBV2	697	921	0.20%	0.041%
15	8.153	894	904	917	rBV	76843	161667	35.17%	7.124%
16	8.276	924	925	929	rVB3	869	817	0.18%	0.036%
17	8.382	942	943	946	rVB	1119	747	0.16%	0.033%
18	8.405	946	947	949	rBV2	935	958	0.21%	0.042%
19	8.664	987	991	992	rBV2	643	631	0.14%	0.028%
20	8.870	1019	1026	1034	rBV3	6221	15230	3.31%	0.671%
21	9.016	1049	1051	1053	rBV	778	623	0.14%	0.027%
22	9.257	1088	1092	1093	rVB2	915	1143	0.25%	0.050%
23	9.281	1093	1096	1097	rBV	742	912	0.20%	0.040%
24	9.328	1099	1104	1108	rBV4	4578	9159	1.99%	0.404%
25	9.839	1189	1191	1195	rBV3	582	862	0.19%	0.038%
26	10.045	1222	1226	1228	rBV3	3933	4967	1.08%	0.219%
27	10.521	1302	1307	1308	rBV2	883	1118	0.24%	0.049%
28	10.603	1315	1321	1327	rBV3	8127	15258	3.32%	0.672%
29	10.785	1349	1352	1354	rBV2	640	678	0.15%	0.030%
30	10.826	1357	1359	1361	rBV2	958	862	0.19%	0.038%
31	10.973	1375	1384	1394	rBV	150056	305622	66.49%	13.467%
32	11.120	1404	1409	1410	rBV4	1977	2608	0.57%	0.115%
33	11.137	1410	1412	1415	rVB3	1120	956	0.21%	0.042%
34	11.337	1444	1446	1447	rVB	1188	669	0.15%	0.029%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
 Data File : BG022073.D
 Acq On : 26 May 2016 9:40
 Operator : UM/SJ
 Sample : H3201-10 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZG9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

35	11.402	1455	1457	1459	rBV	689	673	0.15%	0.030%
36	11.649	1496	1499	1500	rBV3	835	748	0.16%	0.033%
37	11.672	1500	1503	1505	rVB2	555	593	0.13%	0.026%
38	11.801	1522	1525	1527	rBV2	529	621	0.14%	0.027%
39	11.954	1550	1551	1553	rBV	745	628	0.14%	0.028%
40	12.260	1600	1603	1606	rVB	435	588	0.13%	0.026%
41	12.824	1698	1699	1702	rBV	651	763	0.17%	0.034%
42	13.188	1759	1761	1765	rBV2	633	644	0.14%	0.028%
43	13.411	1794	1799	1805	rBV2	852	1662	0.36%	0.073%
44	14.175	1923	1929	1933	rBV	23762	37274	8.11%	1.642%
45	14.222	1933	1937	1943	rVV	11147	17016	3.70%	0.750%
46	14.263	1943	1944	1948	rVB2	1130	807	0.18%	0.036%
47	14.310	1948	1952	1954	rBV2	585	786	0.17%	0.035%
48	14.475	1971	1980	1989	rBV	32501	55862	12.15%	2.462%
49	14.639	2006	2008	2013	rVB4	1663	2248	0.49%	0.099%
50	14.780	2024	2032	2047	rBV	254581	447529	97.36%	19.720%
51	15.033	2071	2075	2079	rVB	659	989	0.22%	0.044%
52	15.074	2079	2082	2085	rBV	796	918	0.20%	0.040%
53	15.127	2089	2091	2095	rVV2	673	750	0.16%	0.033%
54	15.244	2106	2111	2112	rBV2	580	789	0.17%	0.035%
55	15.421	2138	2141	2144	rBV2	594	717	0.16%	0.032%
56	15.456	2144	2147	2149	rBV2	631	572	0.12%	0.025%
57	15.591	2167	2170	2174	rBV2	3491	4919	1.07%	0.217%
58	15.767	2194	2200	2209	rBV2	39603	66782	14.53%	2.943%
59	15.832	2209	2211	2214	rVB3	504	569	0.12%	0.025%
60	15.897	2218	2222	2224	rBV2	2068	2043	0.44%	0.090%
61	15.996	2234	2239	2243	rVB3	1257	2351	0.51%	0.104%
62	16.067	2248	2251	2253	rVB	887	722	0.16%	0.032%
63	16.202	2270	2274	2277	rVB2	573	778	0.17%	0.034%
64	16.261	2281	2284	2286	rVB	711	608	0.13%	0.027%
65	16.455	2310	2317	2326	rVV5	3814	8076	1.76%	0.356%
66	16.519	2326	2328	2330	rVB	641	570	0.12%	0.025%
67	16.637	2347	2348	2352	rVB2	589	596	0.13%	0.026%
68	16.678	2352	2355	2357	rVB2	672	809	0.18%	0.036%
69	16.696	2357	2358	2360	rBV	993	725	0.16%	0.032%
70	16.743	2363	2366	2368	rBV2	552	590	0.13%	0.026%
71	16.772	2368	2371	2374	rVV2	555	707	0.15%	0.031%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
 Data File : BG022073.D
 Acq On : 26 May 2016 9:40
 Operator : UM/SJ
 Sample : H3201-10 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZG9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

72	16.807	2374	2377	2380	rVB3	686	848	0.18%	0.037%
73	16.913	2393	2395	2398	rVB2	1074	807	0.18%	0.036%
74	17.013	2409	2412	2413	rBV2	1170	963	0.21%	0.042%
75	17.072	2419	2422	2426	rVB2	1279	1400	0.30%	0.062%
76	17.113	2426	2429	2430	rBV2	580	697	0.15%	0.031%
77	17.201	2442	2444	2446	rBV2	842	747	0.16%	0.033%
78	17.248	2446	2452	2456	rVV3	2631	4047	0.88%	0.178%
79	17.289	2456	2459	2462	rVV3	1725	2639	0.57%	0.116%
80	17.318	2462	2464	2465	rVV2	1612	1076	0.23%	0.047%
81	17.336	2465	2467	2470	rVB2	842	866	0.19%	0.038%
82	17.524	2491	2499	2509	rBV	263598	459682	100.00%	20.256%
83	17.624	2509	2516	2525	rVB2	38695	69161	15.05%	3.048%
84	17.753	2536	2538	2540	rBV2	1185	938	0.20%	0.041%
85	17.783	2540	2543	2544	rBV2	1610	1336	0.29%	0.059%
86	17.877	2558	2559	2561	rVB2	1082	736	0.16%	0.032%
87	17.912	2563	2565	2568	rVB3	1091	1029	0.22%	0.045%
88	17.982	2575	2577	2582	rVB4	1730	1925	0.42%	0.085%
89	18.153	2603	2606	2607	rBV	1206	966	0.21%	0.043%
90	18.335	2634	2637	2639	rBV4	1481	1576	0.34%	0.069%
91	18.511	2664	2667	2668	rBV3	1556	1109	0.24%	0.049%
92	18.564	2674	2676	2678	rBV3	1970	1635	0.36%	0.072%
93	18.582	2678	2679	2681	rVB2	1703	966	0.21%	0.043%
94	18.781	2711	2713	2715	rBV3	1967	1673	0.36%	0.074%
95	19.898	2898	2903	2911	rBV2	49895	89171	19.40%	3.929%
96	21.801	3222	3227	3235	rVB	209013	386890	84.16%	17.048%


Sum of corrected areas: 2269389

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
Data File : BG022073.D
Acq On : 26 May 2016 9:40
Operator : UM/SJ
Sample : H3201-10 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
BCZG9

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

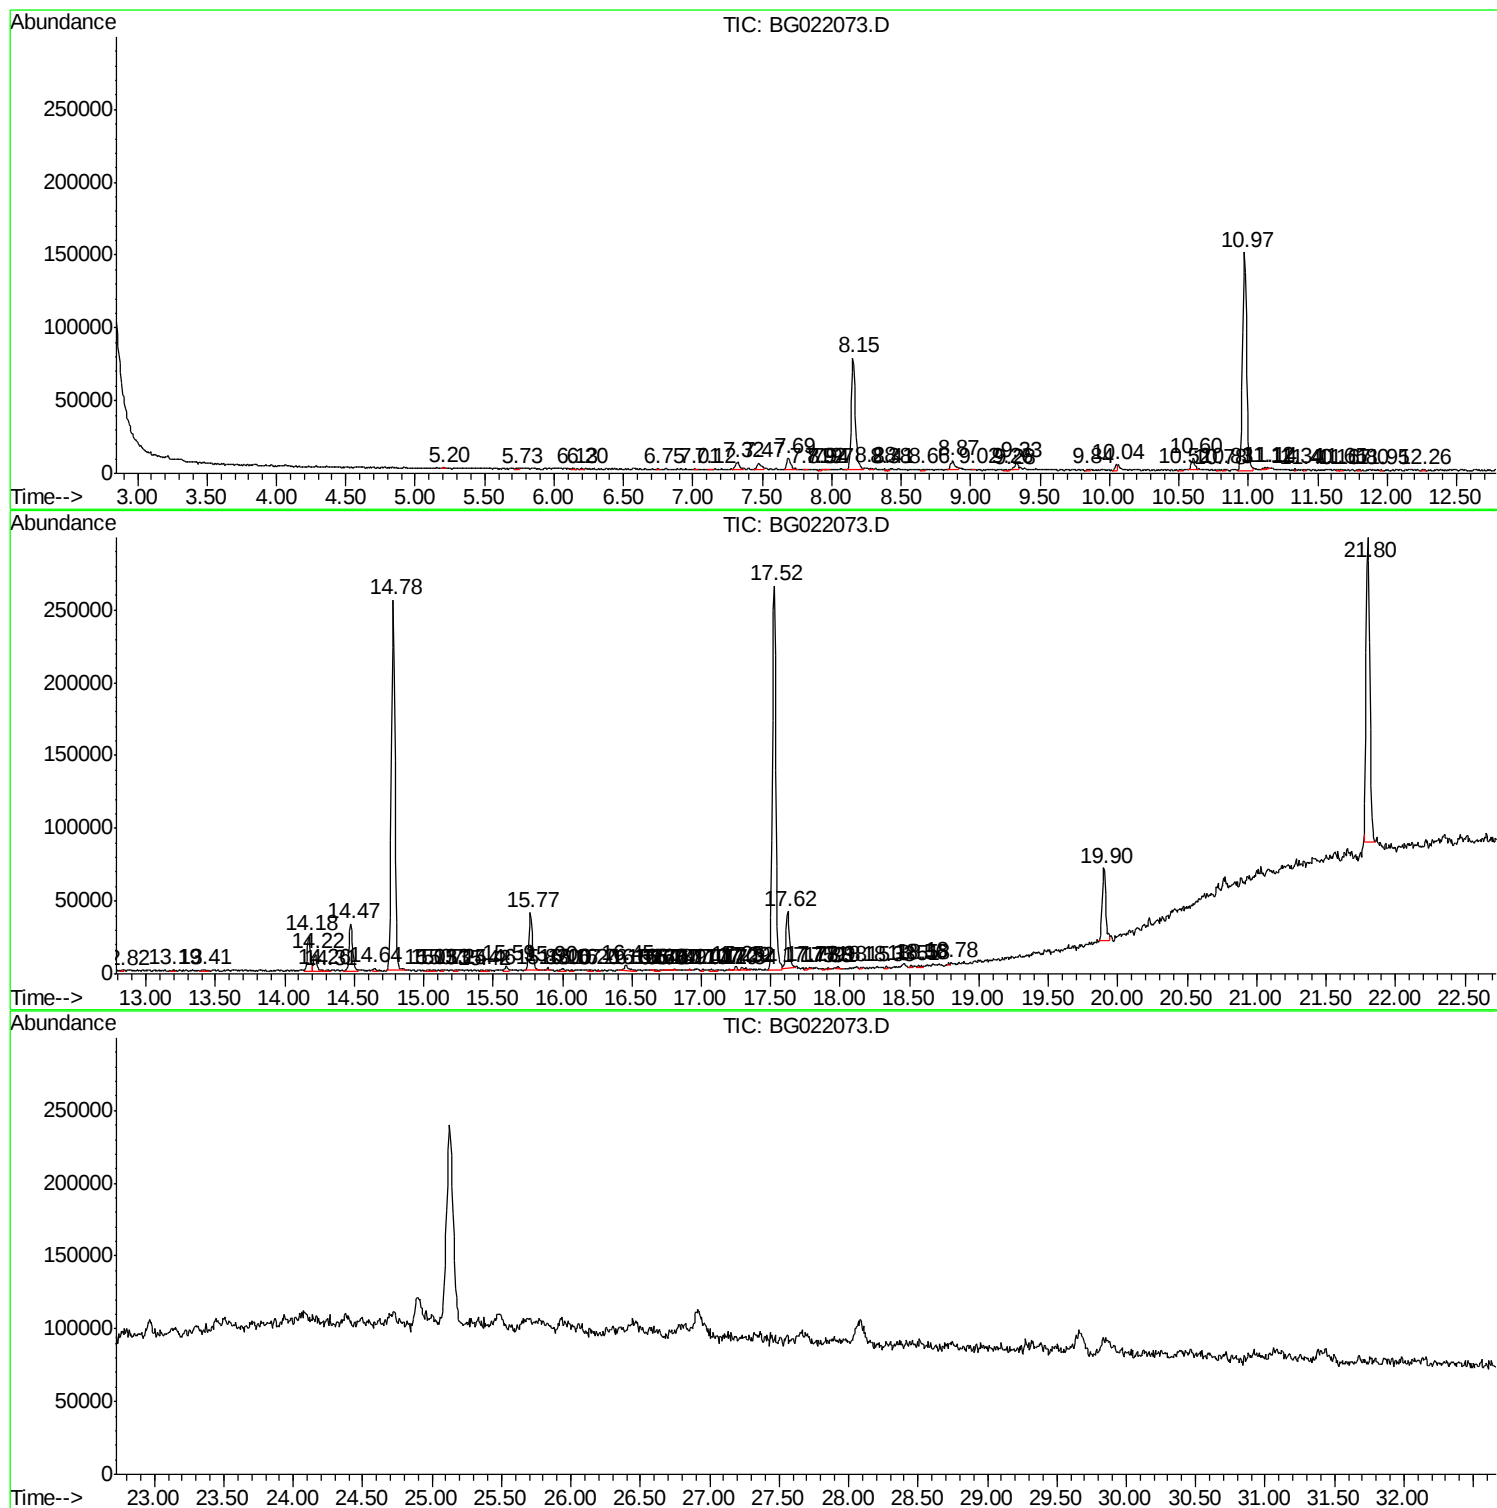

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052616\
Data File : BG022073.D
Acq On : 26 May 2016 9:40
Operator : UM/SJ
Sample : H3201-10 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCZG9

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052616\
Data File : BG022073.D
Acq On : 26 May 2016 9:40
Operator : UM/SJ
Sample : H3201-10 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCZG9

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc