

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
 Data File : BG022098.D
 Acq On : 27 May 2016 2:32
 Operator : UM/SJ
 Sample : H3205-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.155	52	54	60	rVB4	1204	1377	0.29%	0.070%
2	3.396	94	95	98	rVB3	1915	1272	0.26%	0.064%
3	3.420	98	99	104	rBV4	1093	1447	0.30%	0.073%
4	3.484	109	110	114	rBV2	1009	998	0.21%	0.051%
5	3.514	114	115	120	rVB2	1222	928	0.19%	0.047%
6	3.572	123	125	127	rVB2	1110	836	0.17%	0.042%
7	3.596	127	129	130	rBV	1040	808	0.17%	0.041%
8	3.684	142	144	146	rBV3	939	864	0.18%	0.044%
9	4.295	246	248	251	rVB3	987	790	0.16%	0.040%
10	4.413	265	268	269	rBV2	812	785	0.16%	0.040%
11	4.759	323	327	331	rBV4	553	906	0.19%	0.046%
12	5.041	374	375	379	rBV3	728	1010	0.21%	0.051%
13	5.153	391	394	396	rBV3	619	829	0.17%	0.042%
14	5.235	406	408	411	rVB2	817	996	0.21%	0.050%
15	5.288	415	417	420	rVV3	696	840	0.17%	0.043%
16	5.370	427	431	433	rVB4	887	1183	0.25%	0.060%
17	5.441	439	443	445	rVV2	767	1118	0.23%	0.057%
18	5.940	524	528	529	rVB3	721	762	0.16%	0.039%
19	6.328	591	594	596	rVV3	845	991	0.21%	0.050%
20	6.434	611	612	617	rBV2	761	869	0.18%	0.044%
21	6.545	628	631	634	rBV2	938	1176	0.24%	0.060%
22	6.722	659	661	664	rBV3	850	891	0.19%	0.045%
23	6.892	687	690	692	rVB2	1023	800	0.17%	0.041%
24	6.933	694	697	700	rBV2	770	846	0.18%	0.043%
25	7.039	713	715	718	rVB2	721	774	0.16%	0.039%
26	7.086	718	723	724	rBV2	1169	1309	0.27%	0.066%
27	7.380	770	773	774	rBV3	920	864	0.18%	0.044%
28	7.632	813	816	818	rVB	644	760	0.16%	0.038%
29	7.703	824	828	829	rBV3	623	763	0.16%	0.039%
30	7.903	858	862	867	rVB	871	1598	0.33%	0.081%
31	8.050	885	887	890	rBV2	881	845	0.18%	0.043%
32	8.161	899	906	923	rBV	89676	187038	38.85%	9.470%
33	8.273	923	925	928	rVV	1130	1387	0.29%	0.070%
34	8.302	928	930	934	rVV2	1023	1086	0.23%	0.055%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
 Data File : BG022098.D
 Acq On : 27 May 2016 2:32
 Operator : UM/SJ
 Sample : H3205-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

35	8.420	948	950	954	rVB2	868	867	0.18%	0.044%
36	8.455	954	956	959	rBV2	890	1000	0.21%	0.051%
37	8.725	998	1002	1004	rVB2	670	875	0.18%	0.044%
38	8.778	1007	1011	1013	rBV2	814	946	0.20%	0.048%
39	10.082	1231	1233	1238	rVB	905	1052	0.22%	0.053%
40	10.118	1238	1239	1244	rBV	522	926	0.19%	0.047%
41	10.981	1378	1386	1399	rBV	171558	343776	71.40%	17.405%
42	11.122	1408	1410	1412	rBV2	802	937	0.19%	0.047%
43	11.493	1470	1473	1474	rBV2	810	850	0.18%	0.043%
44	11.910	1538	1544	1546	rVB2	654	980	0.20%	0.050%
45	13.226	1765	1768	1770	rBV2	914	958	0.20%	0.049%
46	13.661	1838	1842	1844	rVB2	702	960	0.20%	0.049%
47	13.761	1854	1859	1860	rBV	1045	1109	0.23%	0.056%
48	13.808	1865	1867	1869	rBV	1134	766	0.16%	0.039%
49	13.978	1893	1896	1897	rVB2	1346	1044	0.22%	0.053%
50	13.996	1897	1899	1900	rBV	1014	768	0.16%	0.039%
51	14.037	1902	1906	1907	rVV2	940	1078	0.22%	0.055%
52	14.048	1907	1908	1910	rVV2	1203	828	0.17%	0.042%
53	14.072	1910	1912	1915	rVB2	1221	1107	0.23%	0.056%
54	14.113	1915	1919	1920	rVB3	1513	1393	0.29%	0.071%
55	14.137	1920	1923	1924	rBV2	1115	1023	0.21%	0.052%
56	14.225	1934	1938	1939	rBV3	1213	1153	0.24%	0.058%
57	14.236	1939	1940	1943	rVB2	979	763	0.16%	0.039%
58	14.260	1943	1944	1946	rBV2	1199	940	0.20%	0.048%
59	14.501	1984	1985	1989	rVB2	1523	1024	0.21%	0.052%
60	14.589	1996	2000	2002	rVB4	1063	1525	0.32%	0.077%
61	14.648	2007	2010	2012	rVB4	742	780	0.16%	0.039%
62	14.730	2019	2024	2025	rVB2	933	1051	0.22%	0.053%
63	14.789	2025	2034	2041	rBV2	270366	481446	100.00%	24.375%
64	14.994	2067	2069	2070	rBV2	1243	1039	0.22%	0.053%
65	15.024	2070	2074	2075	rVB4	1050	1158	0.24%	0.059%
66	15.065	2078	2081	2083	rBV2	1993	2179	0.45%	0.110%
67	15.141	2093	2094	2096	rBV2	1120	809	0.17%	0.041%
68	15.194	2100	2103	2106	rVB5	1769	2246	0.47%	0.114%
69	15.224	2106	2108	2109	rBV2	1532	1327	0.28%	0.067%
70	15.294	2118	2120	2121	rBV2	1185	794	0.16%	0.040%
71	15.306	2121	2122	2124	rVV	1570	1035	0.21%	0.052%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
 Data File : BG022098.D
 Acq On : 27 May 2016 2:32
 Operator : UM/SJ
 Sample : H3205-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

72	15.341	2124	2128	2129	rVV4	1572	1495	0.31%	0.076%
73	15.429	2140	2143	2144	rVB3	1151	1096	0.23%	0.055%
74	15.453	2144	2147	2149	rBV3	1729	2676	0.56%	0.135%
75	15.494	2152	2154	2156	rVB3	1362	1083	0.22%	0.055%
76	15.517	2156	2158	2161	rBV4	1149	1727	0.36%	0.087%
77	15.629	2175	2177	2178	rBV2	1577	1184	0.25%	0.060%
78	15.641	2178	2179	2182	rVV3	2333	1737	0.36%	0.088%
79	15.670	2182	2184	2186	rBV3	1096	1135	0.24%	0.057%
80	15.705	2188	2190	2192	rBV3	1856	1792	0.37%	0.091%
81	15.764	2197	2200	2201	rBV3	1058	1040	0.22%	0.053%
82	15.823	2207	2210	2213	rBV5	3264	3306	0.69%	0.167%
83	15.852	2213	2215	2216	rVV2	1262	892	0.19%	0.045%
84	15.946	2229	2231	2232	rBV2	1564	1034	0.21%	0.052%
85	15.964	2232	2234	2235	rVB2	1871	1018	0.21%	0.052%
86	16.034	2244	2246	2248	rBV3	1308	1189	0.25%	0.060%
87	16.117	2258	2260	2263	rBV4	1596	2145	0.45%	0.109%
88	16.193	2272	2273	2275	rBV2	2144	1481	0.31%	0.075%
89	16.211	2275	2276	2277	rVV	2560	1428	0.30%	0.072%
90	16.246	2280	2282	2283	rVB2	1426	849	0.18%	0.043%
91	16.293	2289	2290	2294	rBV3	3096	3895	0.81%	0.197%
92	16.451	2313	2317	2319	rBV5	2630	4588	0.95%	0.232%
93	16.534	2329	2331	2336	rBV6	2420	3227	0.67%	0.163%
94	16.651	2348	2351	2352	rBV3	3413	3712	0.77%	0.188%
95	16.945	2400	2401	2403	rBV2	4001	3586	0.74%	0.182%
96	17.127	2430	2432	2435	rBV4	5865	6812	1.41%	0.345%
97	17.215	2445	2447	2449	rBV3	4184	3462	0.72%	0.175%
98	17.533	2495	2501	2510	rBV2	256051	444812	92.39%	22.521%
99	17.832	2550	2552	2553	rBV2	6552	5378	1.12%	0.272%
100	21.816	3226	3230	3236	rVB	226560	385103	79.99%	19.498%


Sum of corrected areas: 1975140

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052616\
Data File : BG022098.D
Acq On : 27 May 2016 2:32
Operator : UM/SJ
Sample : H3205-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

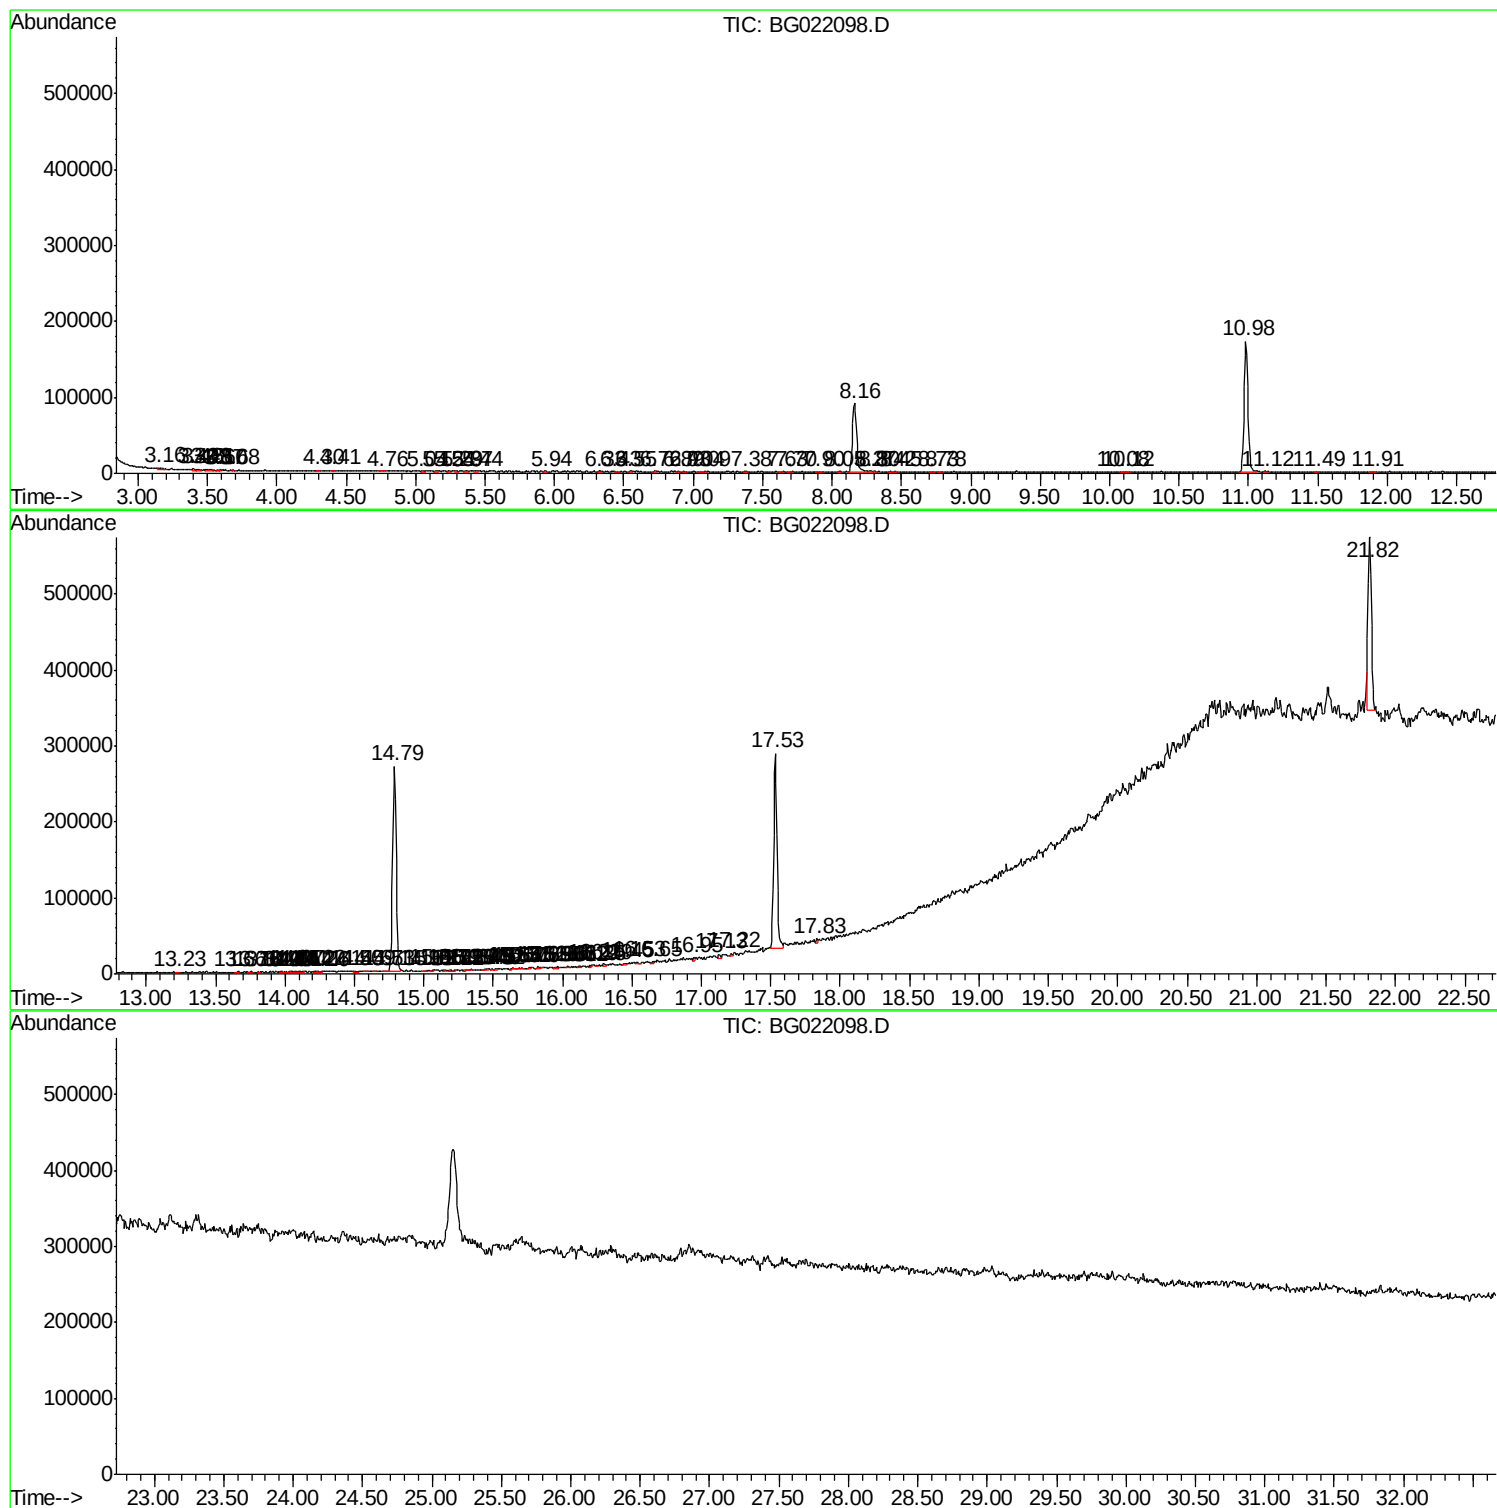

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052616\
Data File : BG022098.D
Acq On : 27 May 2016 2:32
Operator : UM/SJ
Sample : H3205-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052616\
Data File : BG022098.D
Acq On : 27 May 2016 2:32
Operator : UM/SJ
Sample : H3205-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc