
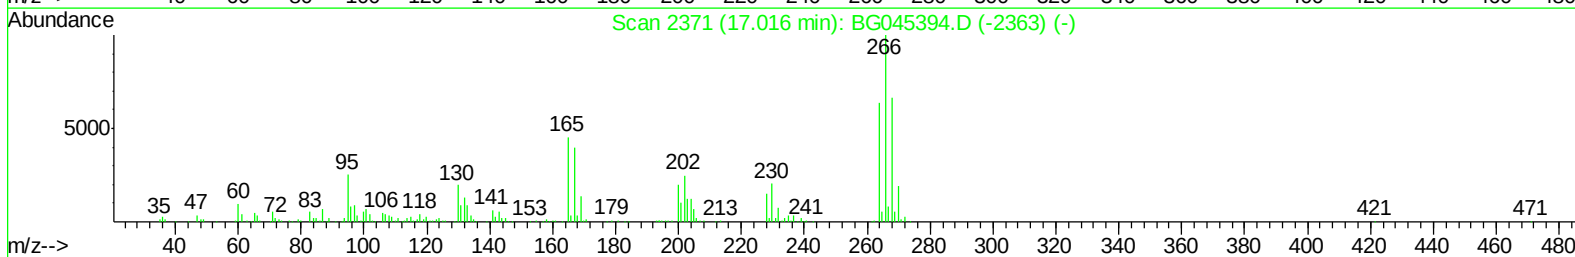
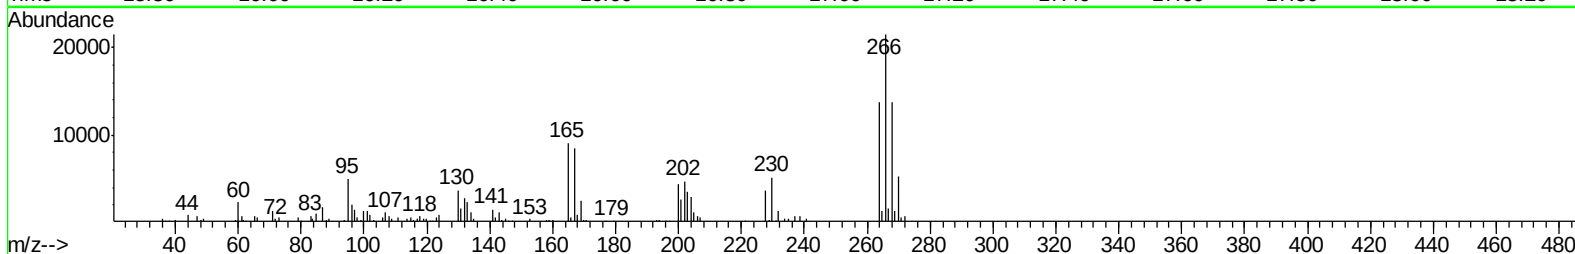


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG052620\
 Data File : BG045454.D
 Acq On : 26 May 2020 12:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 03:21:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 26 14:16:30 2020
 Response via : Initial Calibration

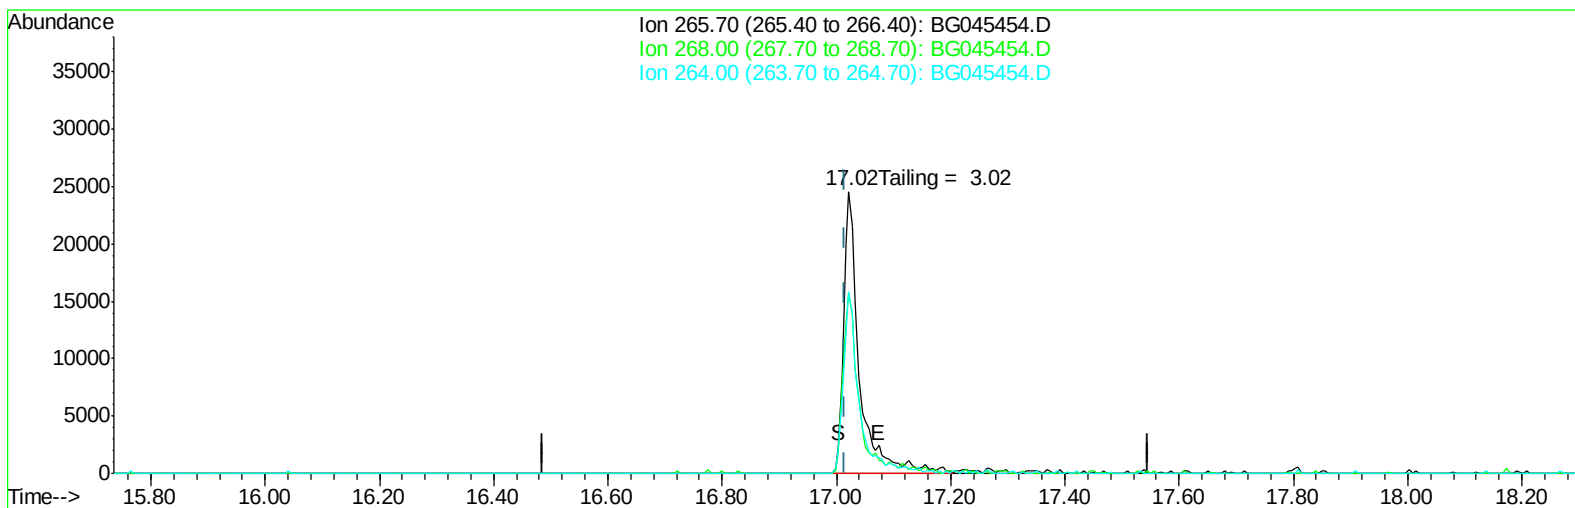

TIC: BG045454.D

(70) Pentachlorophenol (C)




17.021min (+0.005) 0.00ng

response 45544

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	64.18
264.00	63.70	64.60
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG052620\
 Data File : BG045454.D
 Acq On : 26 May 2020 12:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 03:21:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 26 14:16:30 2020
 Response via : Initial Calibration

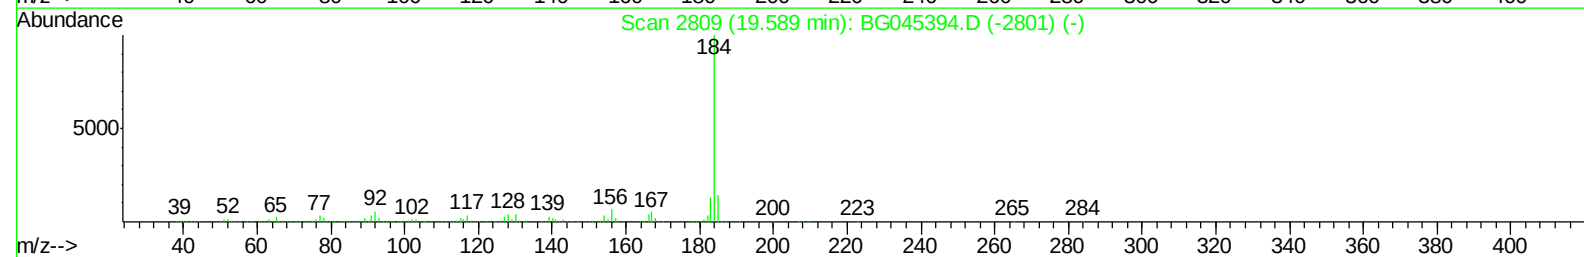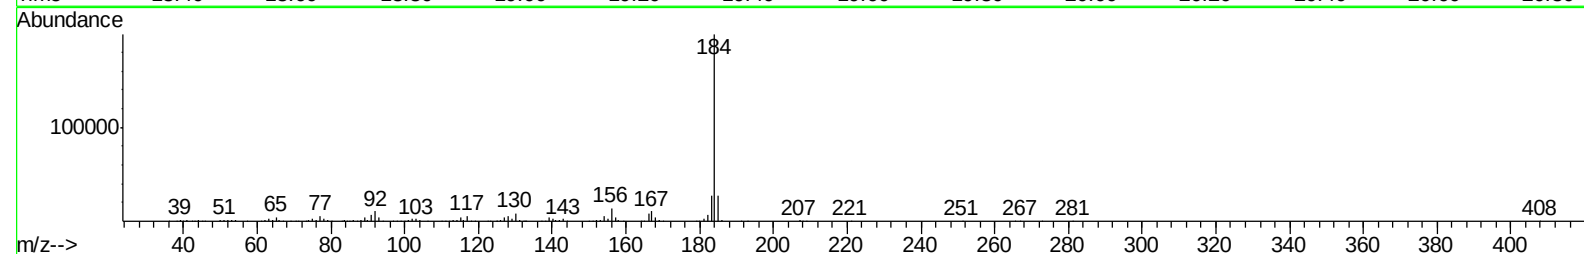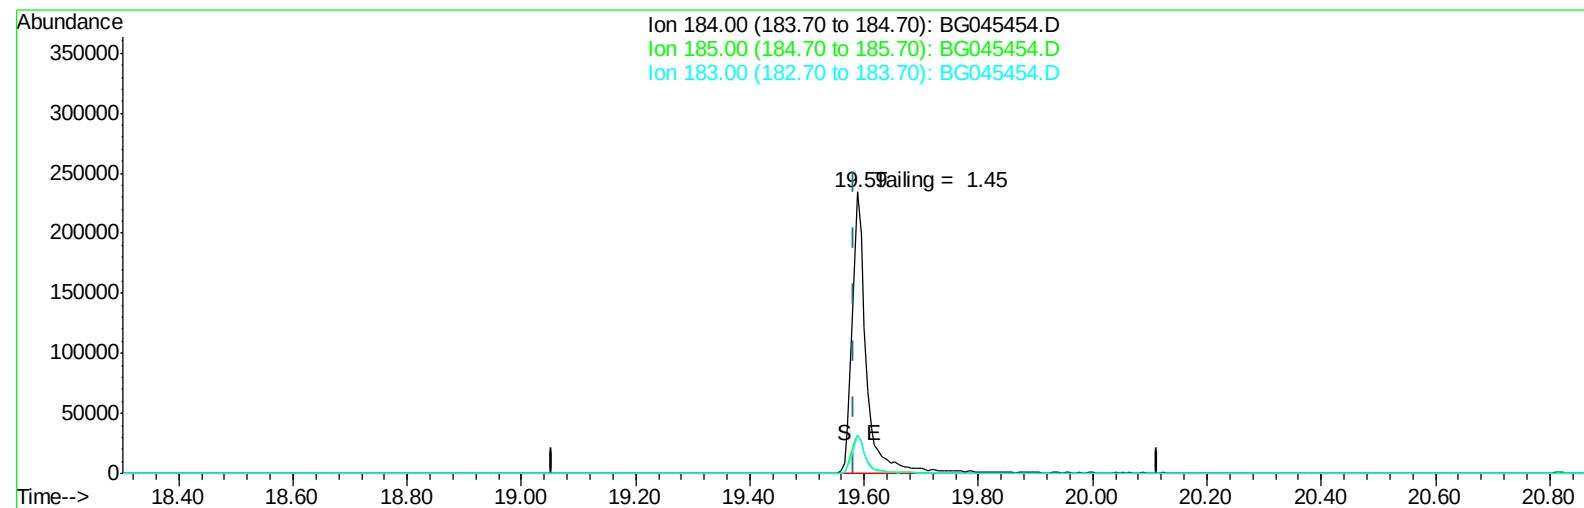

TIC: BG045454.D

(77) Benzidine

19.589min (+0.005) 0.00ng

response 410751

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	13.66
183.00	12.80	13.85
0.00	0.00	0.00