
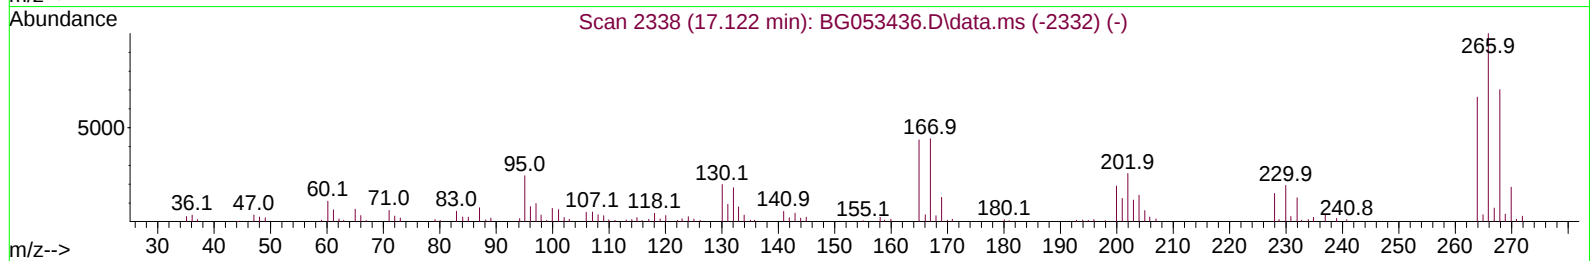
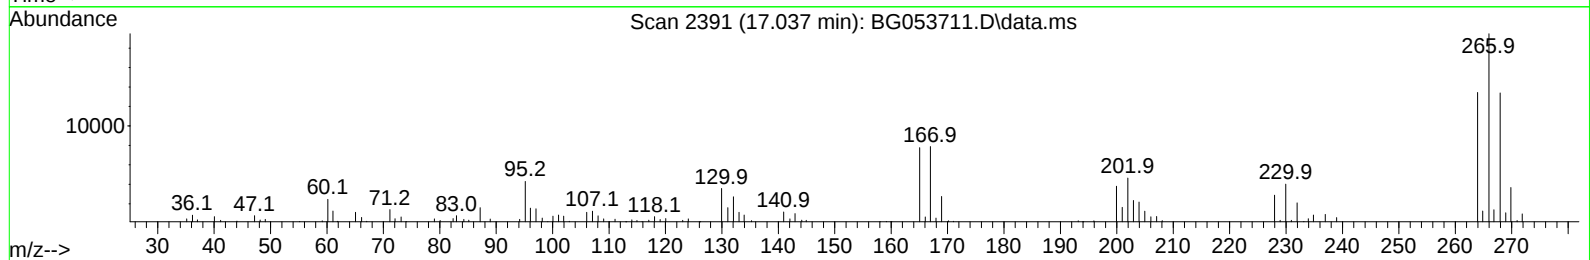


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052622\
Data File : BG053711.D
Acq On : 26 May 2022 10:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 16:05:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

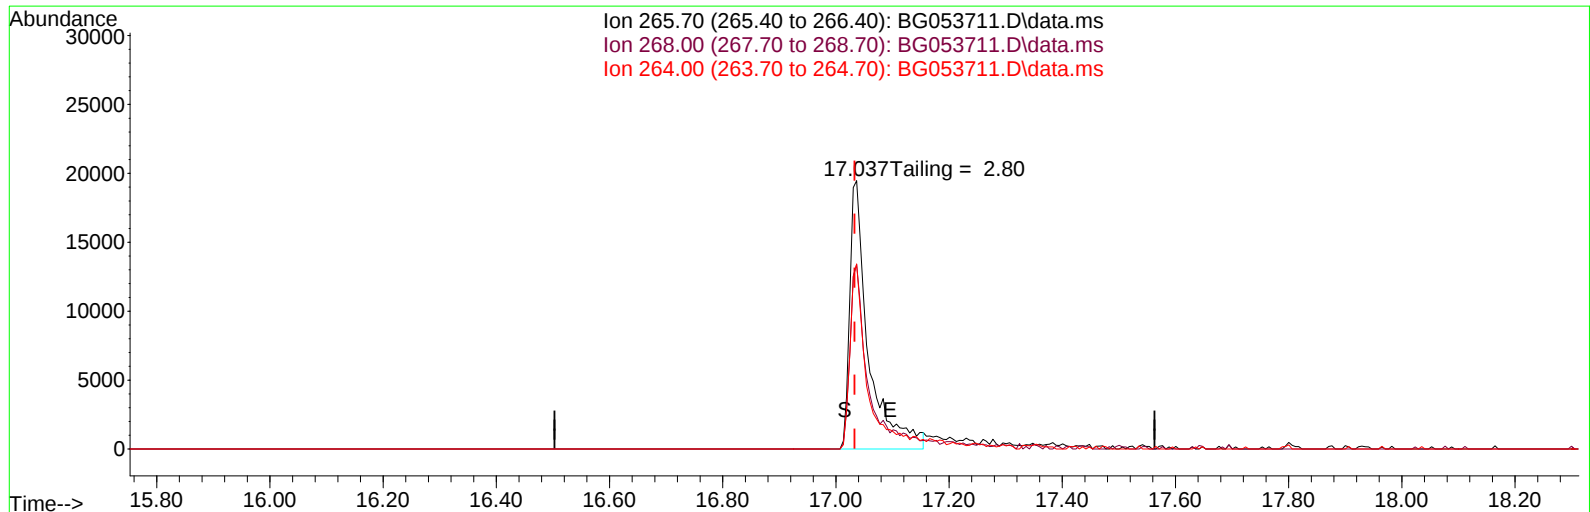

TIC: BG053711.D\data.ms

(70) Pentachlorophenol (C)




17.037min (+ 0.004) 98555.56 ng

response 46847

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	68.77
264.00	66.20	69.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052622\
Data File : BG053711.D
Acq On : 26 May 2022 10:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 16:05:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

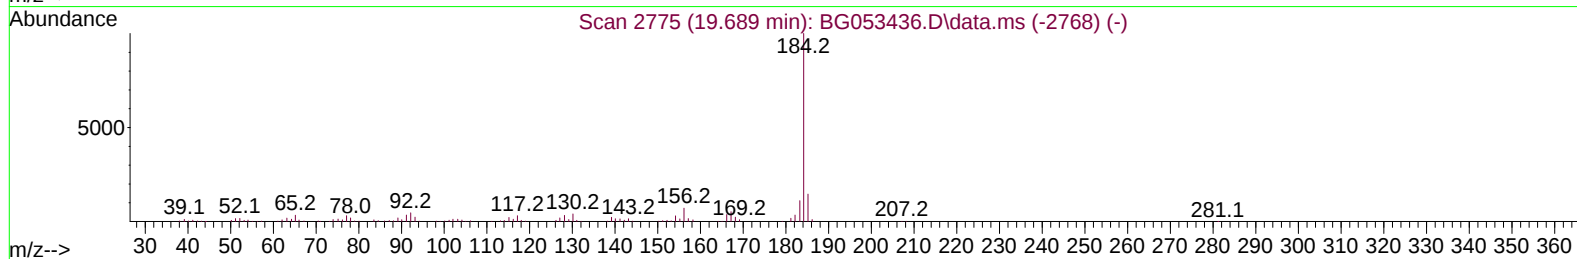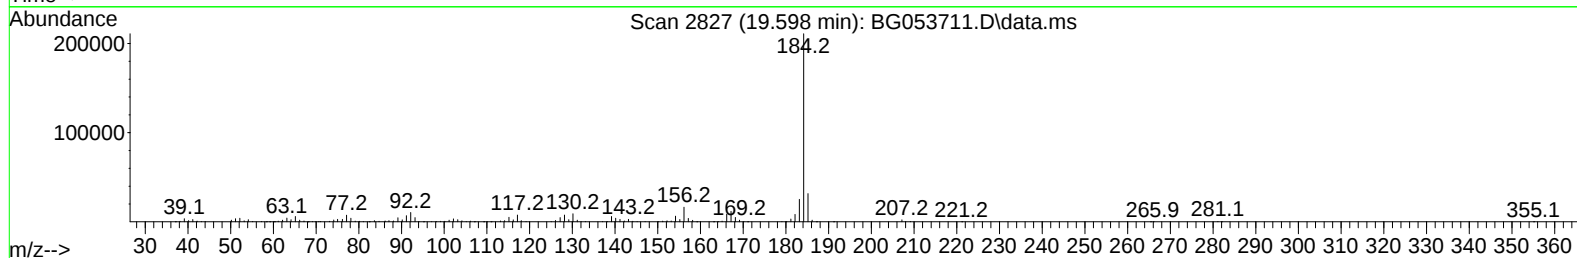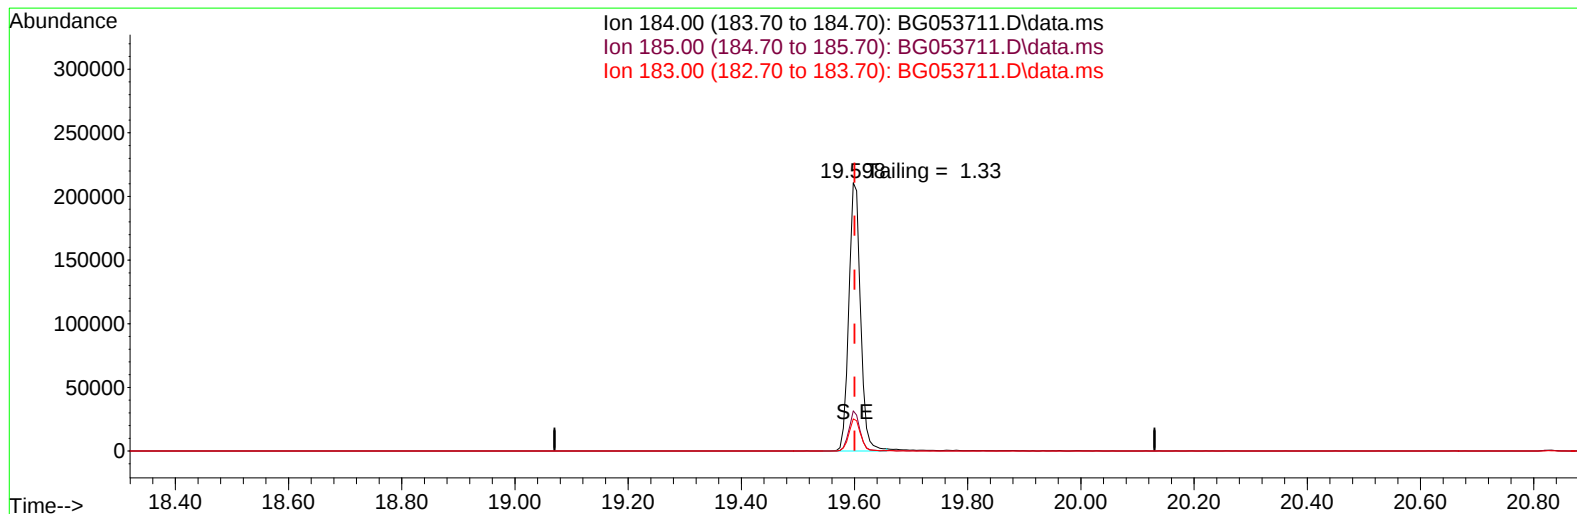

TIC: BG053711.D\data.ms

(77) Benzidine**19.598min (-0.002) 204321.53 ng****response 303868**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.01
183.00	11.10	11.98
0.00	0.00	0.00