

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052622\
 Data File : BG053713.D
 Acq On : 26 May 2022 12:23
 Operator : CG/JU
 Sample : PB145033BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB145033BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.088	13	17	23	rVB2	17278	25797	1.13%	0.298%
2	5.550	430	436	449	rBV	447978	739537	32.28%	8.543%
3	7.159	703	710	722	rBV	462240	809292	35.32%	9.349%
4	7.982	843	850	858	rBV	84077	143547	6.26%	1.658%
5	9.145	1041	1048	1059	rBV	291051	529244	23.10%	6.114%
6	10.795	1321	1329	1342	rBV	109616	204569	8.93%	2.363%
7	13.245	1739	1746	1754	rBV	792597	1247768	54.46%	14.414%
8	14.620	1974	1980	1987	rBV	192245	304699	13.30%	3.520%
9	16.112	2228	2234	2252	rBV	611504	1000391	43.66%	11.556%
10	17.369	2442	2448	2461	rVB	286154	415072	18.12%	4.795%
11	19.977	2886	2892	2898	rBV	1817487	2291297	100.00%	26.468%
12	21.634	3168	3174	3182	rVB	292929	476512	20.80%	5.504%
13	24.835	3709	3719	3729	rVB2	165004	469129	20.47%	5.419%




Sum of corrected areas: 8656854

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052622\
Data File : BG053713.D
Acq On : 26 May 2022 12:23
Operator : CG/JU
Sample : PB145033BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145033BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

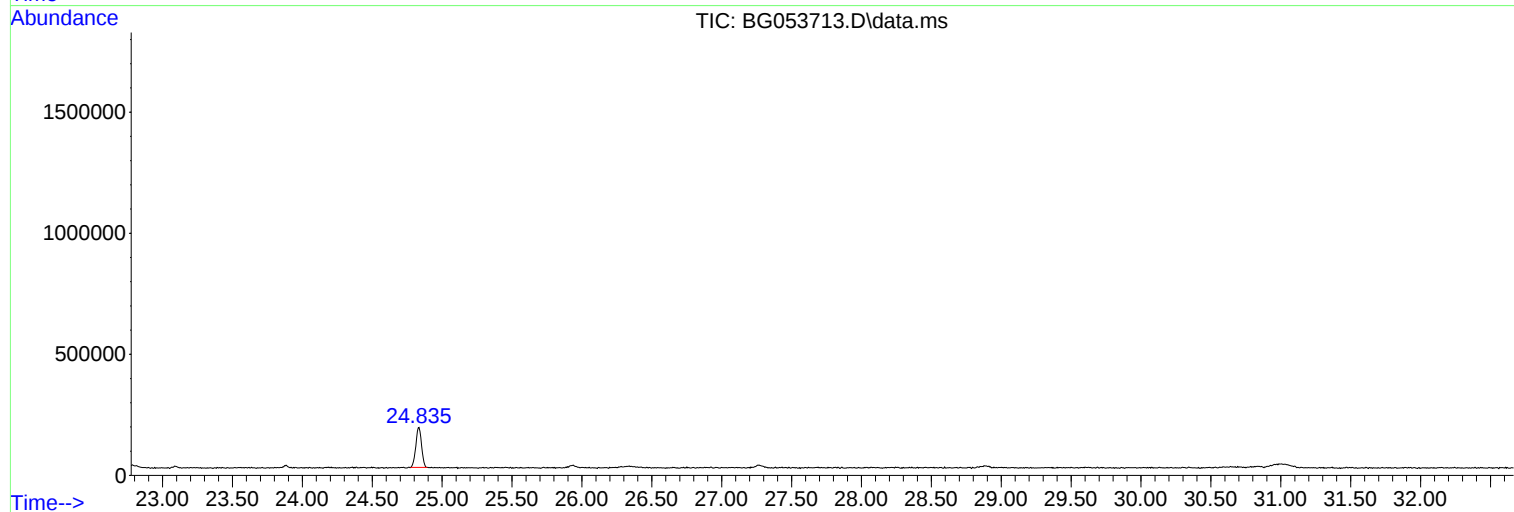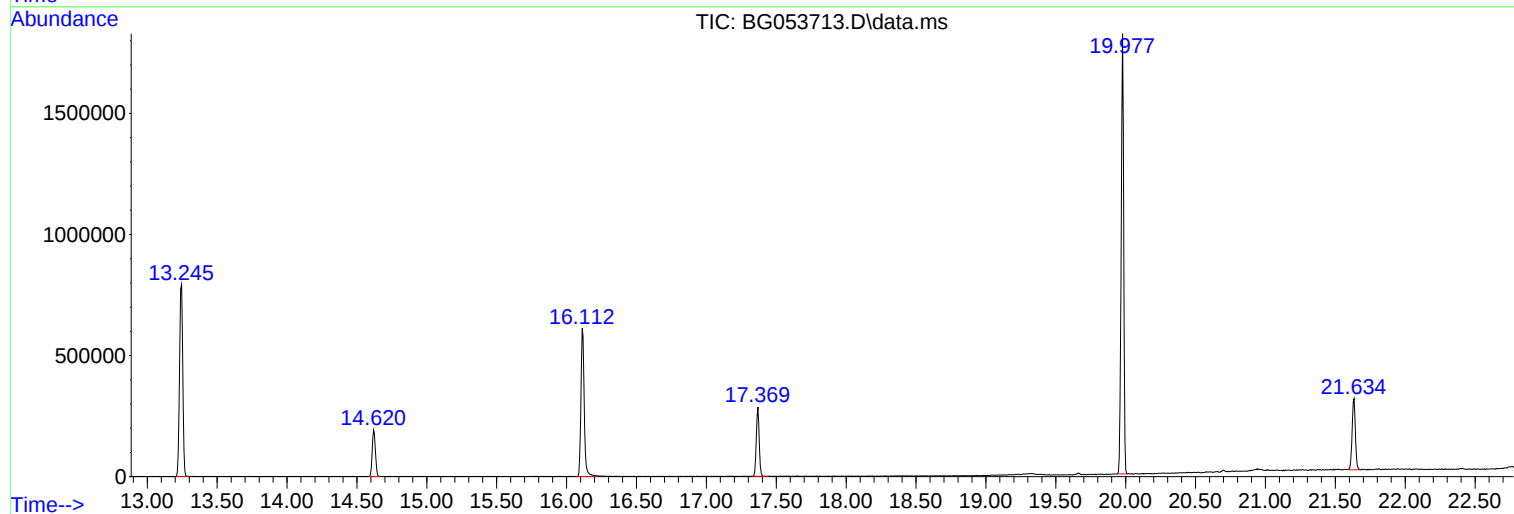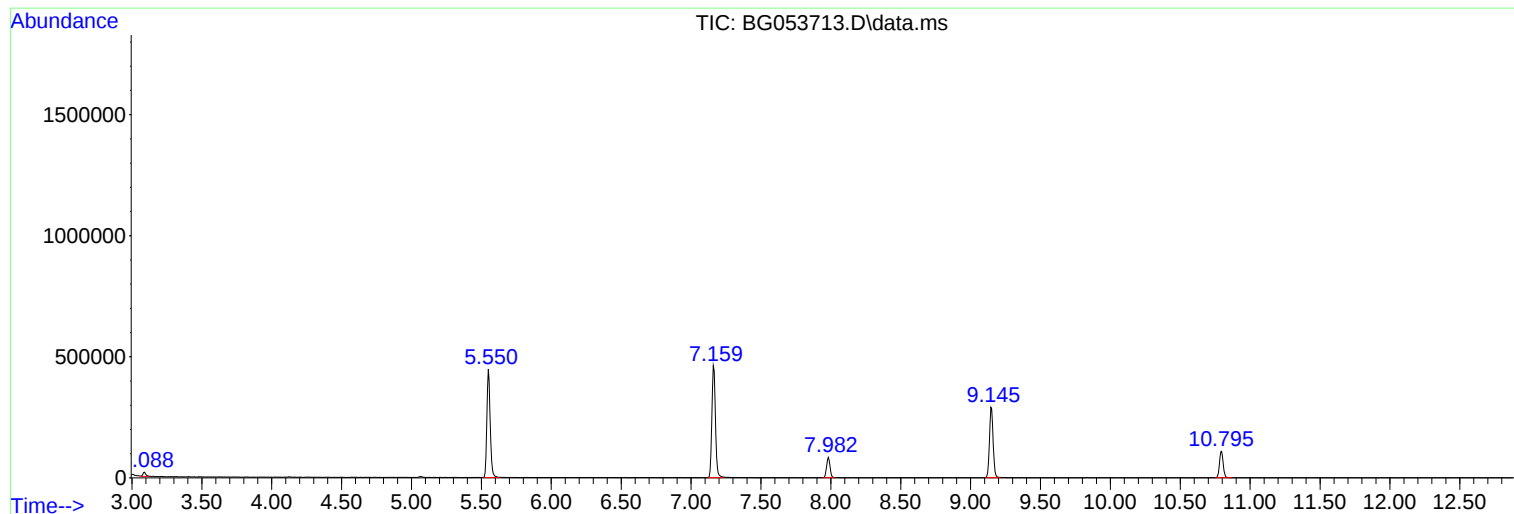

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052622\
Data File : BG053713.D
Acq On : 26 May 2022 12:23
Operator : CG/JU
Sample : PB145033BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145033BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.088	3.59 ng	25797	1,4-Dichlorobenzene-d4	7.981

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
2			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	36
3			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	25
4			1-(2-Methoxyethoxy)-2-methyl-2-p...	162	C8H18O3	1000364-24-4	9
5			Acetic acid, 3-[1,3]dioxolan-2-y...	174	C8H14O4	1000186-02-3	9

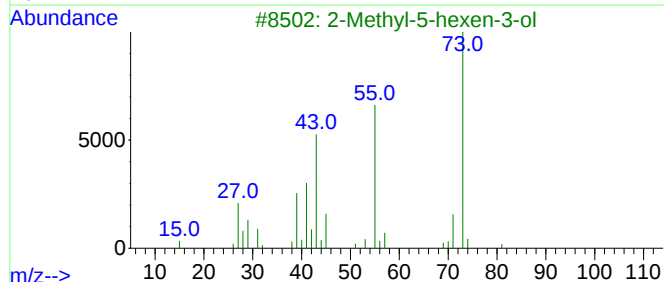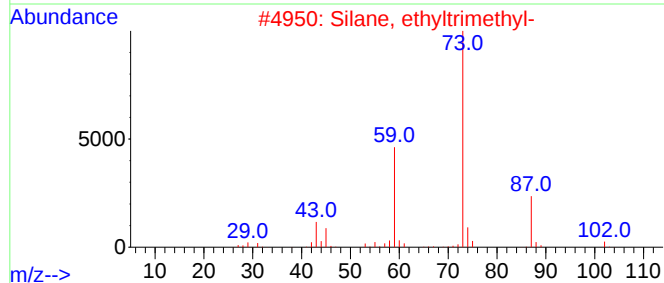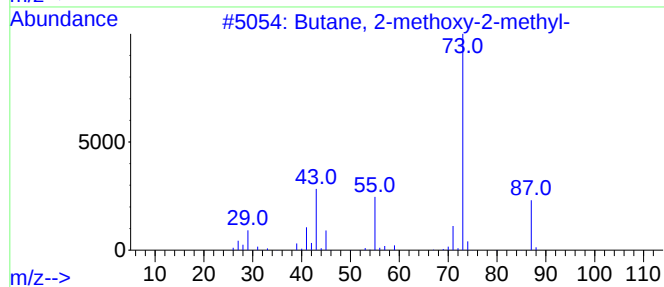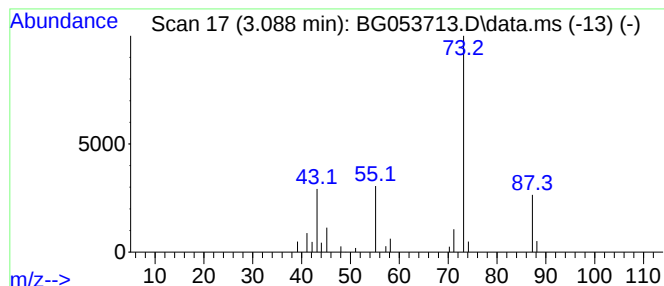

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052622\
Data File : BG053713.D
Acq On : 26 May 2022 12:23
Operator : CG/JU
Sample : PB145033BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145033BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.088	3.6	ng	25797	1	7.981	143547	20.0